


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082720\
 Data File : BN011673.D
 Acq On : 27 Aug 2020 21:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 27 14:34:48 2020

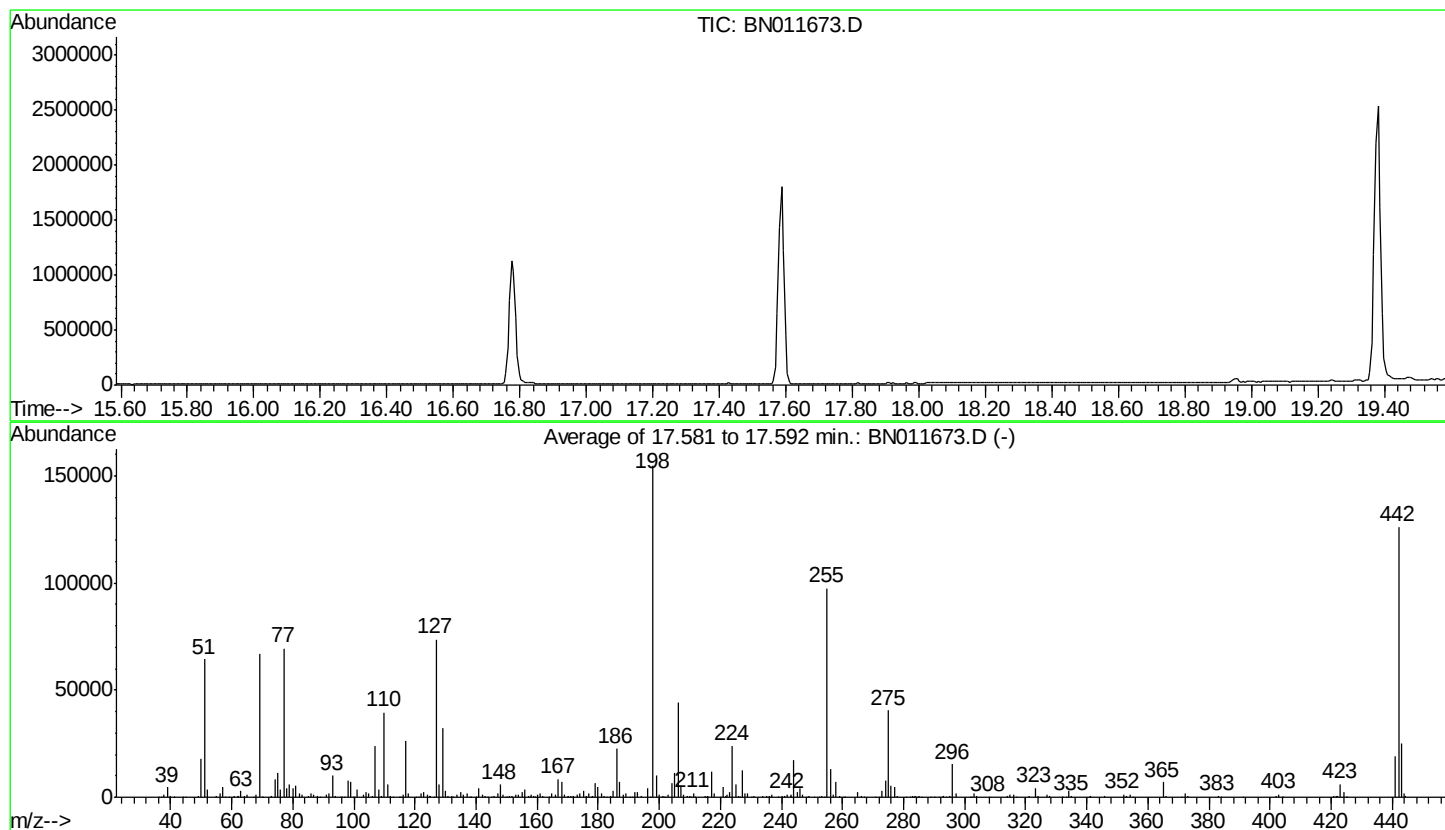

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	64349	PASS
68	69	0.00	2	2.0	1358	PASS
69	198	0.00	100	43.4	67229	PASS
70	69	0.00	2	0.4	299	PASS
127	198	10	80	47.6	73629	PASS
197	198	0.00	2	0.2	242	PASS
198	198	100	100	100.0	154784	PASS
199	198	5	9	6.6	10153	PASS
275	198	10	60	26.1	40426	PASS
365	198	1	100	4.5	6914	PASS
441	198	0.01	100	12.5	19290	PASS
442	198	50	100	81.5	126194	PASS
443	442	15	24	19.8	25037	PASS