

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\
 Data File : BN007452.D
 Acq On : 28 Aug 2019 03:18
 Operator : HP/JU
 Sample : PB122307BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 28 03:57:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 28 02:09:57 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	4632	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	19894	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	11263	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.90	188	1943238	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.03
20) Perylene-d12	22.99	264	1854670	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	12507	0.40	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.05	166	3360	0.069	ng/ul#	Ovalue 14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\
Data File : BN007452.D
Acq On : 28 Aug 2019 03:18
Operator : HP/JU
Sample : PB122307BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 28 03:57:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 28 02:09:57 2019
Response via : Initial Calibration

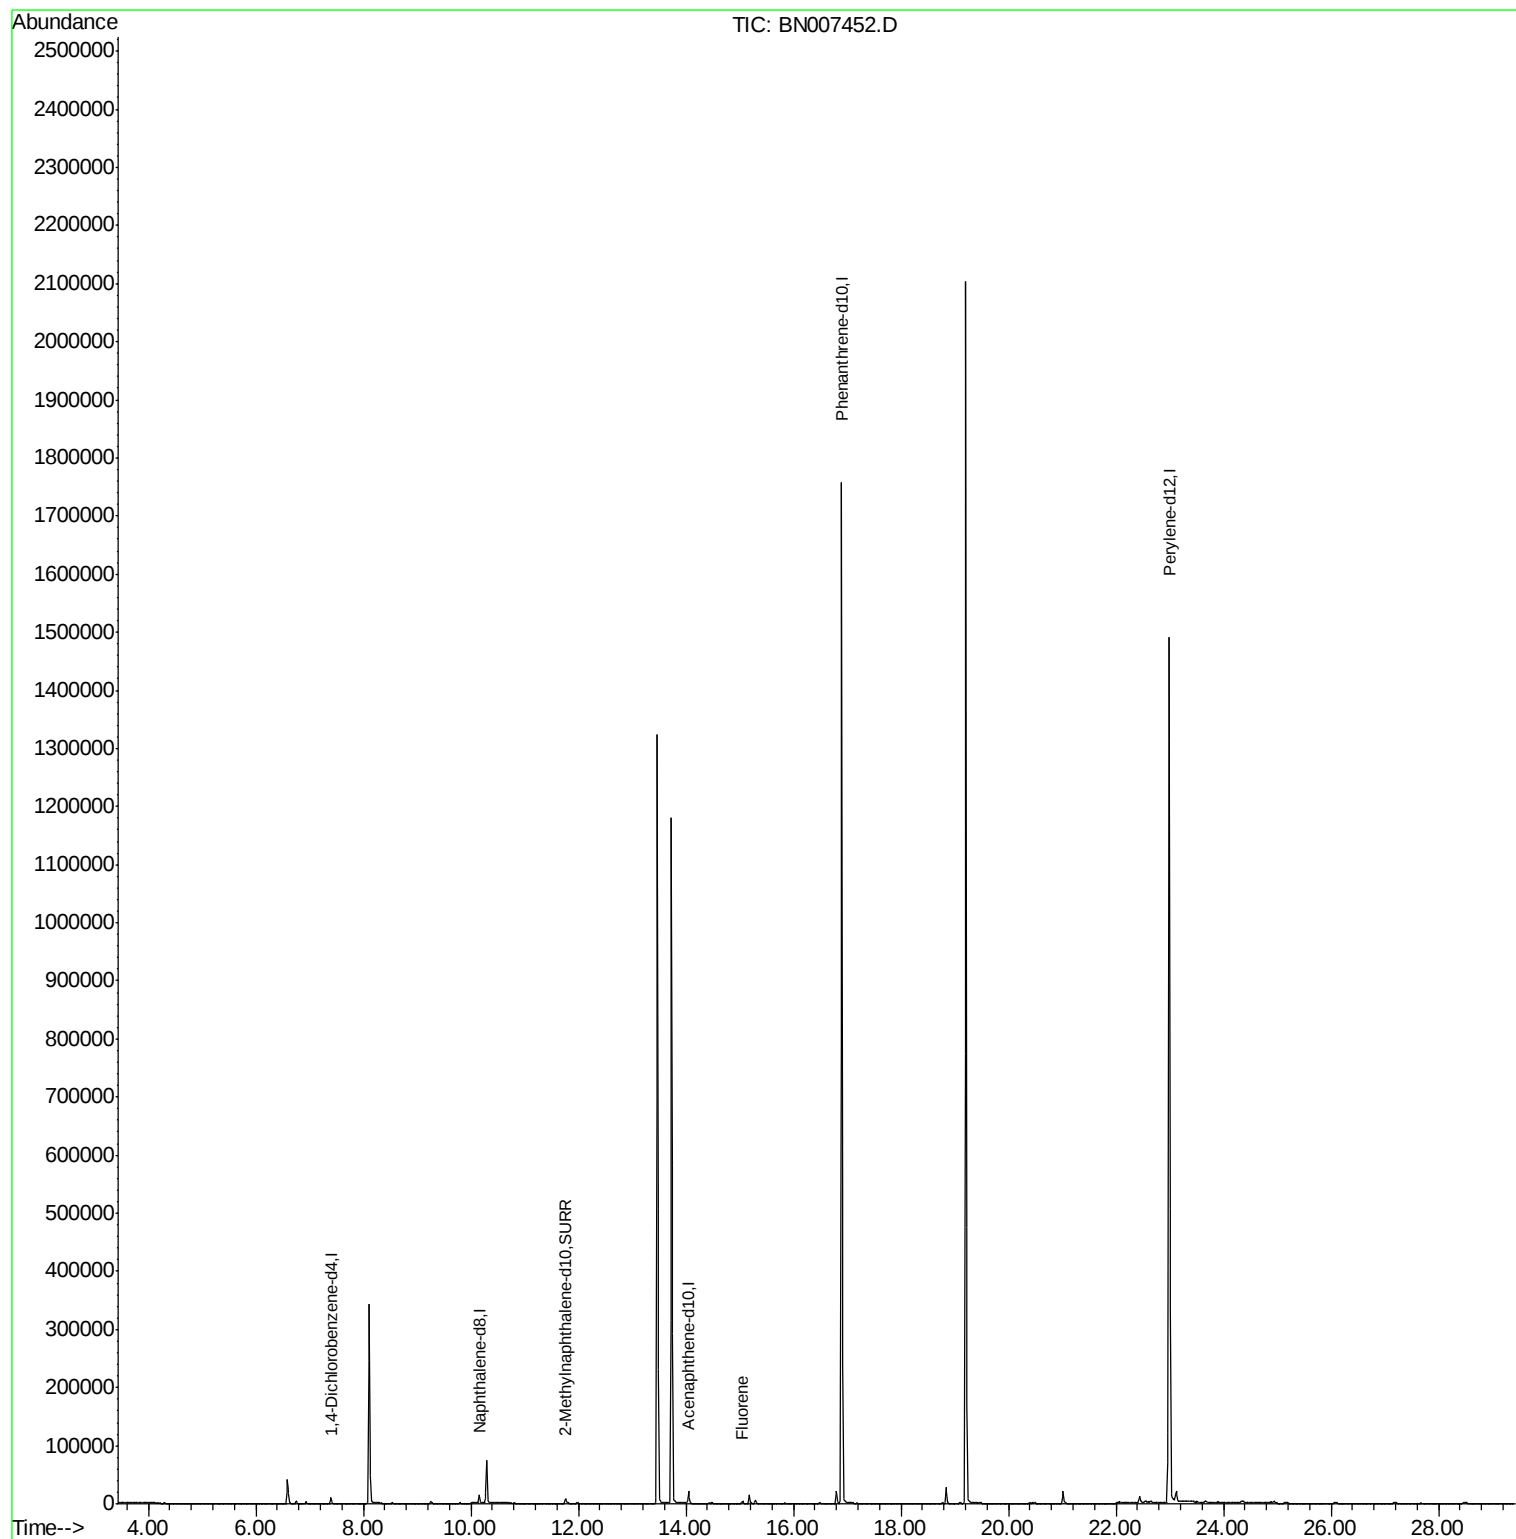

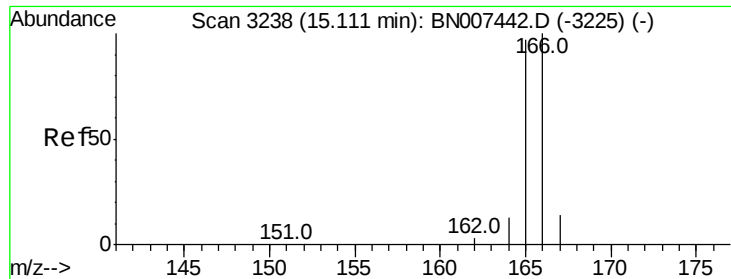

#9

Fluorene

Concen: 0.069 ng/ul

RT: 15.05 min Scan# 3225

Delta R.T. -0.06 min


Lab File: BN007452.D

Acq: 28 Aug 2019 03:18

Instrument :

BNA_N

ClientSampleId :

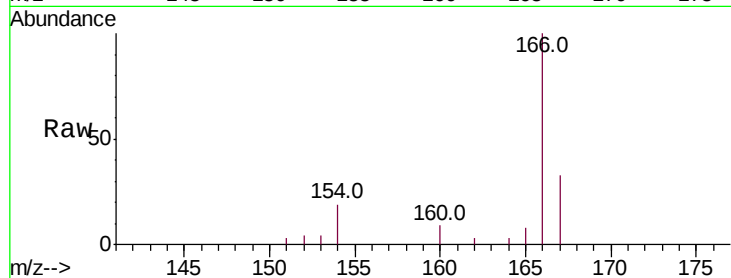


Tot Ion:166 Resp: 3360

Ion Ratio Lower Upper

166 100

165 7.5 79.6 119.4#

167 33.1 11.7 17.5#

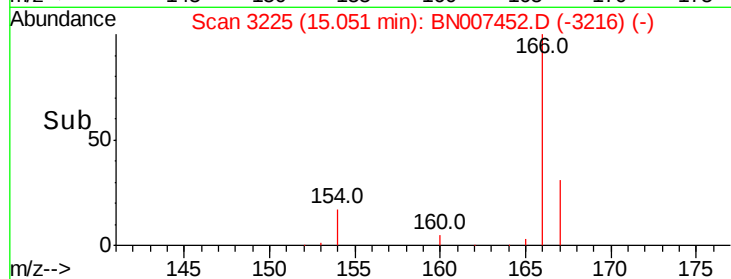

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

