

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\
 Data File : BN007480.D
 Acq On : 28 Aug 2019 22:12
 Operator : HP/JU
 Sample : K4373-21
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 28 23:03:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 27 20:30:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	5328	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	23349	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	12028	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.90	188	2116388	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.03
20) Perylene-d12	23.00	264	1946532	0.40	ng/ul	-0.13
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.75	152	10450	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.20	128	11309	0.172	ng/ul	97
8) Acenaphthene	14.11	153	1206	0.025	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\
Data File : BN007480.D
Acq On : 28 Aug 2019 22:12
Operator : HP/JU
Sample : K4373-21
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 28 23:03:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 20:30:31 2019
Response via : Initial Calibration

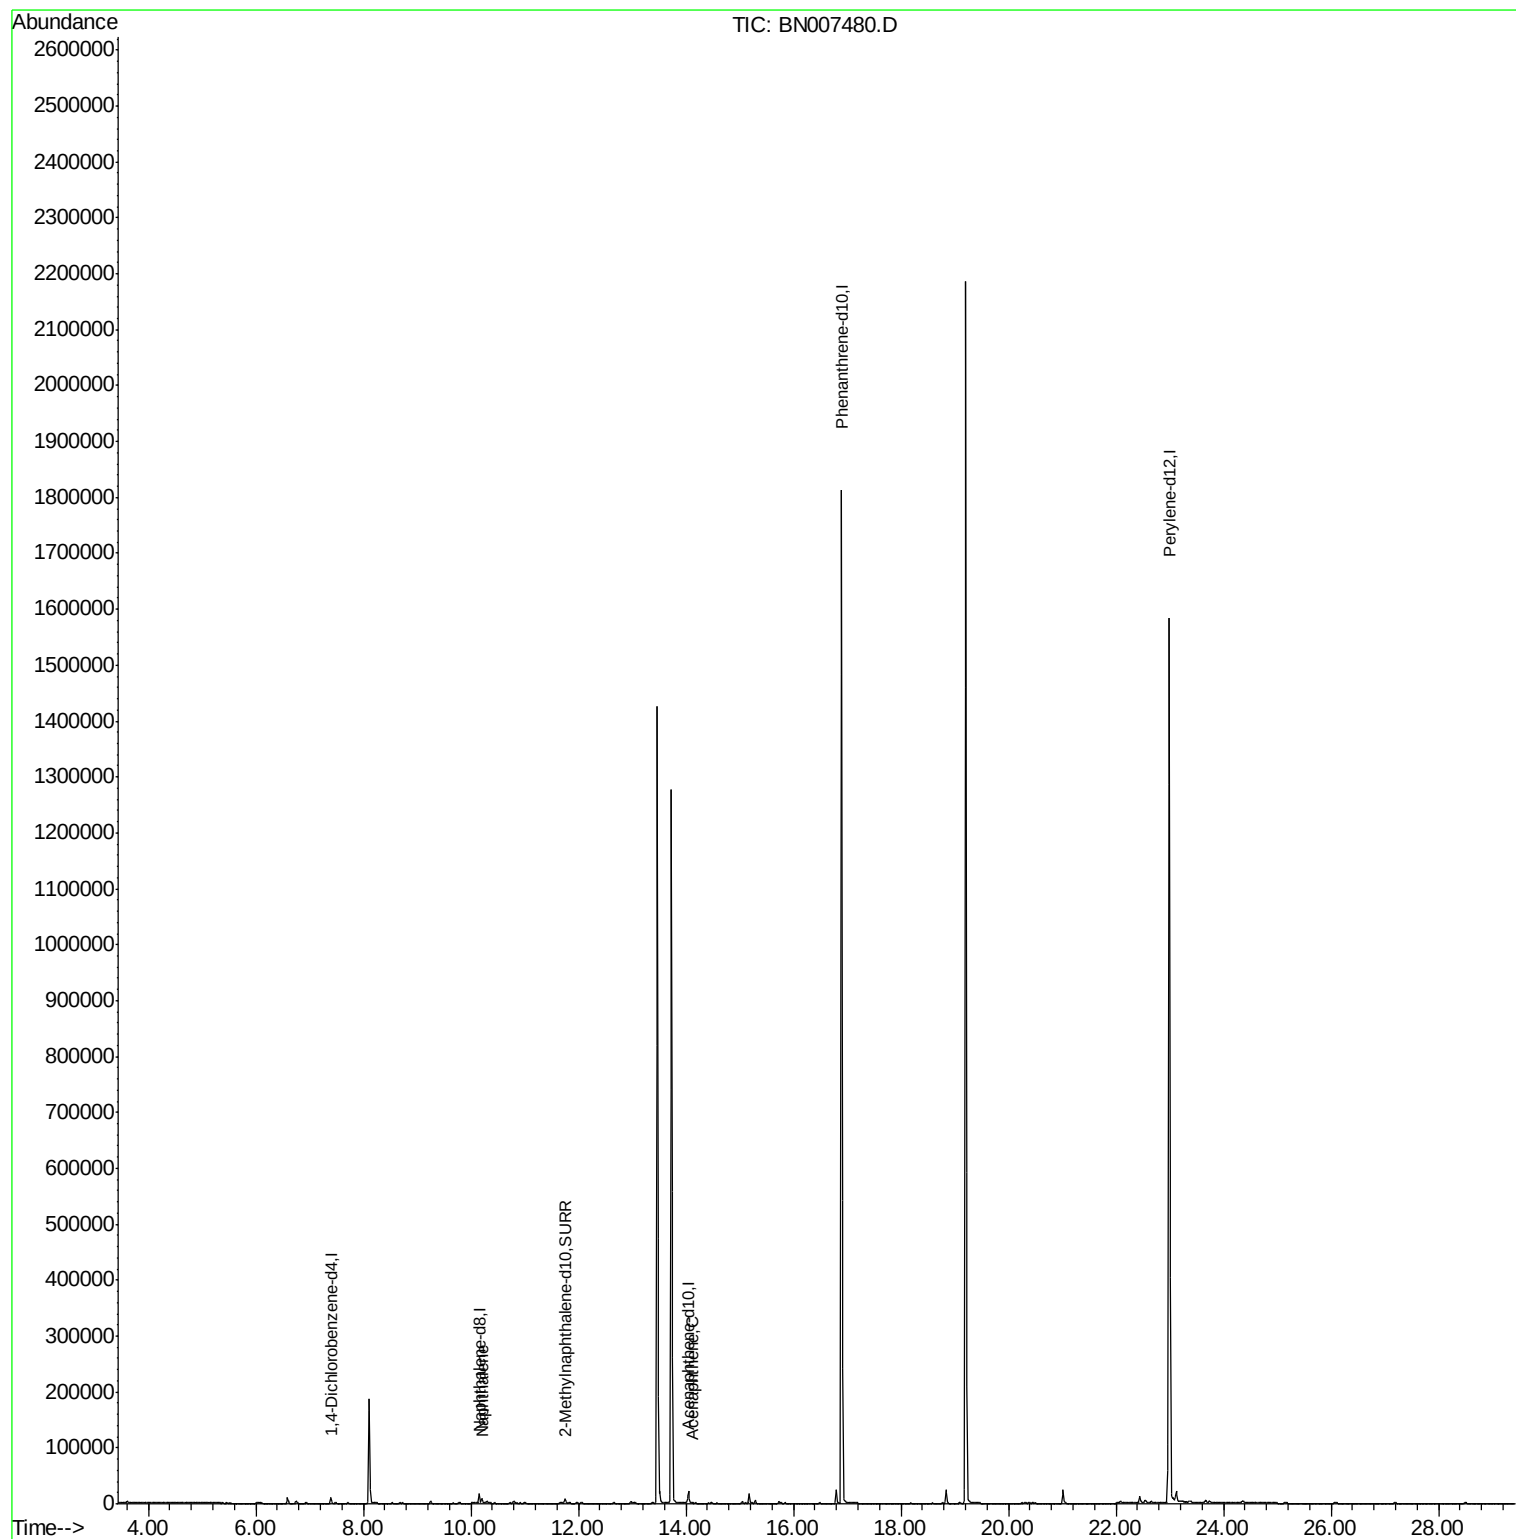

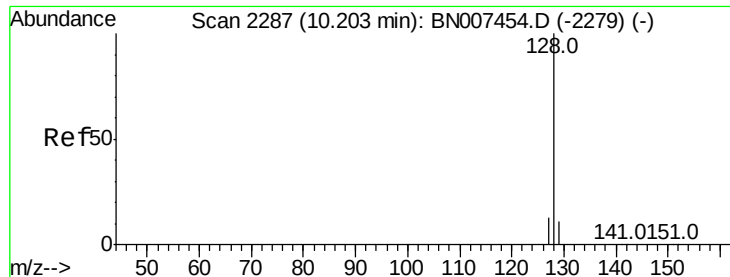

#3

Naphthalene

Concen: 0.172 ng/ul

RT: 10.20 min Scan# 2287

Delta R.T. -0.01 min

Lab File: BN007480.D

Acq: 28 Aug 2019 22:12

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 11309

Ion Ratio Lower Upper

128 100

129 12.7 9.2 13.8




127 13.9 10.4 15.6

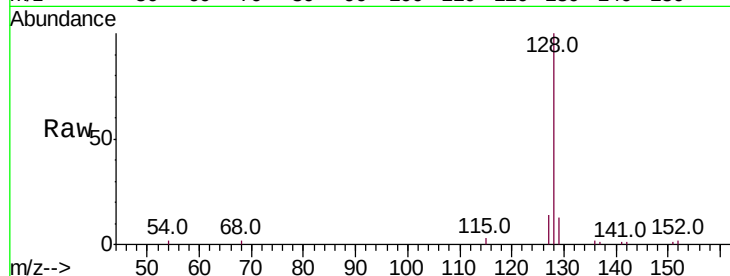

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

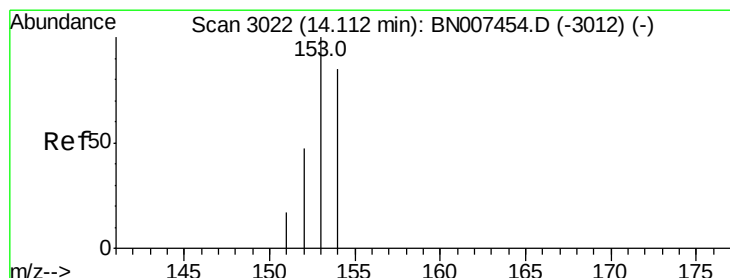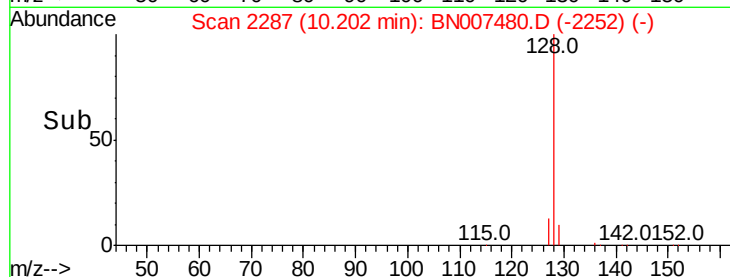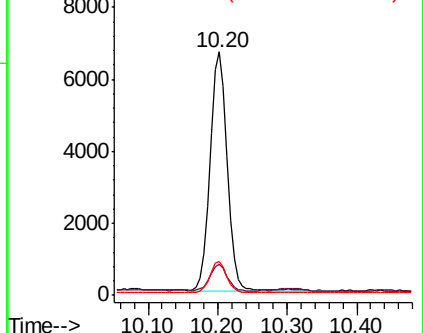

#8

Acenaphthene

Concen: 0.025 ng/ul

RT: 14.11 min Scan# 3022

Delta R.T. -0.00 min

Lab File: BN007480.D

Acq: 28 Aug 2019 22:12


Tgt Ion:153 Resp: 1206

Ion Ratio Lower Upper

153 100

152 51.2 39.1 58.7

154 88.2 69.4 104.2

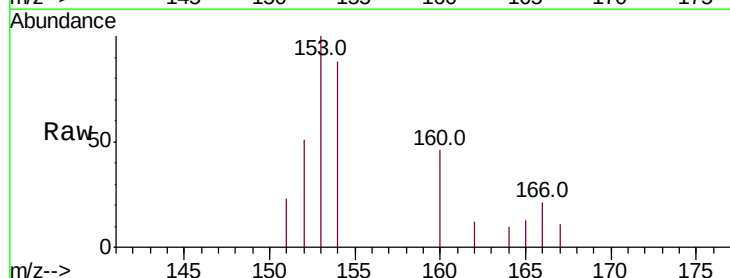

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

