

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:21:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

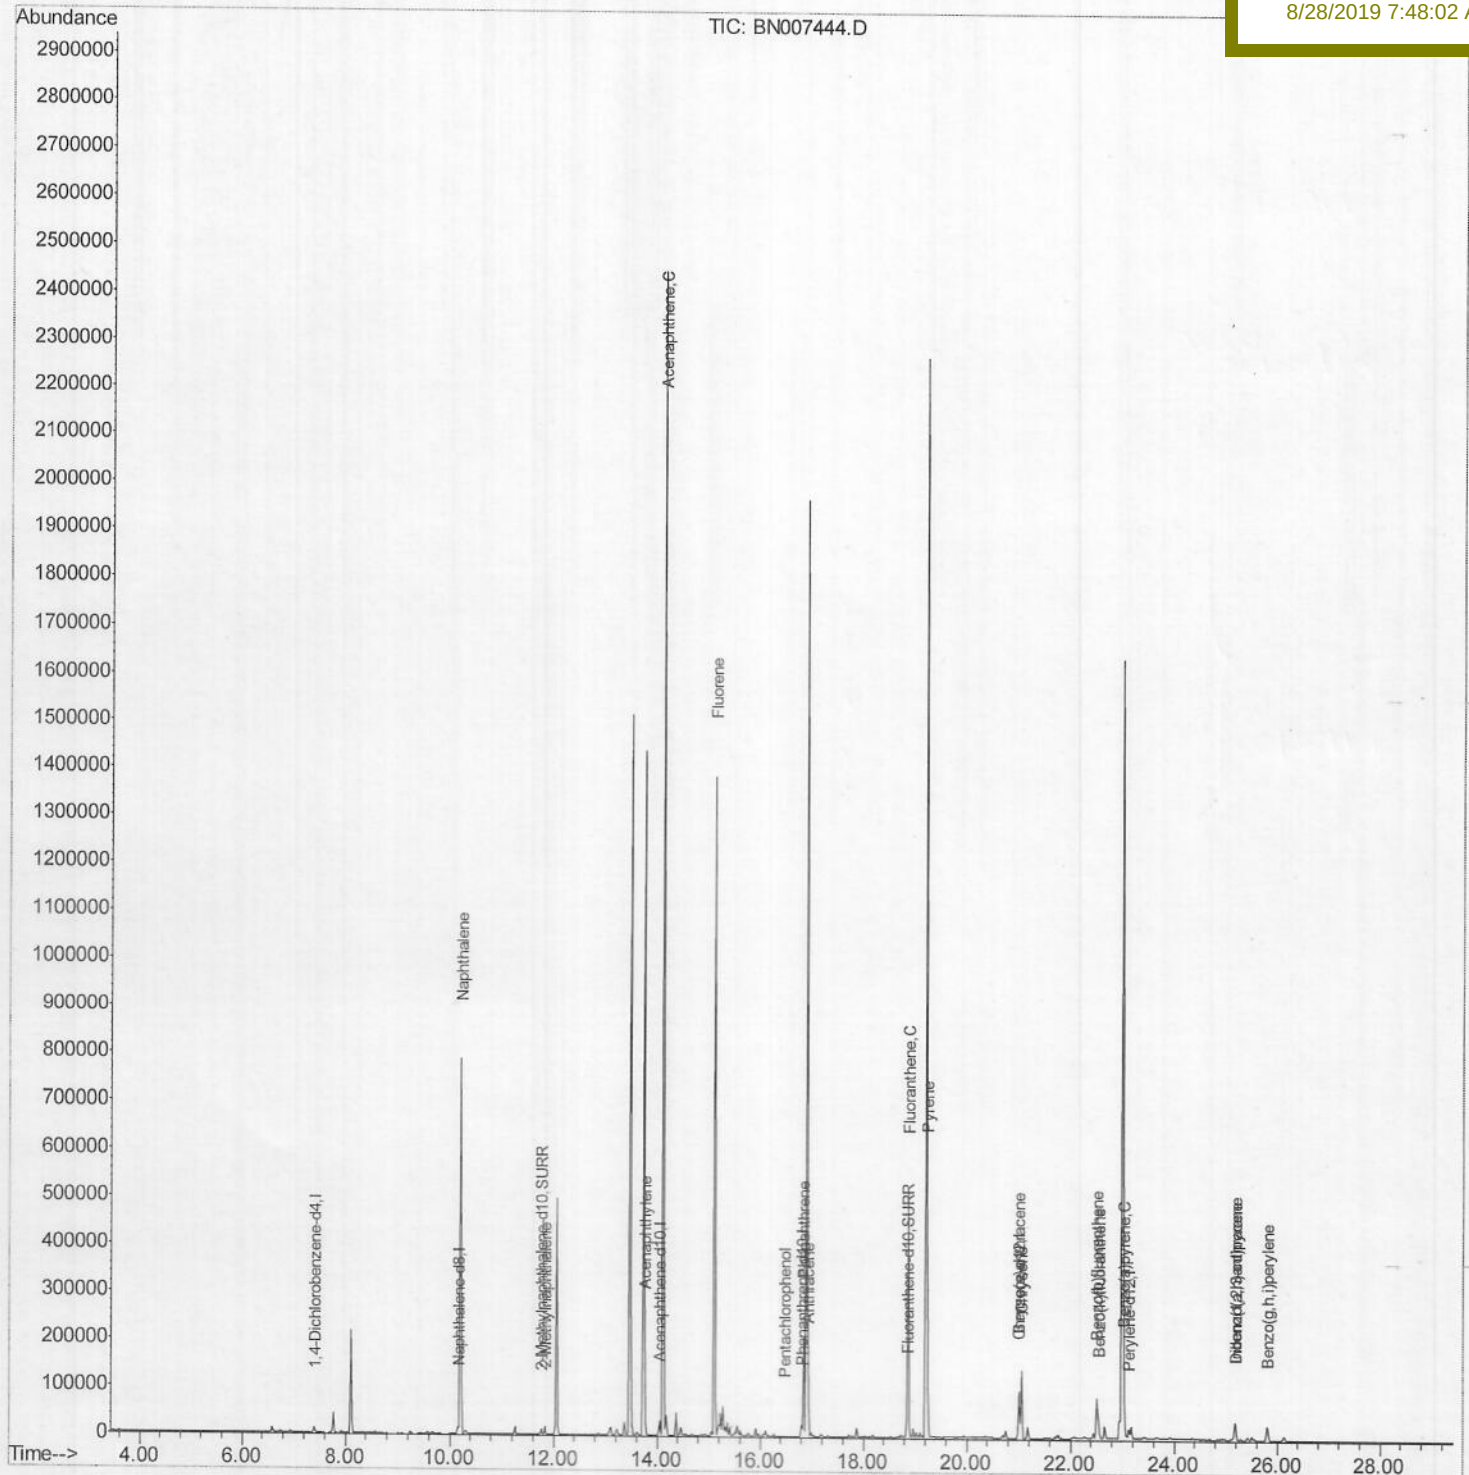
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:04:52 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

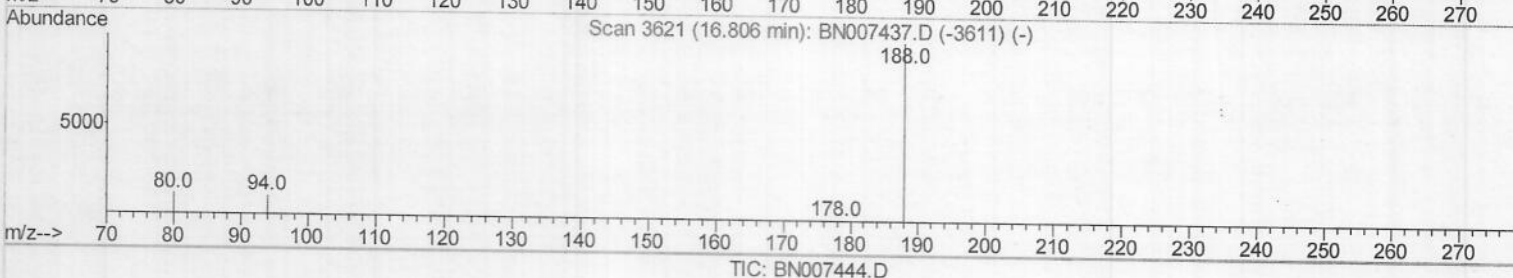
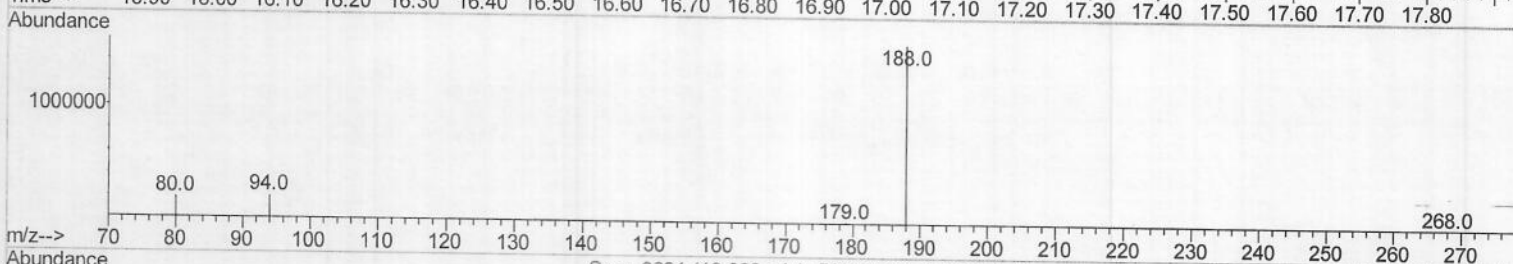
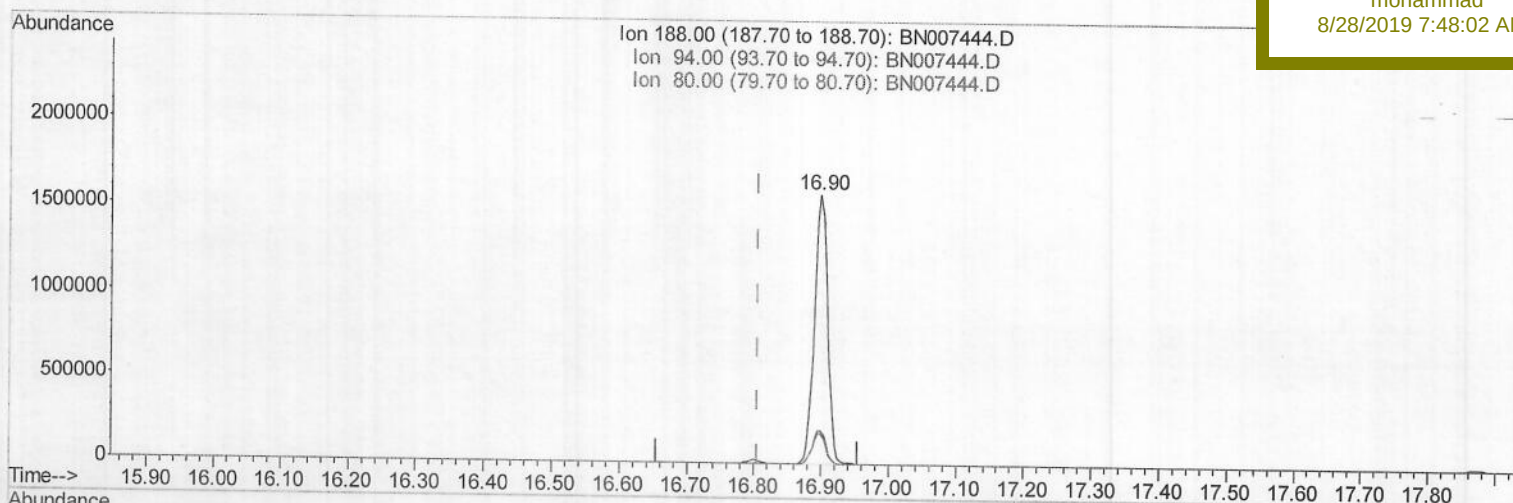
C0AF6

Manual Integrations

APPROVED

mohammad

8/28/2019 7:48:02 AM



(10) Phenanthrene-d10 (I)

16.899min (+0.093) 0.40ng/ul

response 2201493

Ion	Exp%	Act%
188.00	100	100
94.00	11.30	12.48
80.00	12.40	11.49
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:04:52 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

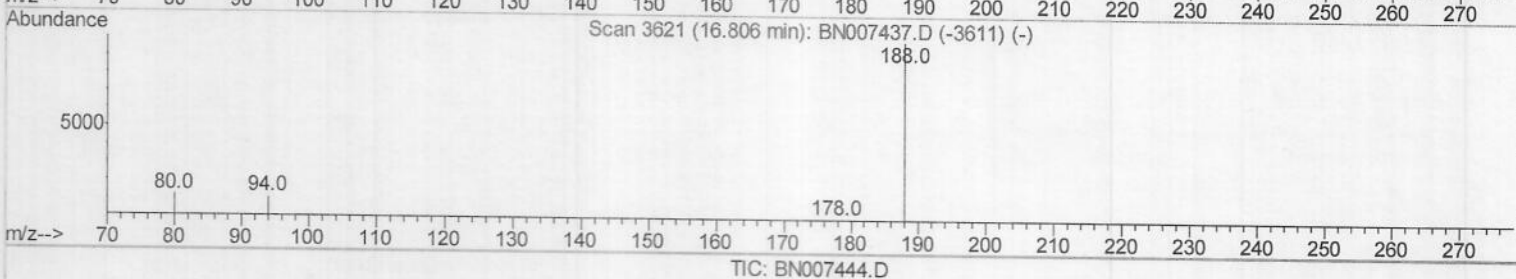
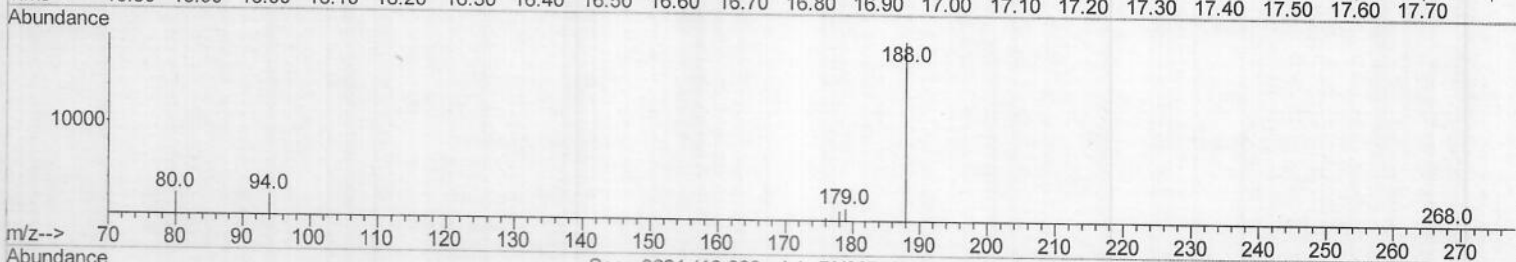
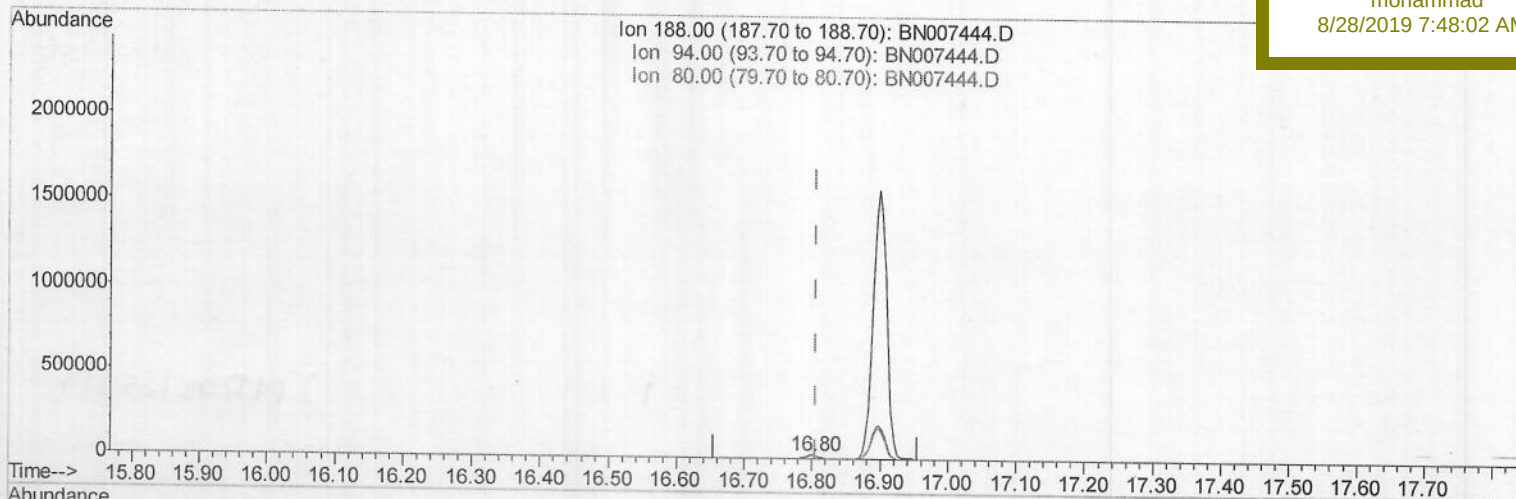
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(10) Phenanthrene-d10 (I)

16.802min (-0.004) 0.40ng/ul m

response 26480

Ion	Exp%	Act%
188.00	100	100
94.00	11.30	11.83
80.00	12.40	12.39
0.00	0.00	0.00

JU
08/28/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

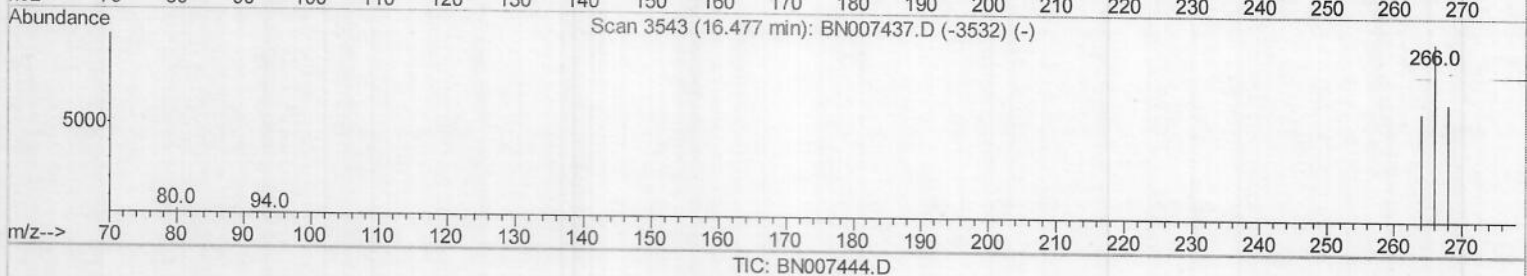
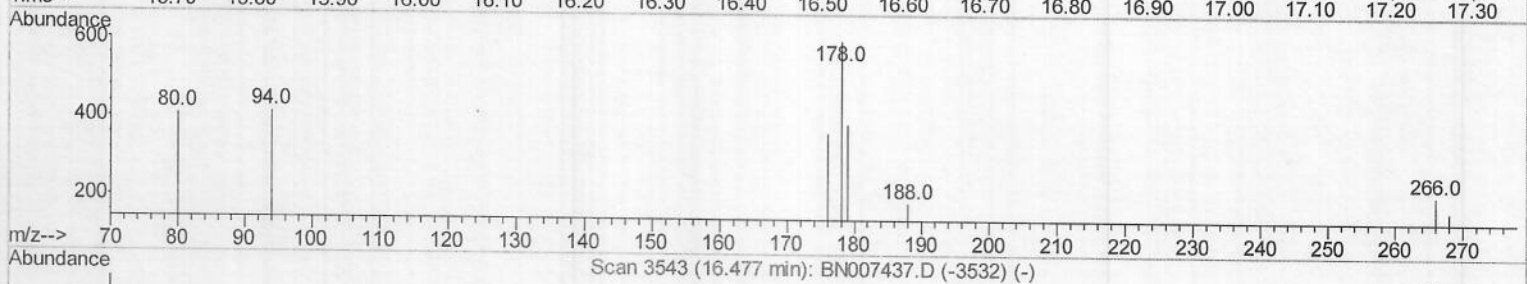
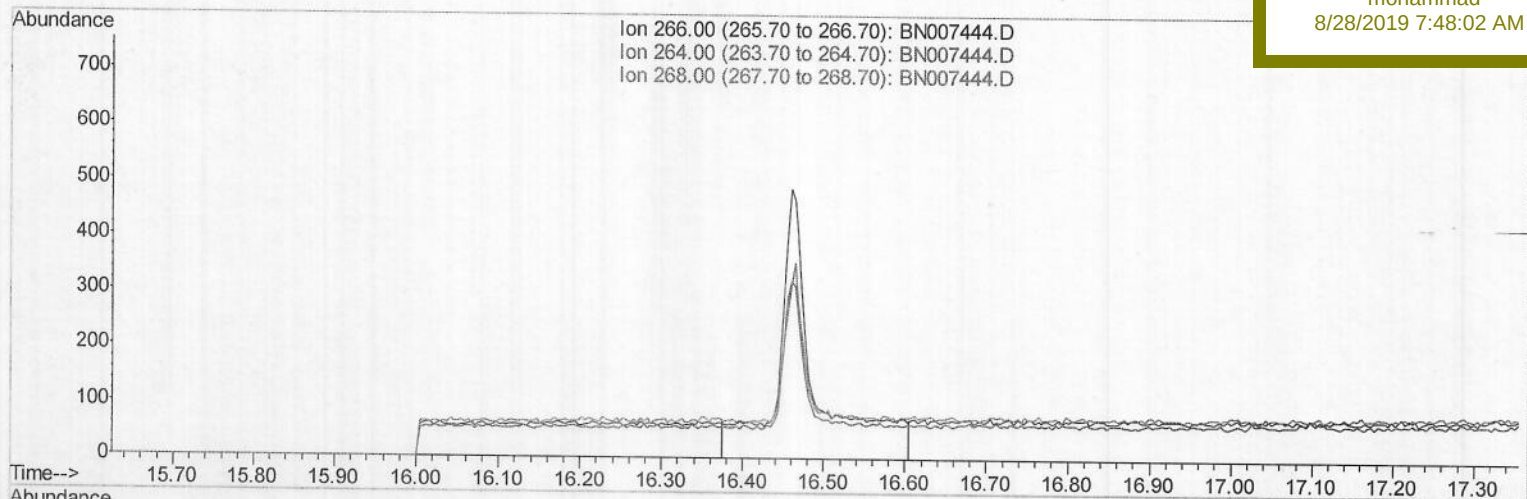
ClientSampleId :

C0AF6

Manual Integrations
APPROVED

mohammad

8/28/2019 7:48:02 AM



(11) Pentachlorophenol

16.477min (-16.477) 0.00ng/ul

response 0

Ion	Exp%	Act%
266.00	100	0.00
264.00	61.30	0.00#
268.00	62.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

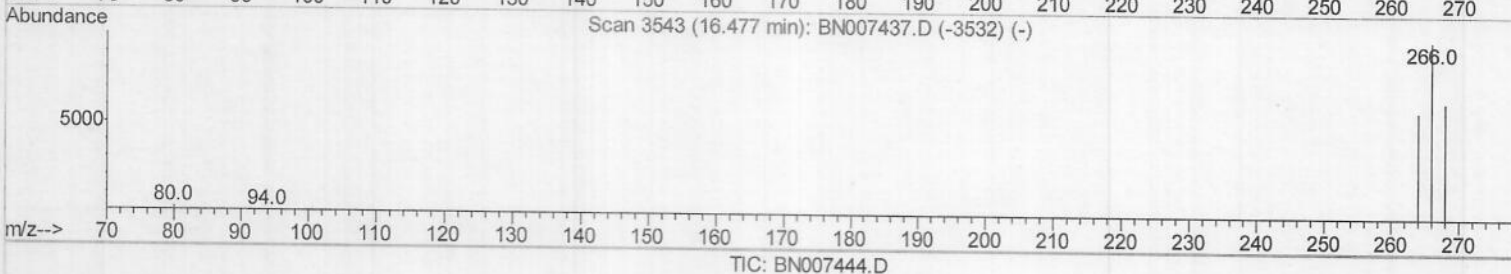
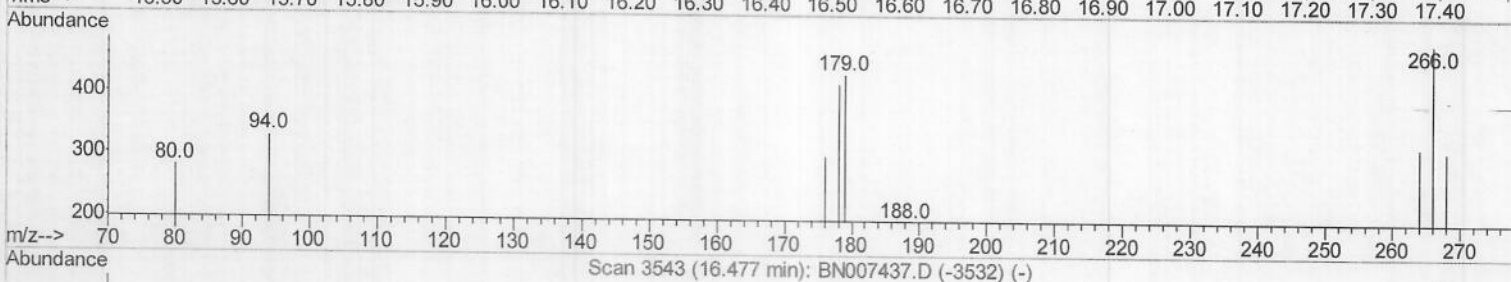
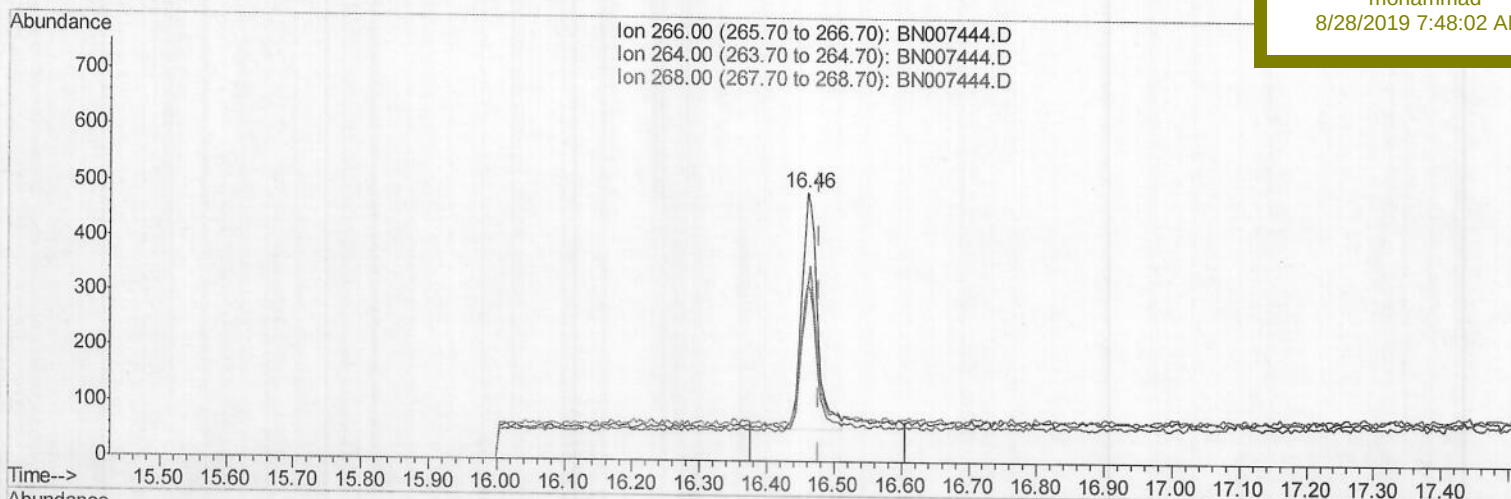
C0AF6

Manual Integrations

APPROVED

mohammad

8/28/2019 7:48:02 AM



(11) Pentachlorophenol

16.460min (-0.017) 0.12ng/ul m) JU
 08/28/19

response 694

Ion	Exp%	Act%
266.00	100	100
264.00	61.30	0.00#
268.00	62.70	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

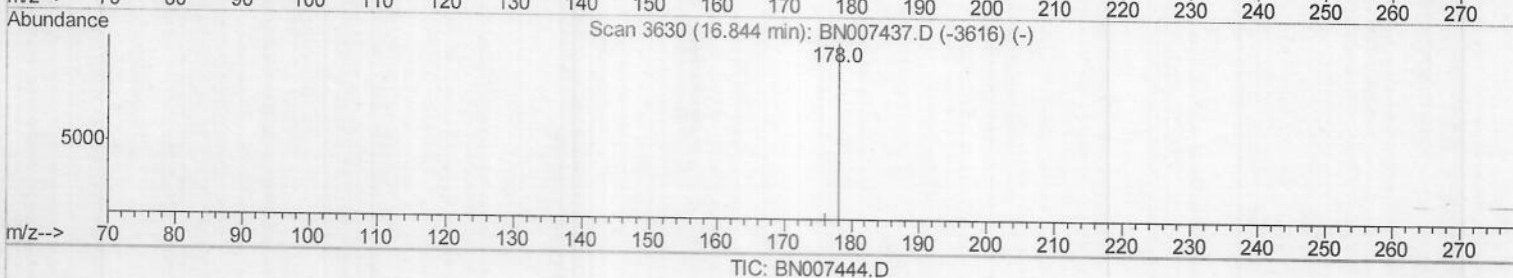
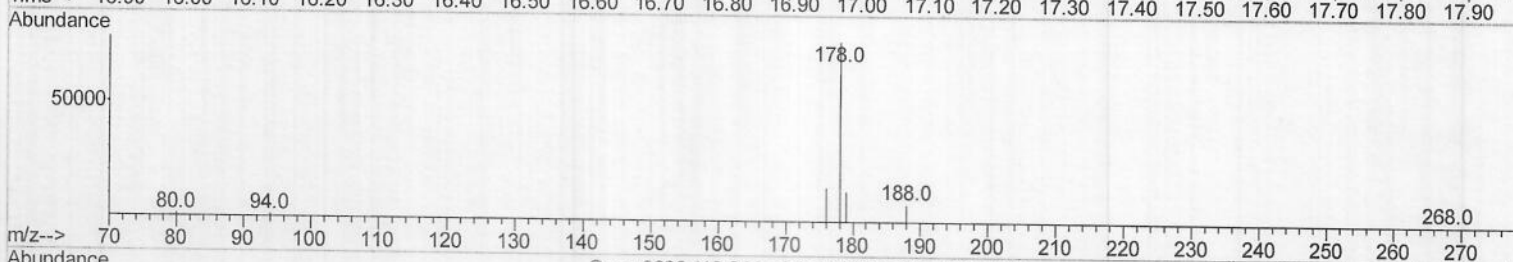
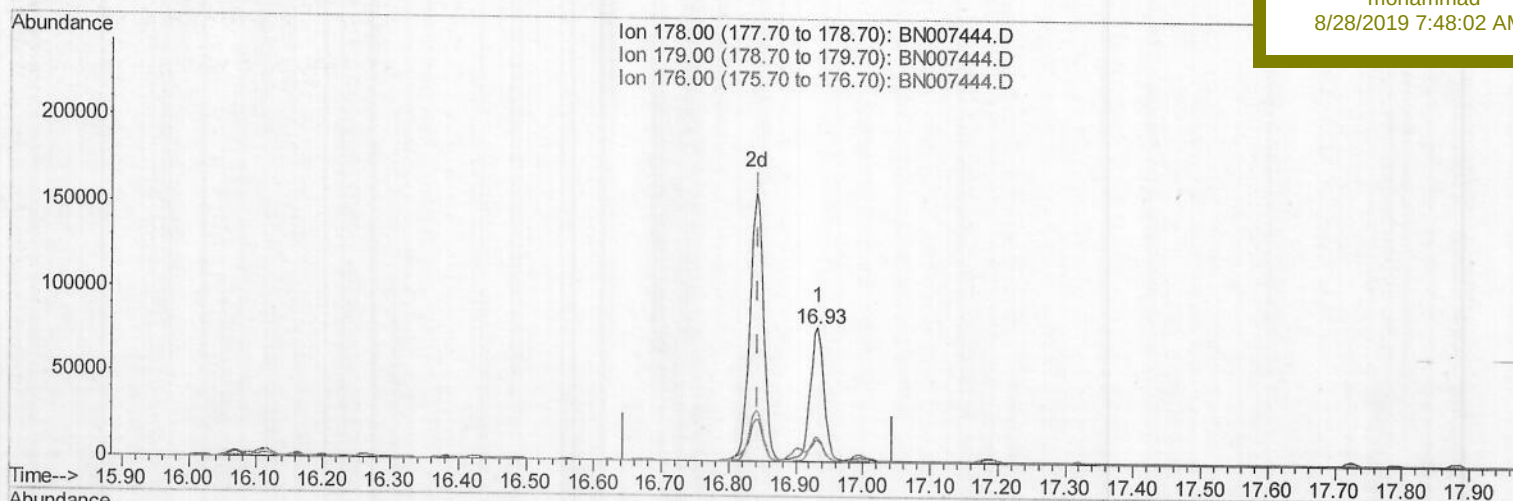
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(12) Phenanthrene

16.933min (+0.089) 1.31ng/ul

response 108378

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	16.33
176.00	19.00	18.41
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

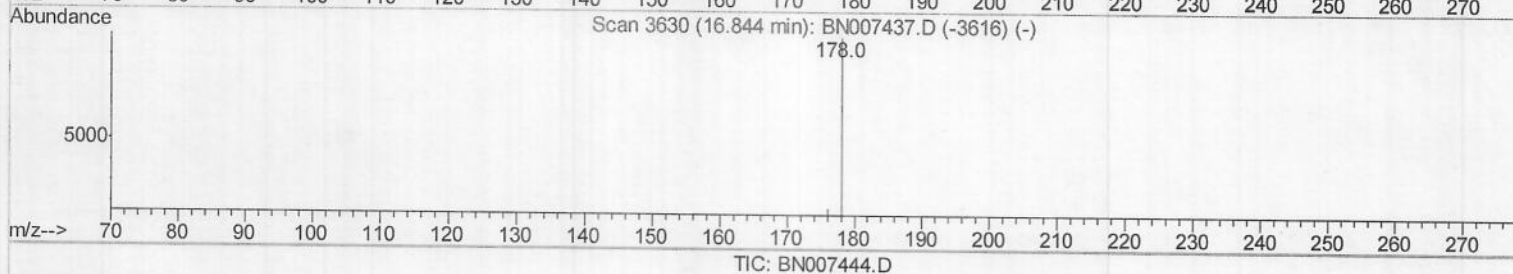
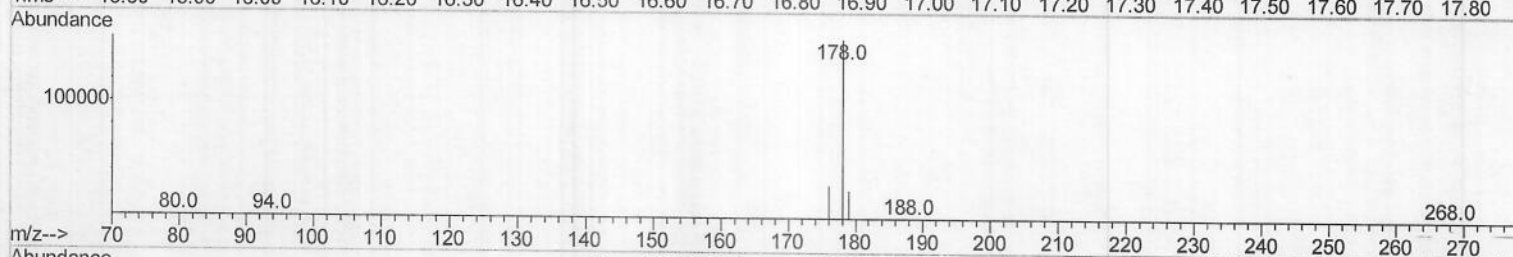
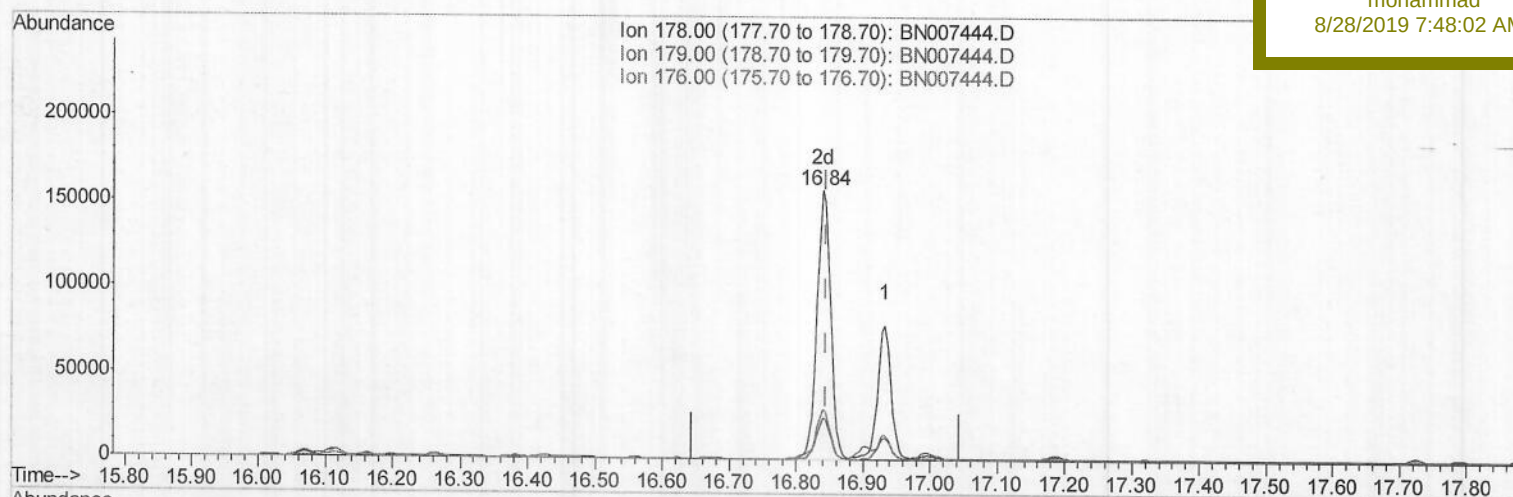
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(12) Phenanthrene

16.840min (-0.004) 2.74ng/ul m)JU
08/28/19

response 226440

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	15.56
176.00	19.00	18.85
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

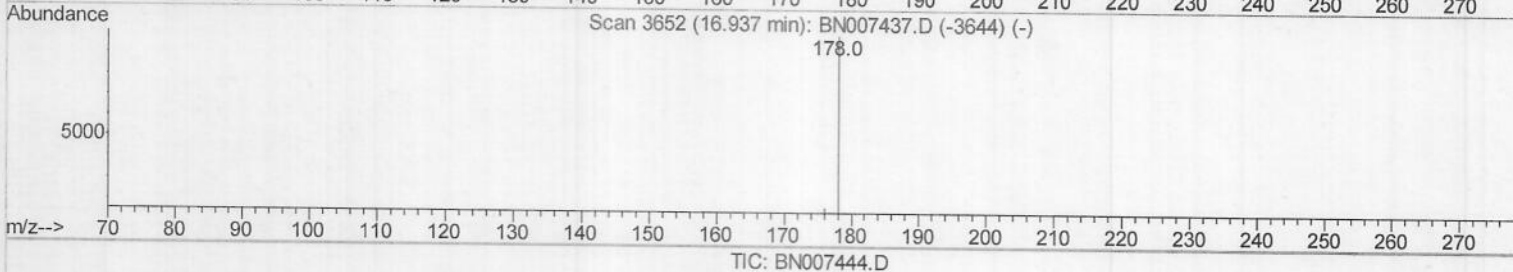
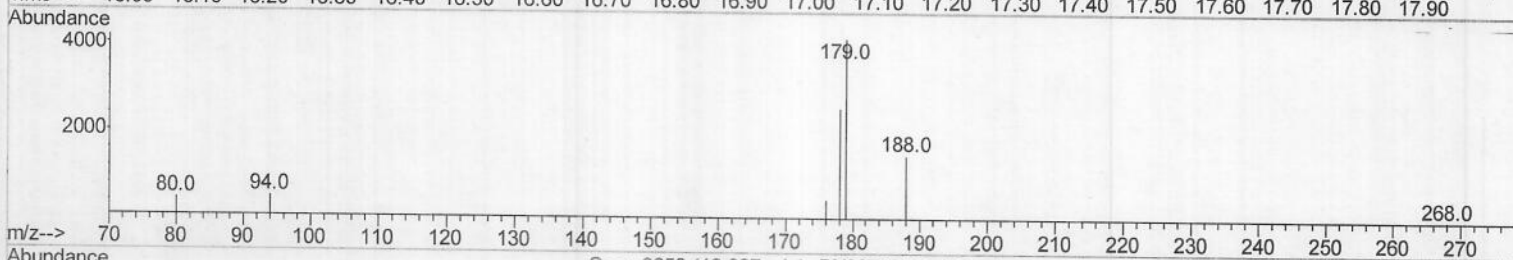
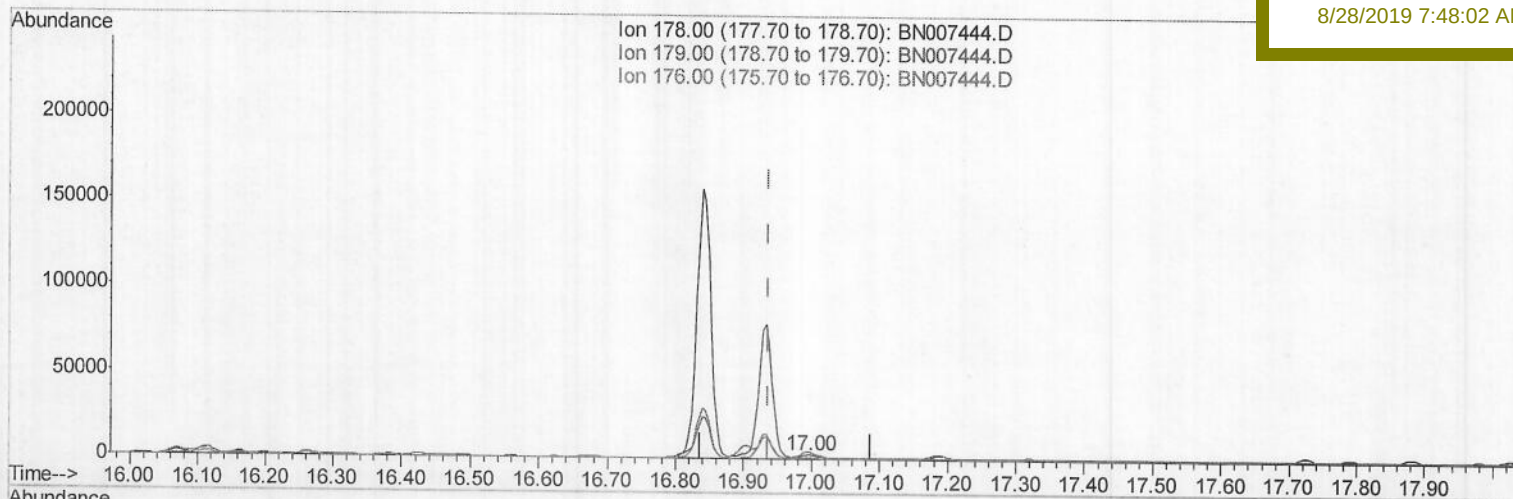
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(13) Anthracene

16.996min (+0.059) 0.04ng/ul

response 3354

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	162.43#
176.00	18.20	18.57
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

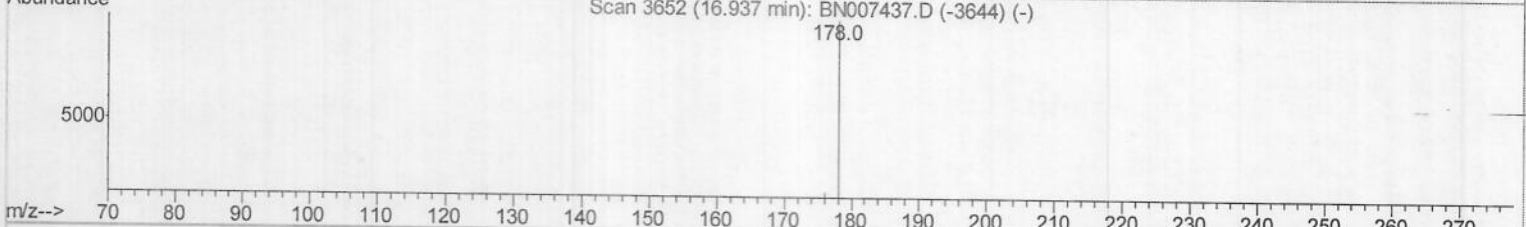
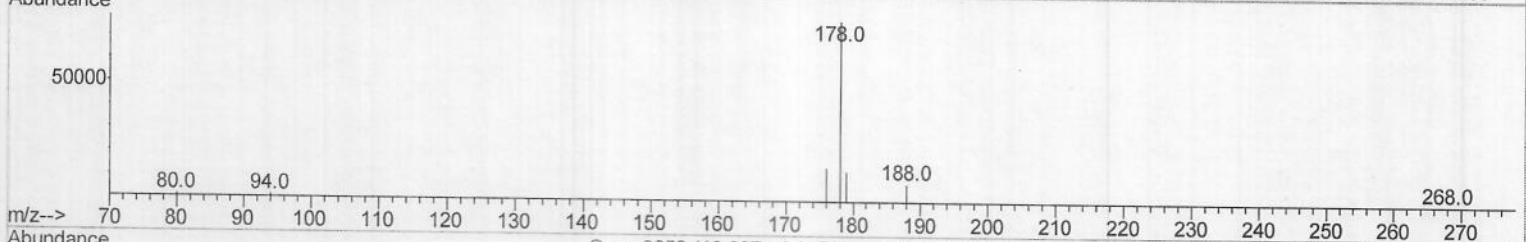
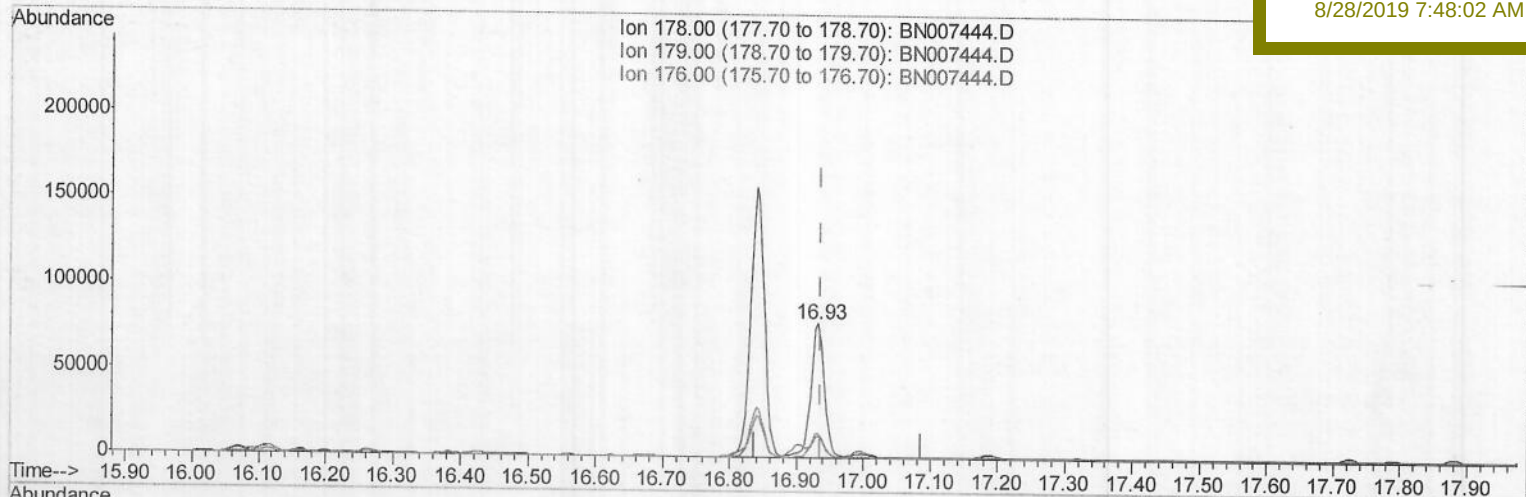
C0AF6

Manual Integrations

APPROVED

mohammad

8/28/2019 7:48:02 AM



TIC: BN007444.D

(13) Anthracene

16.933min (-0.004) 1.38ng/ul m) JU
08/28/19

response 107776

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	16.33
176.00	18.20	18.41
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

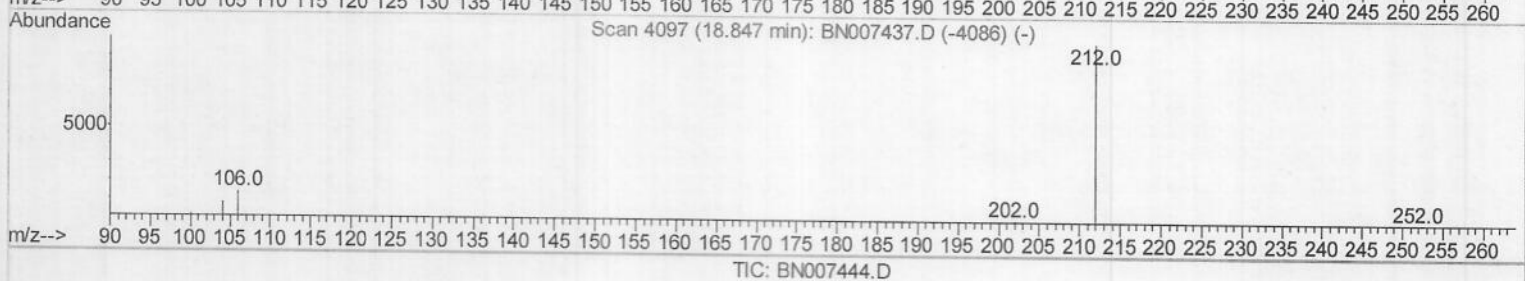
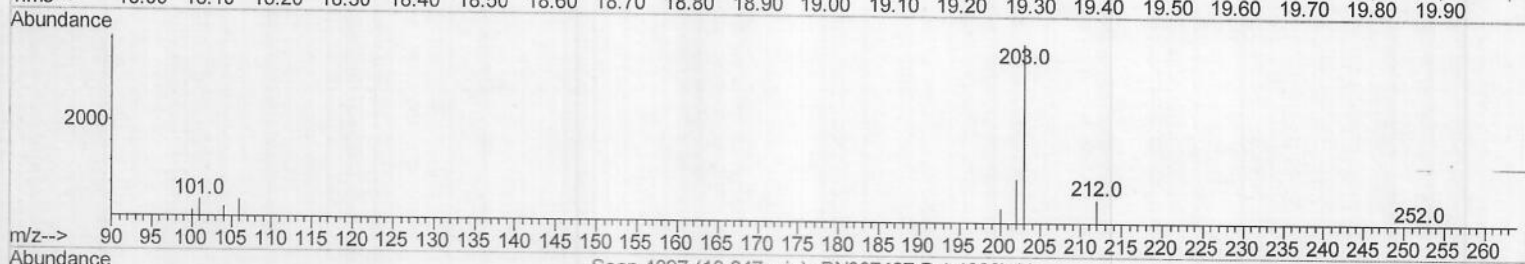
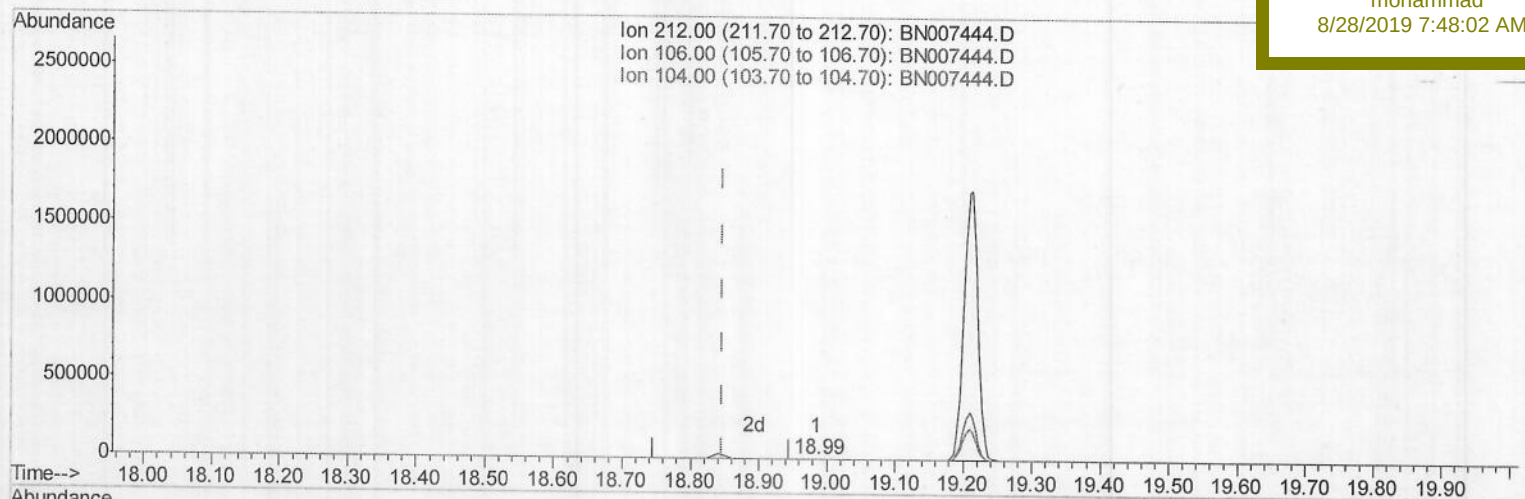
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(14) Fluoranthene-d10 (SURR)

18.986min (+0.139) 0.01ng/ul

response 670

Ion	Exp%	Act%
212.00	100	100
106.00	14.30	0.00#
104.00	8.00	16.12#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

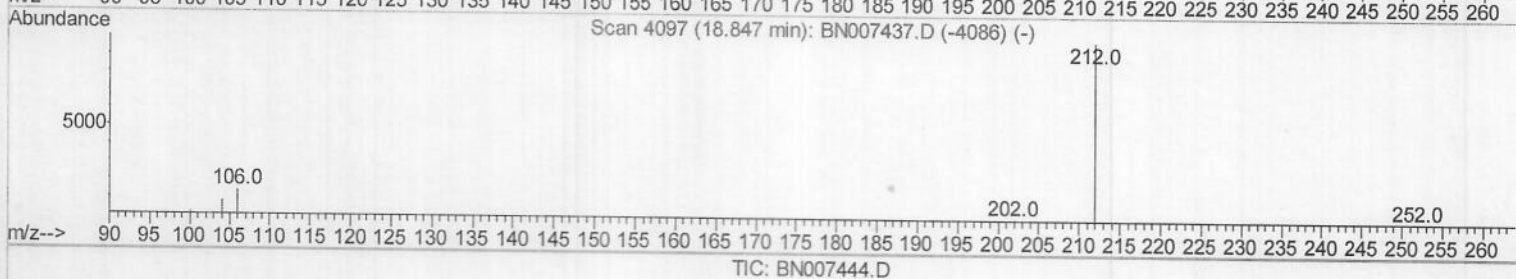
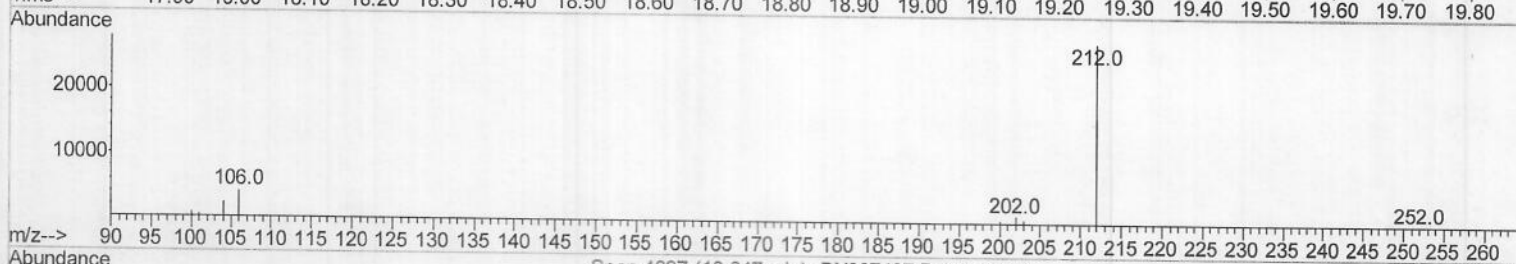
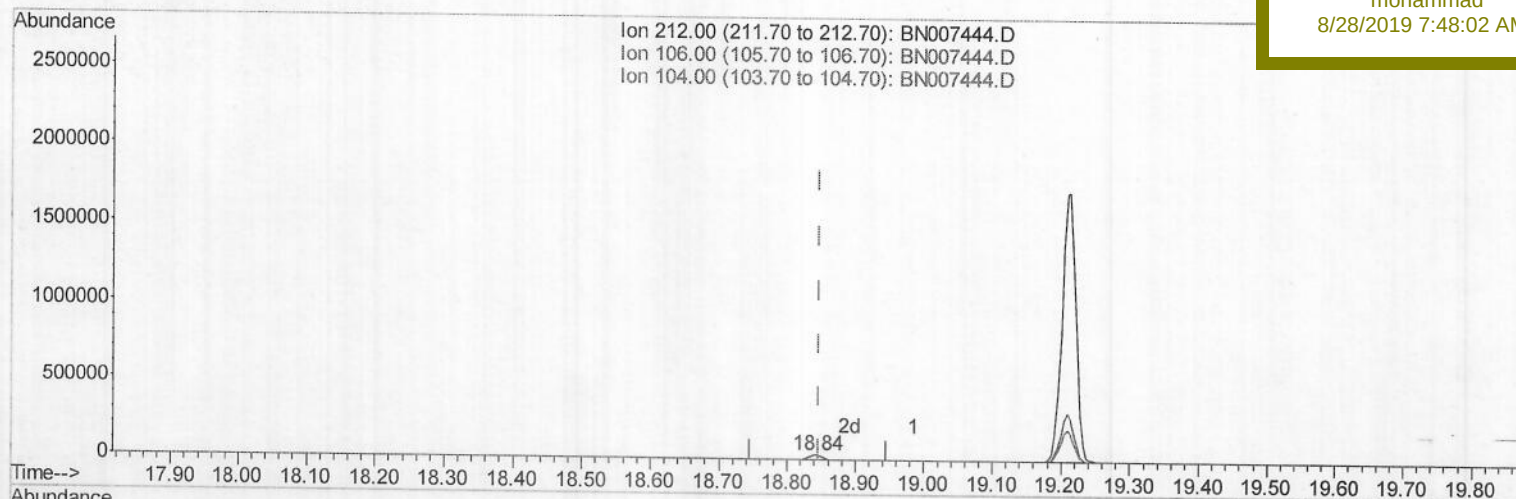
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(14) Fluoranthene-d10 (SURR)

18.842min (-0.005) 0.42ng/ul m

response 35984

Ion	Exp%	Act%
212.00	100	100
106.00	14.30	0.00#
104.00	8.00	0.30#
0.00	0.00	0.00

JU
08/28/19

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

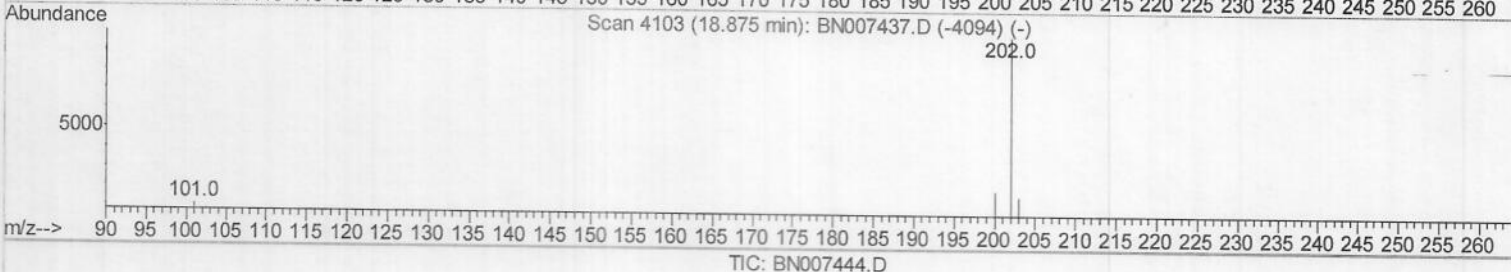
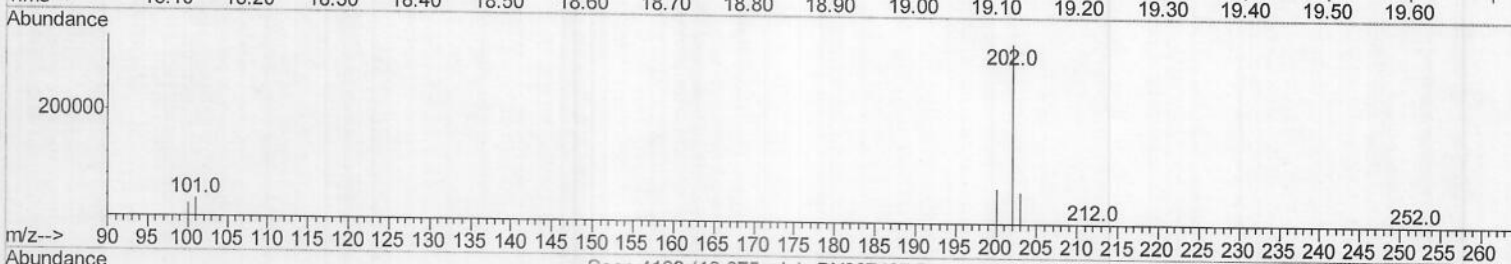
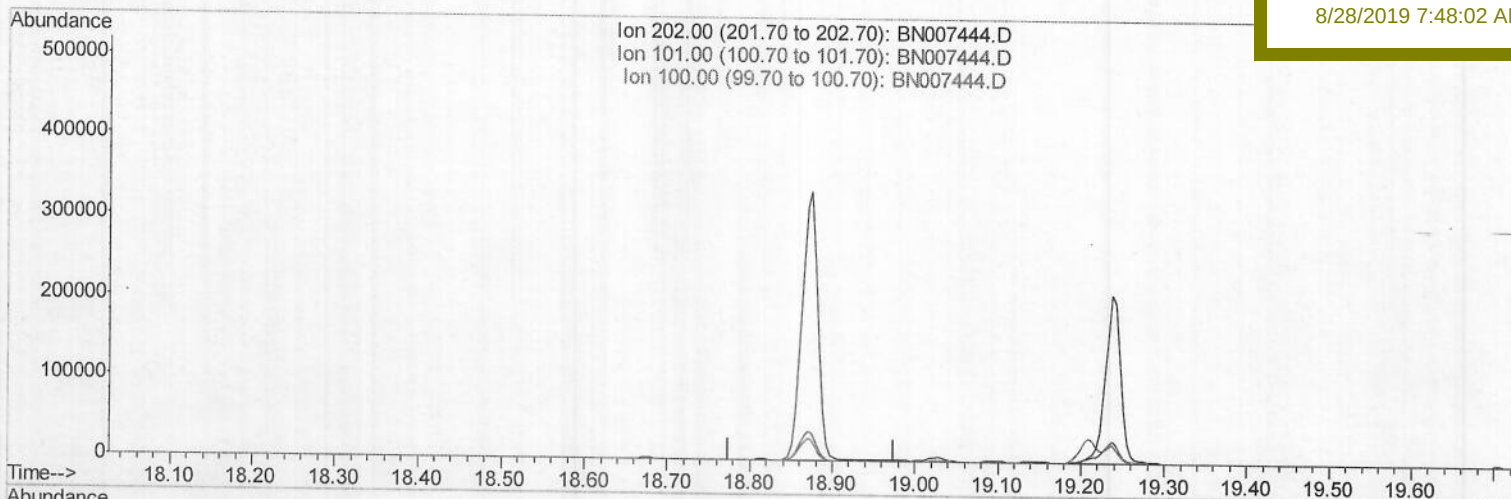
C0AF6

Manual Integrations

APPROVED

mohammad

8/28/2019 7:48:02 AM



(15) Fluoranthene (C)

18.875min (-18.875) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	11.30	0.00
100.00	8.50	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

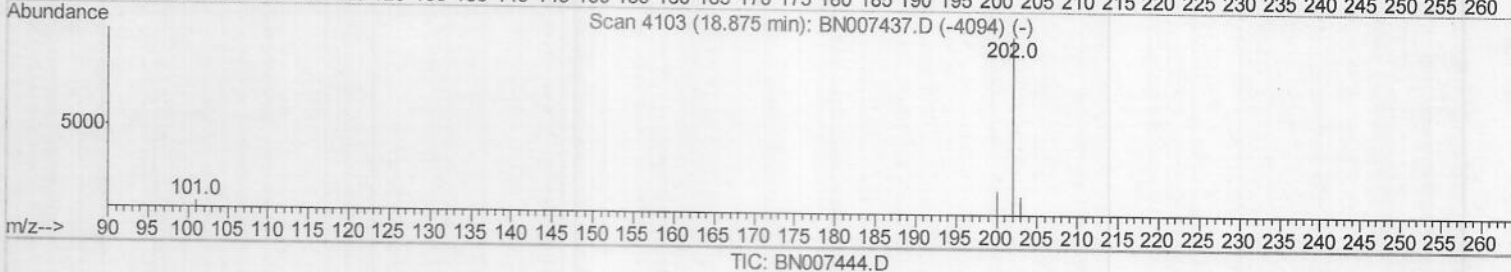
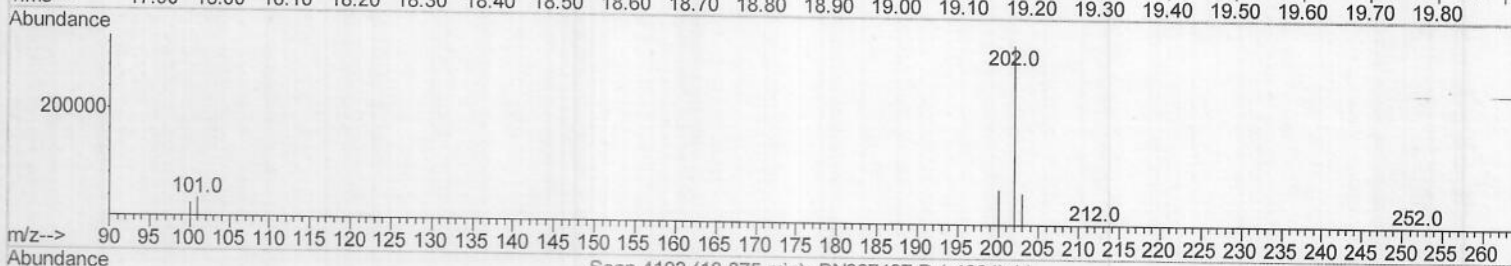
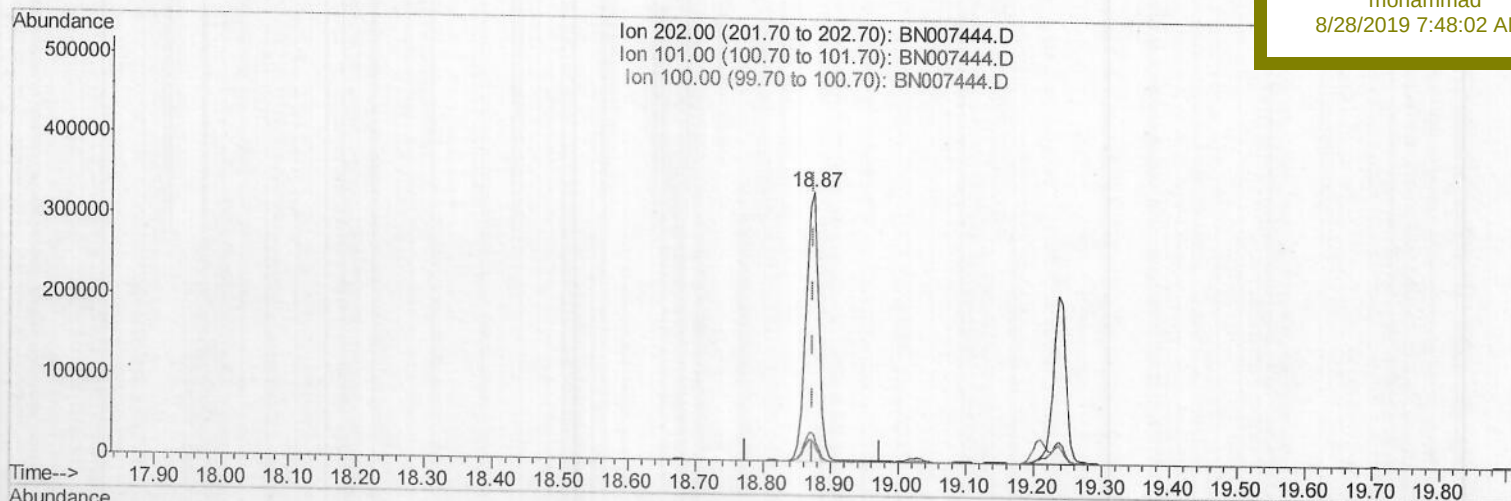
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(15) Fluoranthene (C)

18.875min (-0.000) 4.04ng/ul m) JU
08/28/19

response 446396

Ion	Exp%	Act%
202.00	100	100
101.00	11.30	10.05
100.00	8.50	7.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

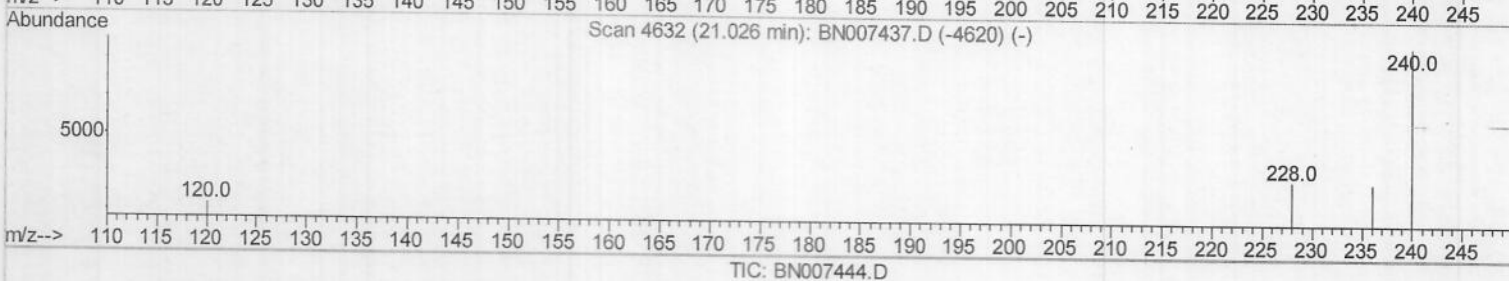
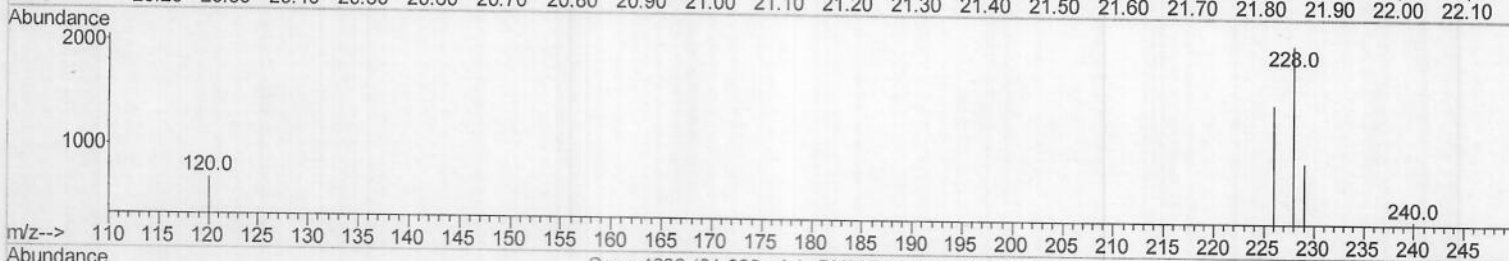
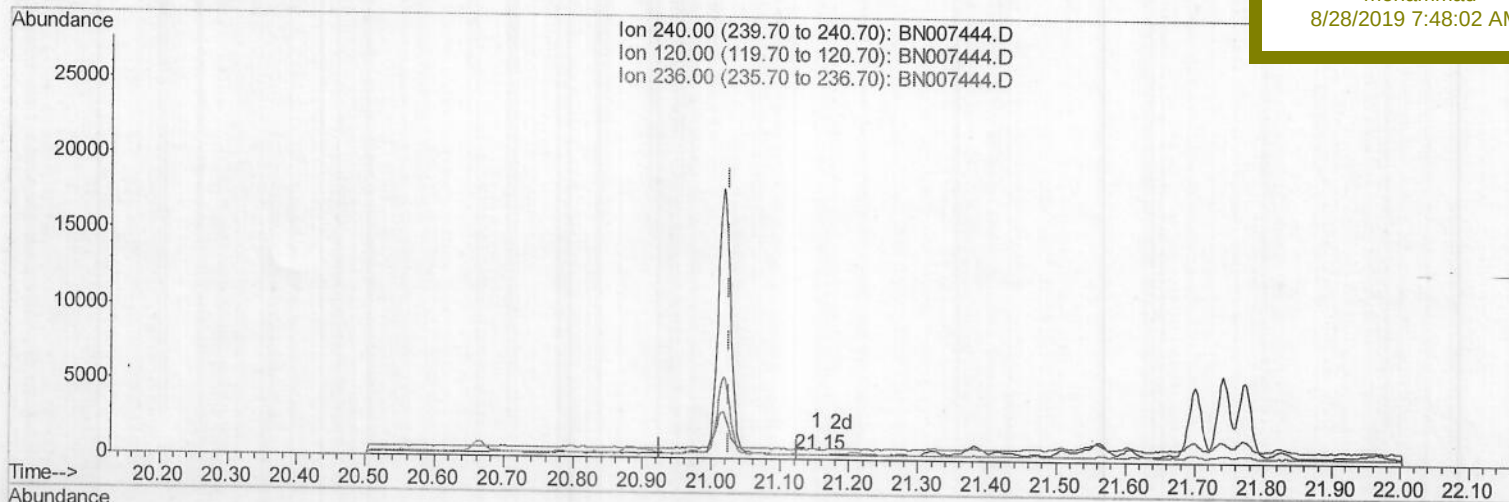
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(16) Chrysene-d12 (I)

21.154min (+0.128) 0.40ng/ul

response 93

Ion	Exp%	Act%
240.00	100	100
120.00	15.00	188.74#
236.00	28.60	91.21#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:17:11 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

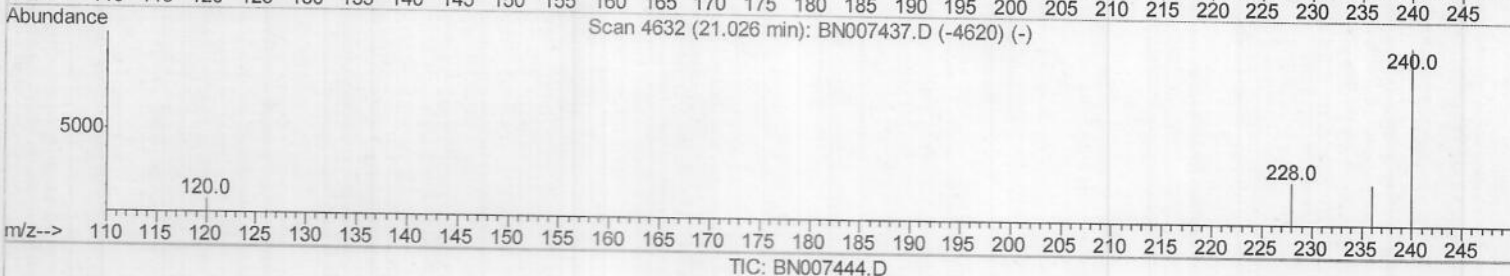
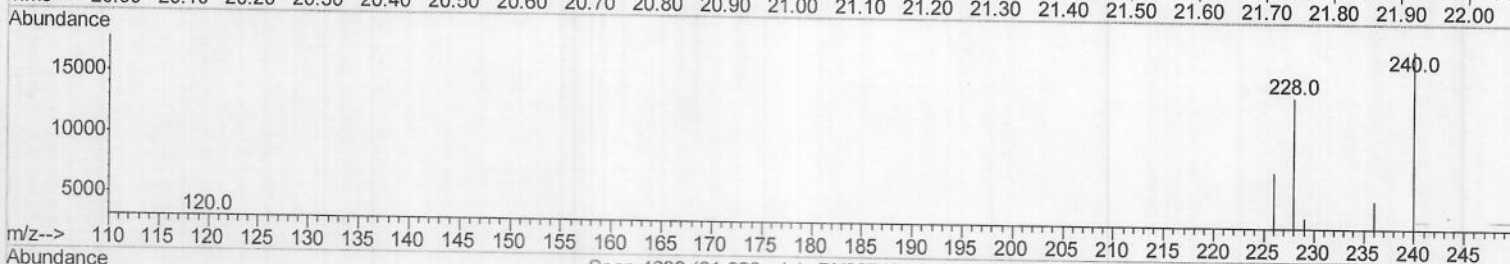
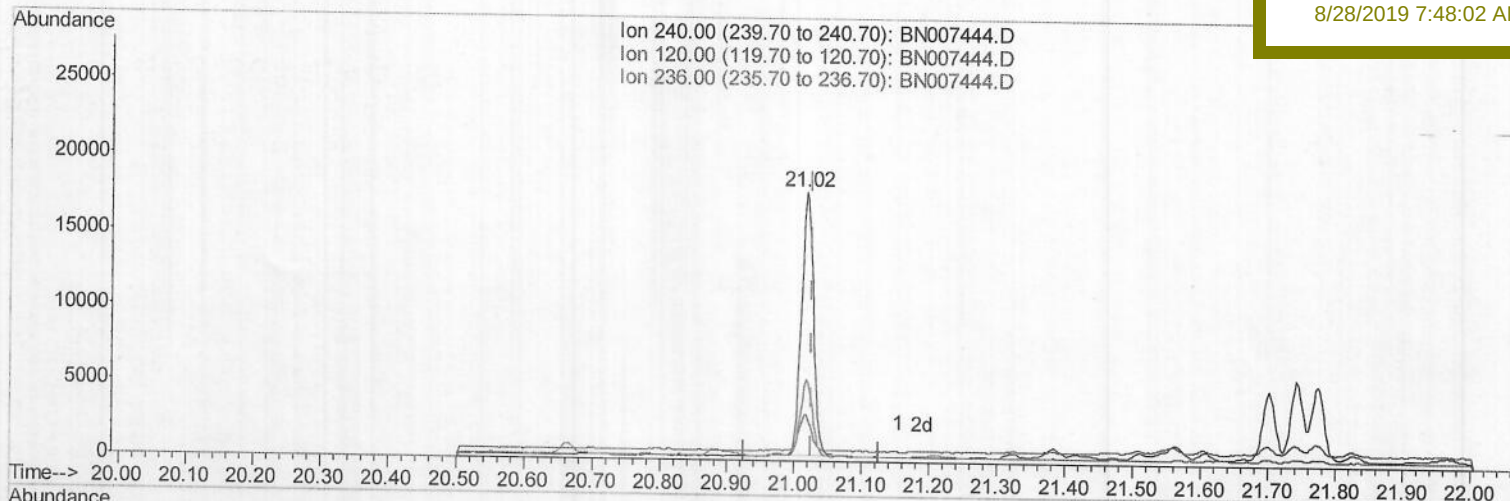
C0AF6

Manual Integrations

APPROVED

mohammad

8/28/2019 7:48:02 AM



(16) Chrysene-d12 (I)

21.017min (-0.009) 0.40ng/ul m

response 21639

JU
08/28/19

Ion	Exp%	Act%
240.00	100	100
120.00	15.00	17.35
236.00	28.60	30.33
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:19:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

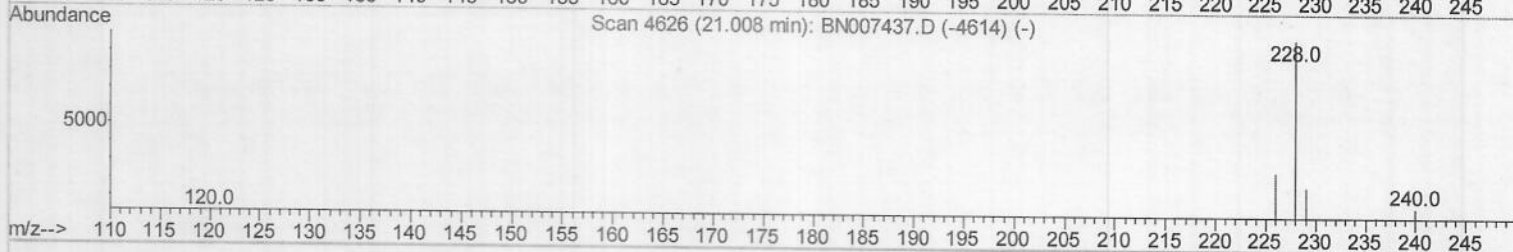
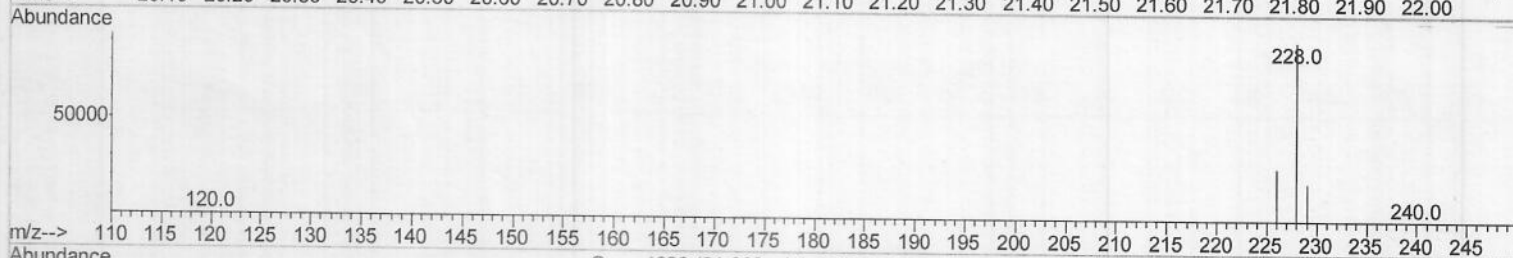
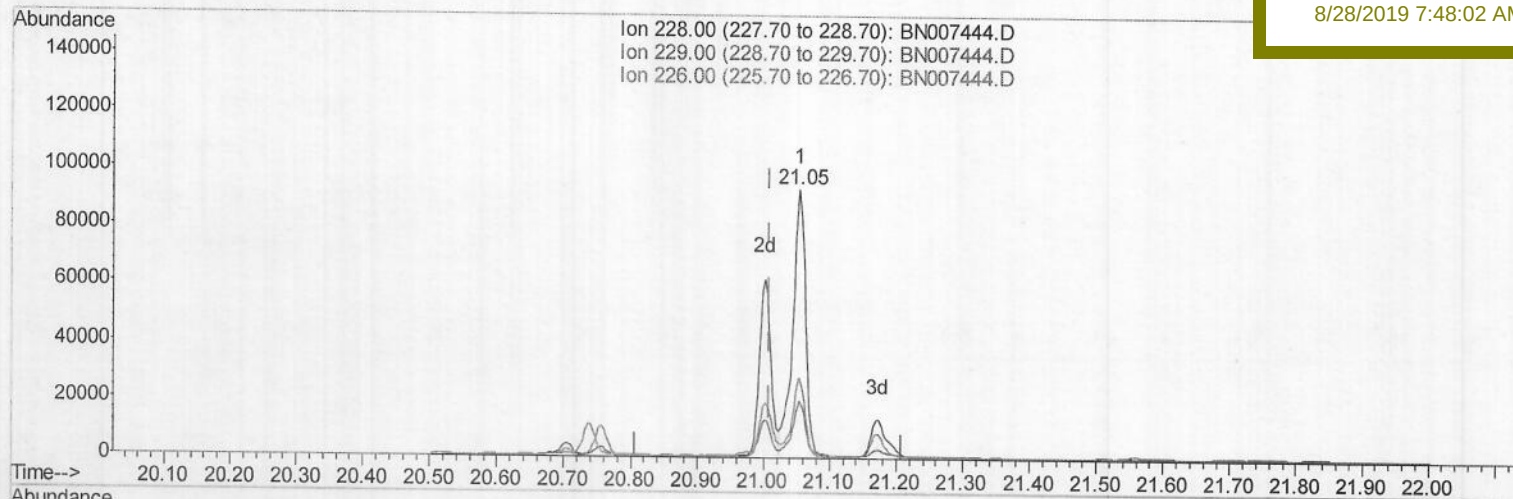
C0AF6

Manual Integrations

APPROVED

mohammad

8/28/2019 7:48:02 AM



(18) Benzo(a)anthracene

21.055min (+0.047) 1.30ng/ul

response 125752

Ion	Exp%	Act%
228.00	100	100
229.00	19.30	21.48
226.00	27.50	29.89
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:19:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

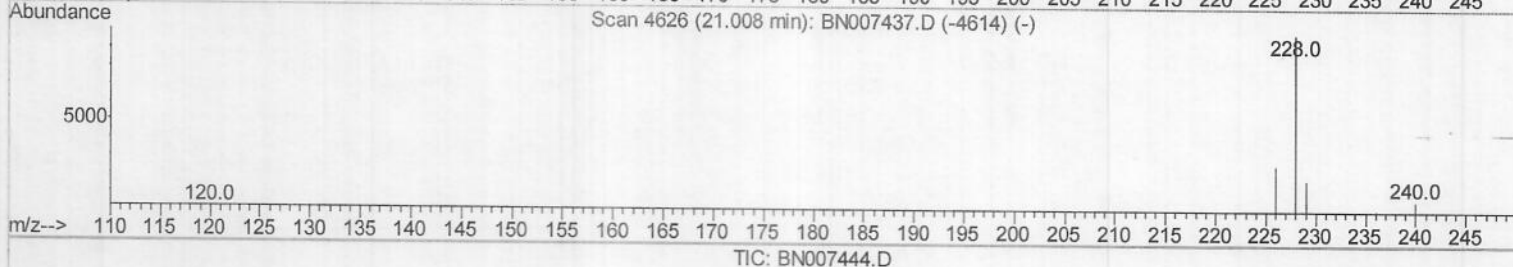
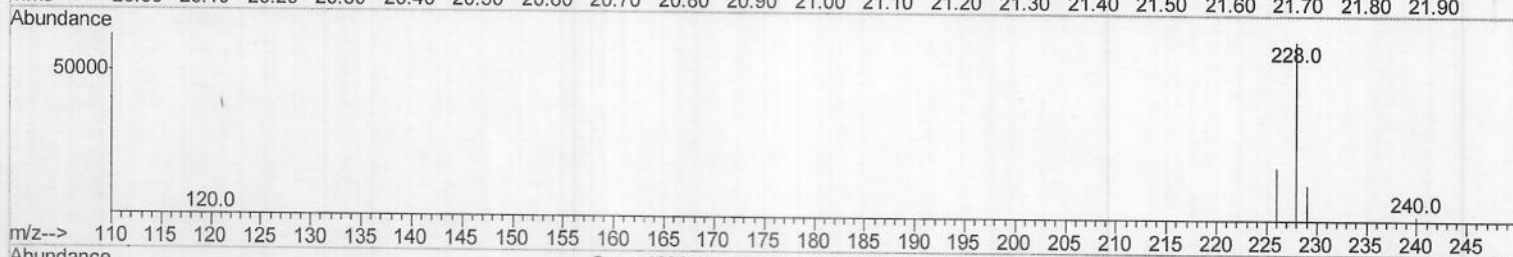
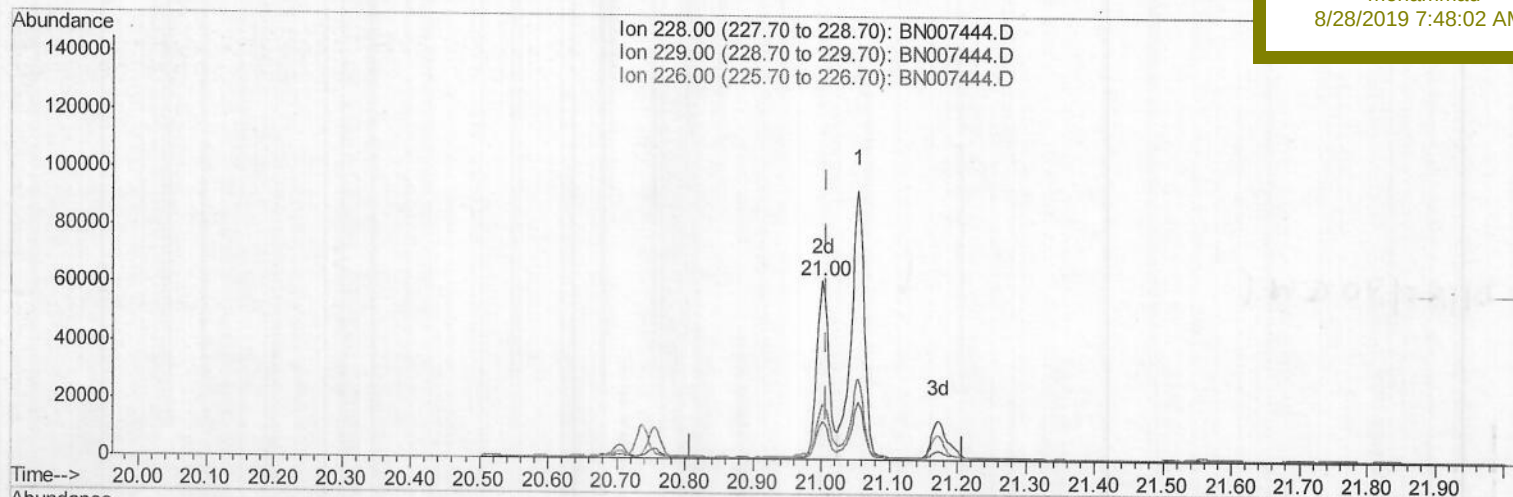
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(18) Benzo(a)anthracene

21.002min (-0.006) 0.78ng/ul m

response 75282

Ion	Exp%	Act%
228.00	100	100
229.00	19.30	21.44
226.00	27.50	30.70
0.00	0.00	0.00

JU
08/28/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:19:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

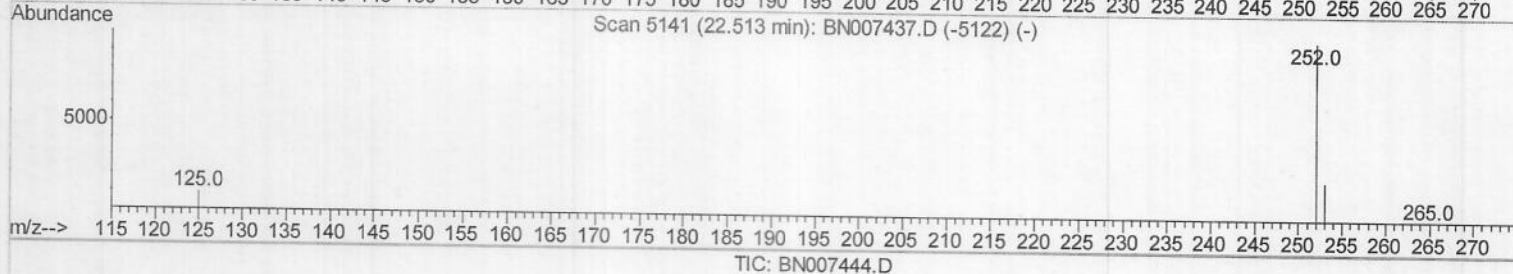
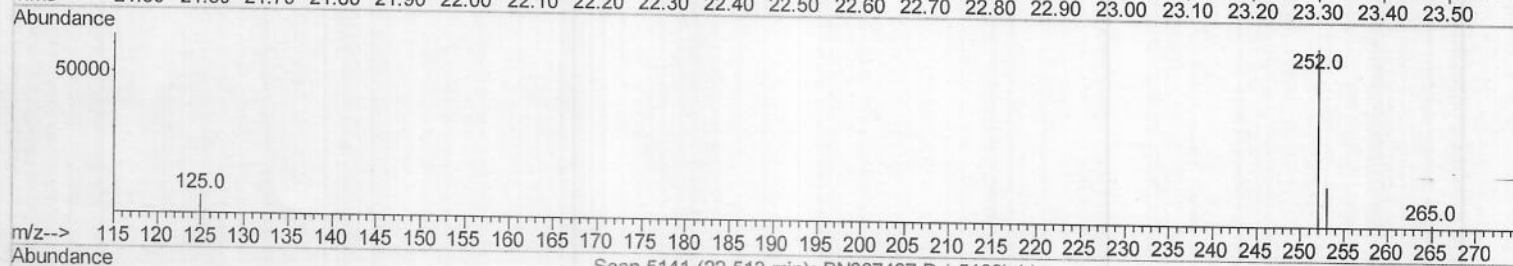
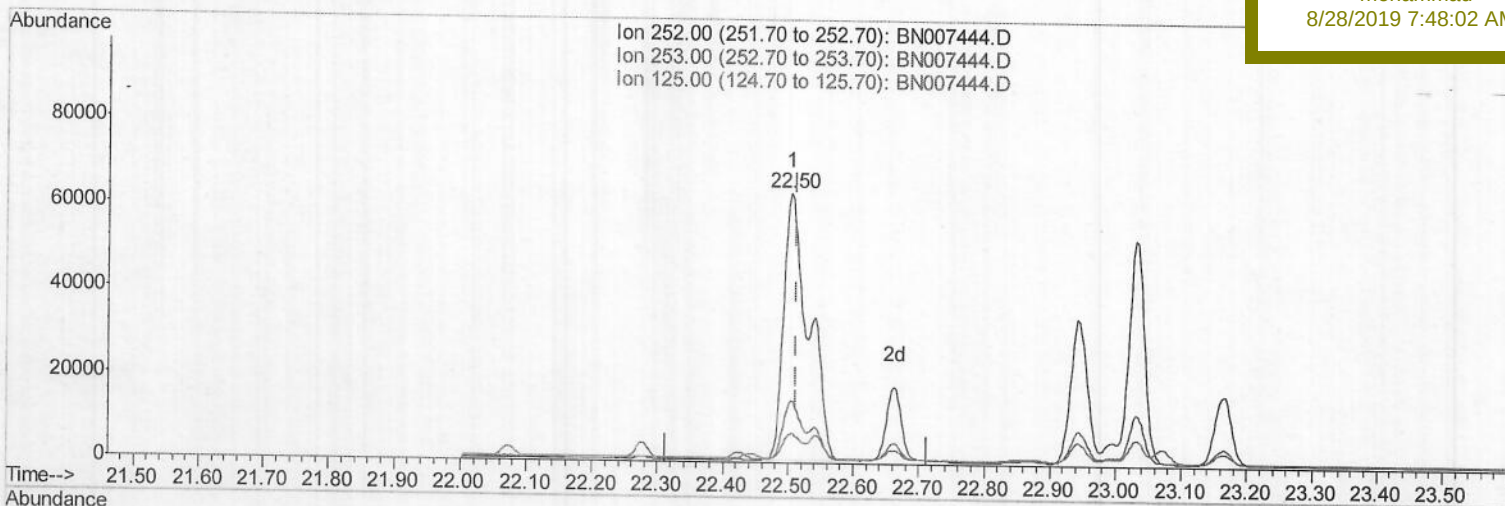
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(21) Benzo(b)fluoranthene

22.504min (-0.009) 1.47ng/ul

response 168525

Ion	Exp%	Act%
252.00	100	100
253.00	23.50	23.10
125.00	12.40	10.76
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:19:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

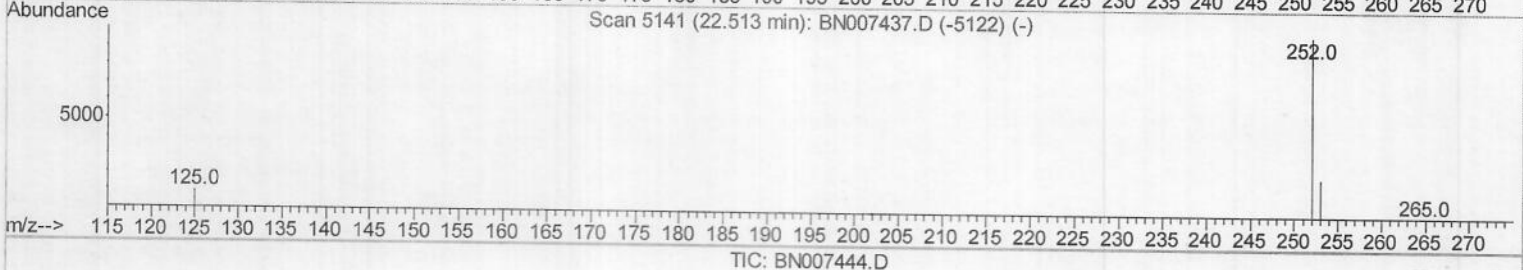
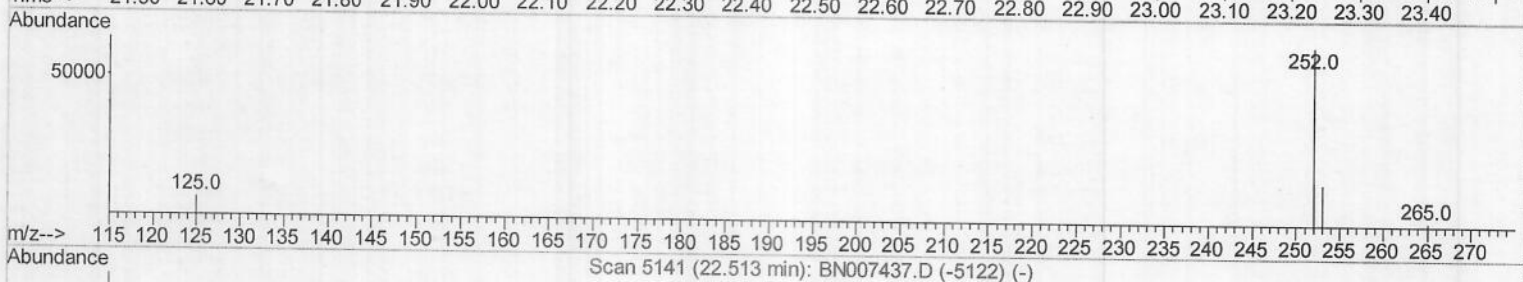
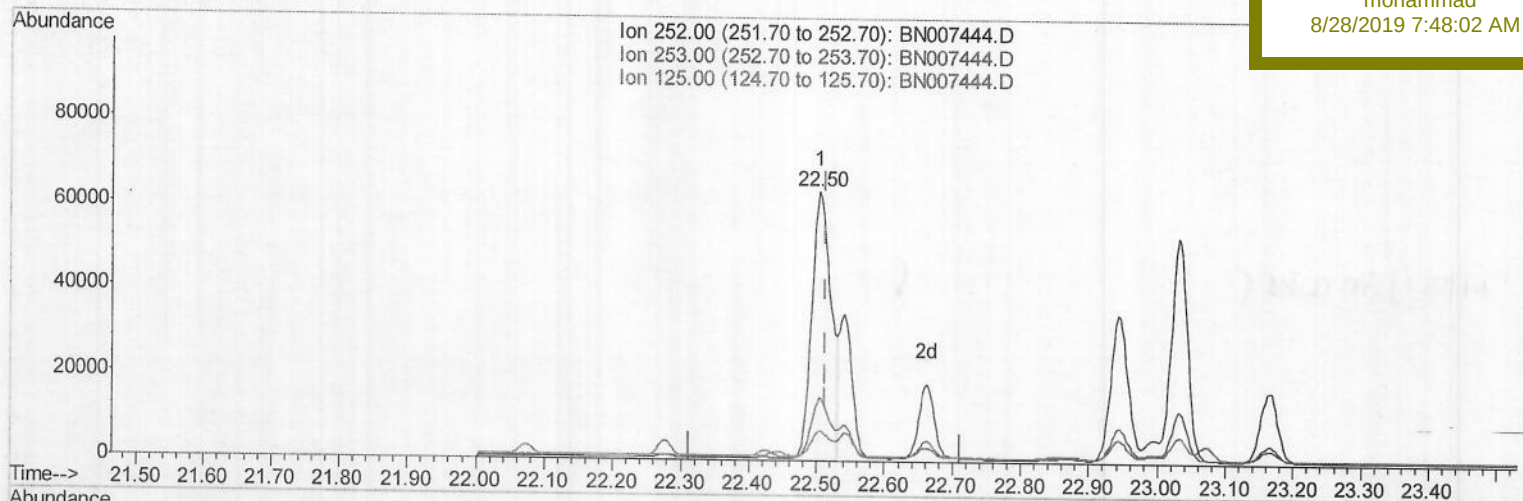
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

(21) Benzo(b)fluoranthene

22.504min (-0.009) 1.09ng/ul m) JU

response 124155

08/28/19

Ion	Exp%	Act%
252.00	100	100
253.00	23.50	23.10
125.00	12.40	10.76
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:19:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

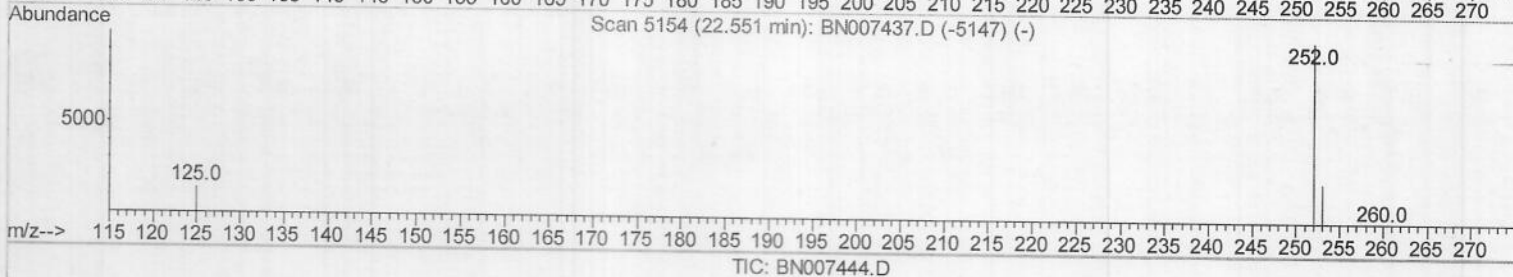
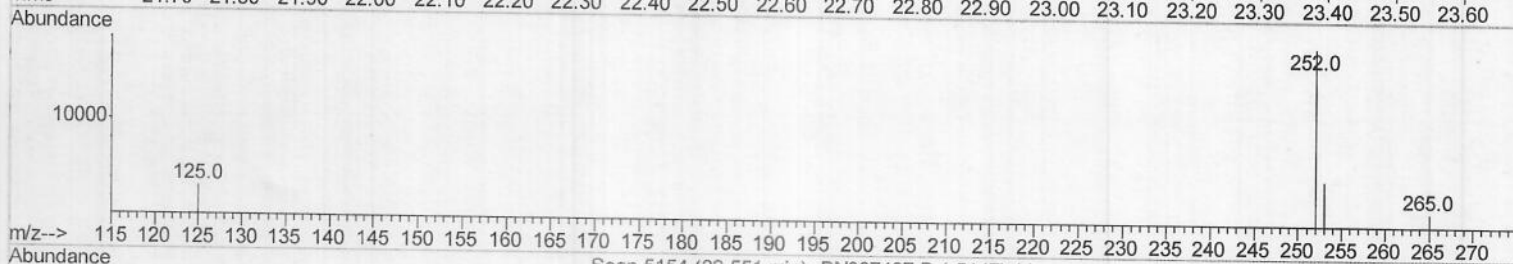
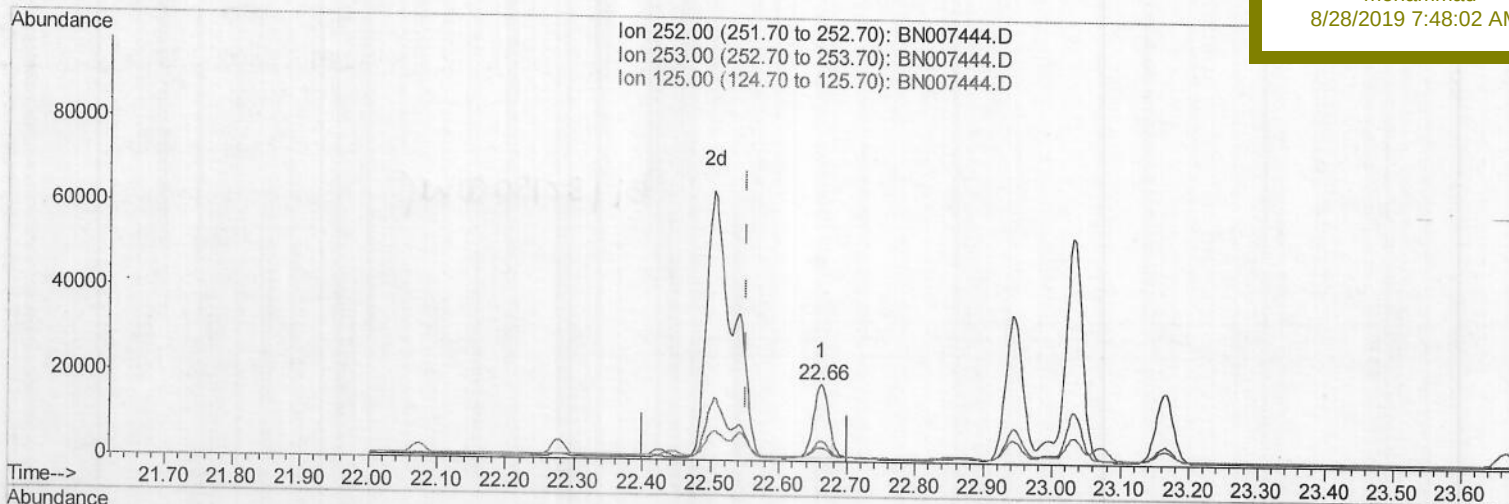
C0AF6

Manual Integrations

APPROVED

mohammad

8/28/2019 7:48:02 AM



(22) Benzo(k)fluoranthene

22.662min (+0.111) 0.22ng/ul

response 26324

Ion	Exp%	Act%
252.00	100	100
253.00	23.40	26.49
125.00	15.50	17.91
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:19:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

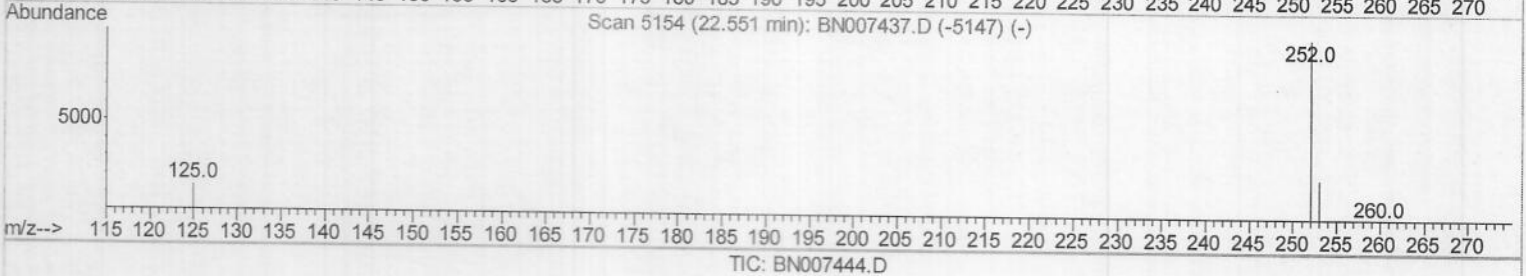
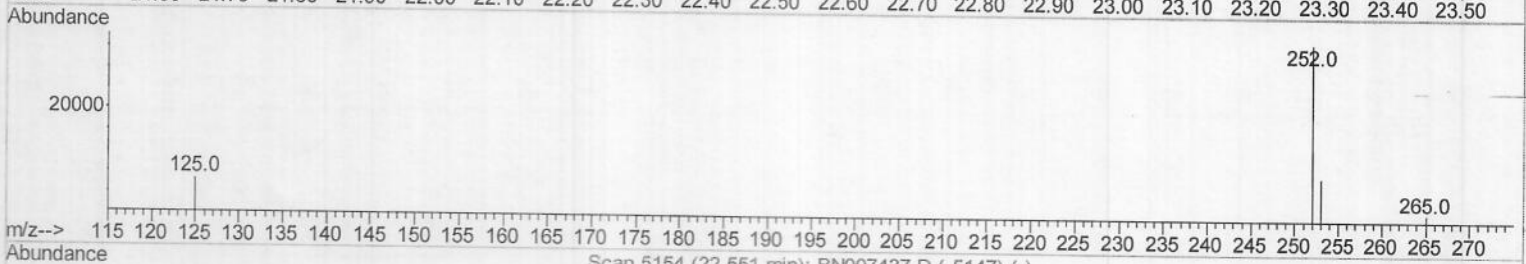
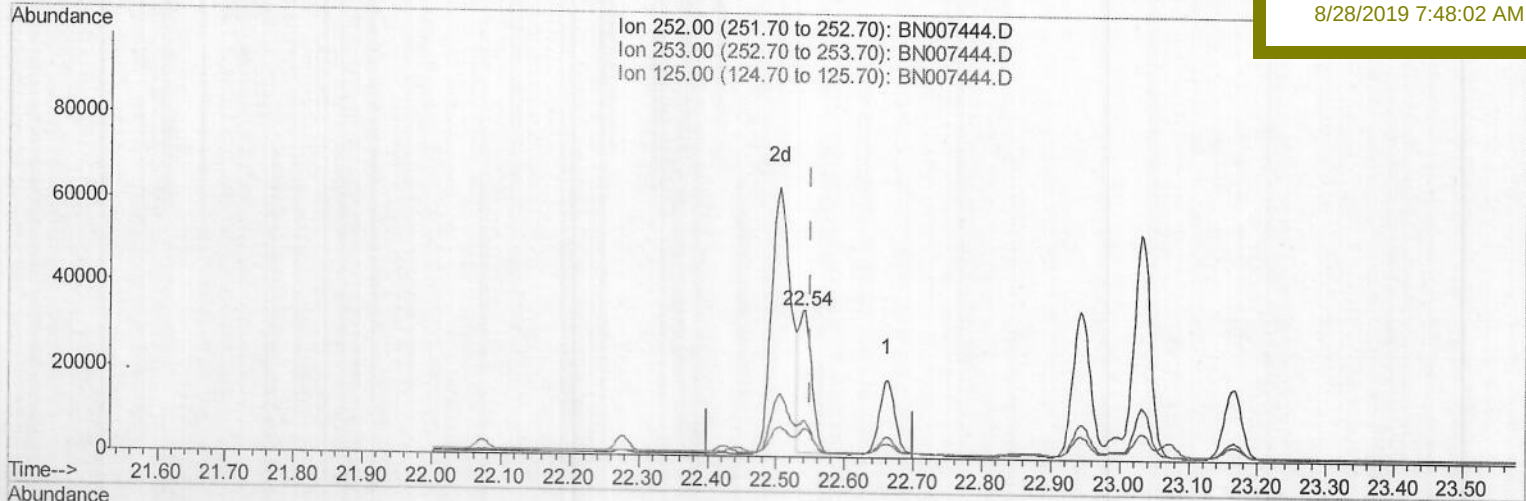
C0AF6

Manual Integrations

APPROVED

mohammad

8/28/2019 7:48:02 AM



(22) Benzo(k)fluoranthene

22.542min (-0.009) 0.36ng/ul m

response 42990

Ion Exp% Act%

252.00 100 100

253.00 23.40 24.36

125.00 15.50 19.38#

0.00 0.00 0.00

JU
08/28/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082819\

Data File : BN007444.D

Acq On : 27 Aug 2019 22:29

Operator : HP/JU

Sample : K4337-14

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 28 00:21:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 27 20:30:31 2019

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :

C0AF6

Manual Integrations
APPROVEDmohammad
8/28/2019 7:48:02 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	5319	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	22561	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	13214	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.80	188	26480m	0.40	ng/ul	0.00
16) Chrysene-d12	21.02	240	21639m	0.40	ng/ul	0.00
20) Perylene-d12	23.12	264	26158	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.76	152	14951	0.43	ng/ul	0.00
14) Fluoranthene-d10	18.84	212	35984m	0.42	ng/ul	0.00

Target Compounds

					Ovalue	
3) Naphthalene	10.20	128	1033866	16.227	ng/ul	99
5) 2-Methylnaphthalene	11.83	142	11722	0.274	ng/ul	100
7) Acenaphthylene	13.76	152	37538	0.511	ng/ul#	94
8) Acenaphthene	14.11	153	1419262	26.865	ng/ul	97
9) Fluorene	15.11	166	890153	15.572	ng/ul	97
11) Pentachlorophenol	16.46	266	694m	0.116	ng/ul	
12) Phenanthrene	16.84	178	226440m	2.740	ng/ul	
13) Anthracene	16.93	178	107776m	1.384	ng/ul	
15) Fluoranthene	18.87	202	446396m	4.036	ng/ul	
17) Pyrene	19.24	202	269845	2.549	ng/ul	99
18) Benzo(a)anthracene	21.00	228	75282m	0.778	ng/ul	
19) Chrysene	21.05	228	125298	1.206	ng/ul	99
21) Benzo(b)fluoranthene	22.50	252	124155m	1.087	ng/ul	
22) Benzo(k)fluoranthene	22.54	252	42990m	0.360	ng/ul	
23) Benzo(a)pyrene	23.03	252	86688	0.761	ng/ul	96
24) Indeno(1,2,3-cd)pyrene	25.18	276	59233	0.465	ng/ul#	92
25) Dibenzo(a,h)anthracene	25.18	278	12897	0.128	ng/ul#	86
26) Benzo(a,h,i)perylene	25.81	276	56007	0.515	ng/ul	100

(#)= qualifier out of range (m)= manual integration (+)= signals summed