
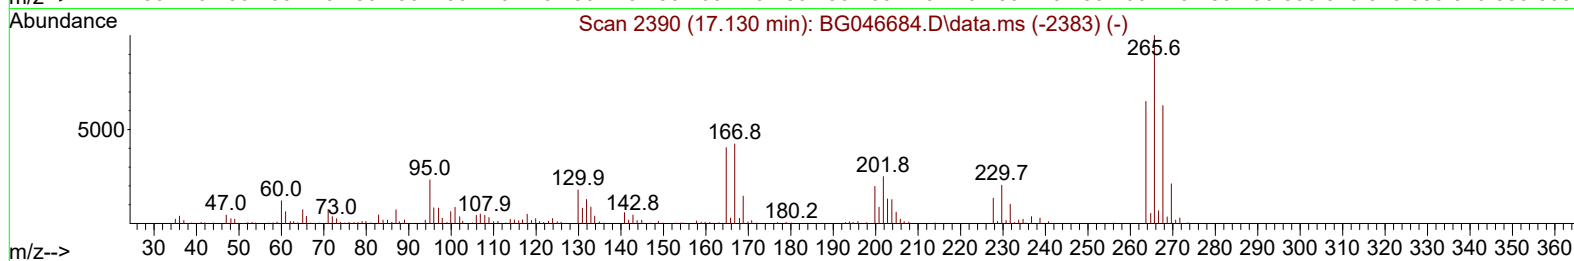
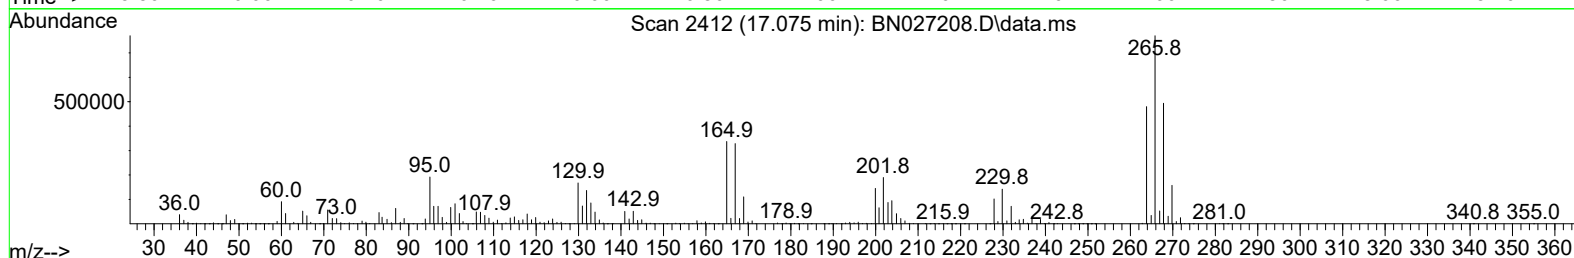


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082823\
Data File : BN027208.D
Acq On : 28 Aug 2023 08:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 03:48:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 03:48:36 2023
Response via : Initial Calibration

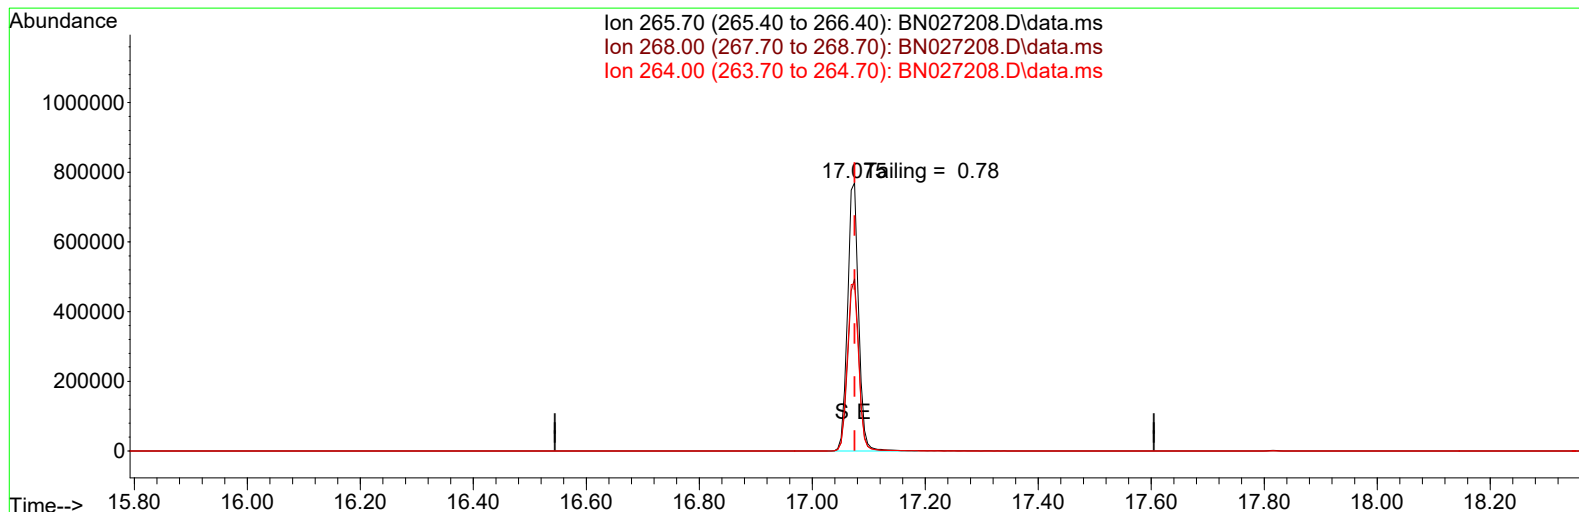

TIC: BN027208.D\data.ms

(70) Pentachlorophenol (C)




17.075min (0.000) 27435.58 ng

response 1047471

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.12
264.00	61.60	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082823\
Data File : BN027208.D
Acq On : 28 Aug 2023 08:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 03:48:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 03:48:36 2023
Response via : Initial Calibration

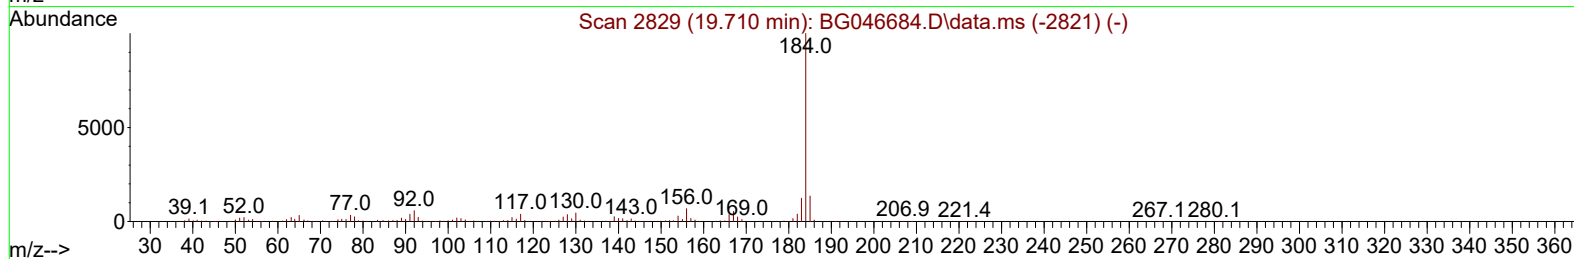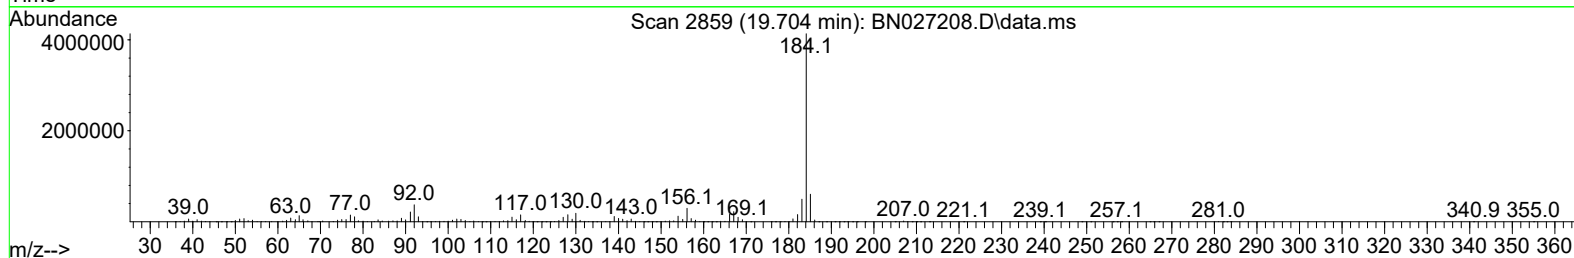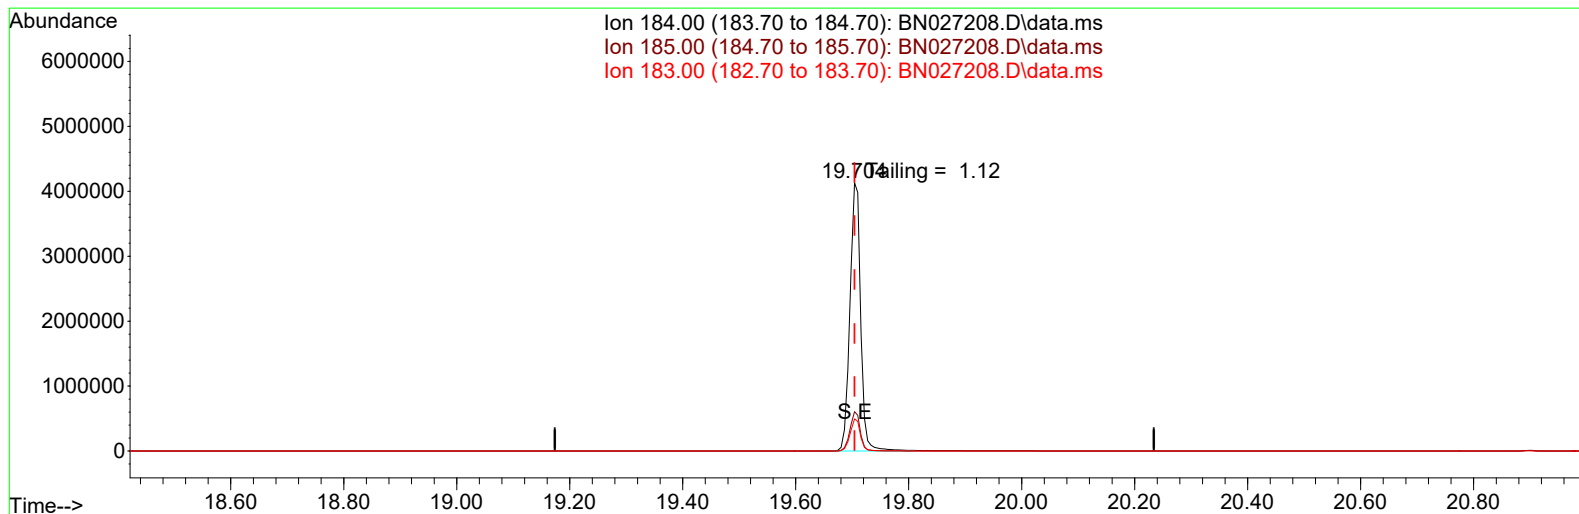

TIC: BN027208.D\data.ms

(77) Benzidine**19.704min (0.000) 212862.32 ng****response 5446095**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	12.03
0.00	0.00	0.00