


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082823\
 Data File : BN027208.D
 Acq On : 28 Aug 2023 08:49
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 29 03:21:06 2023

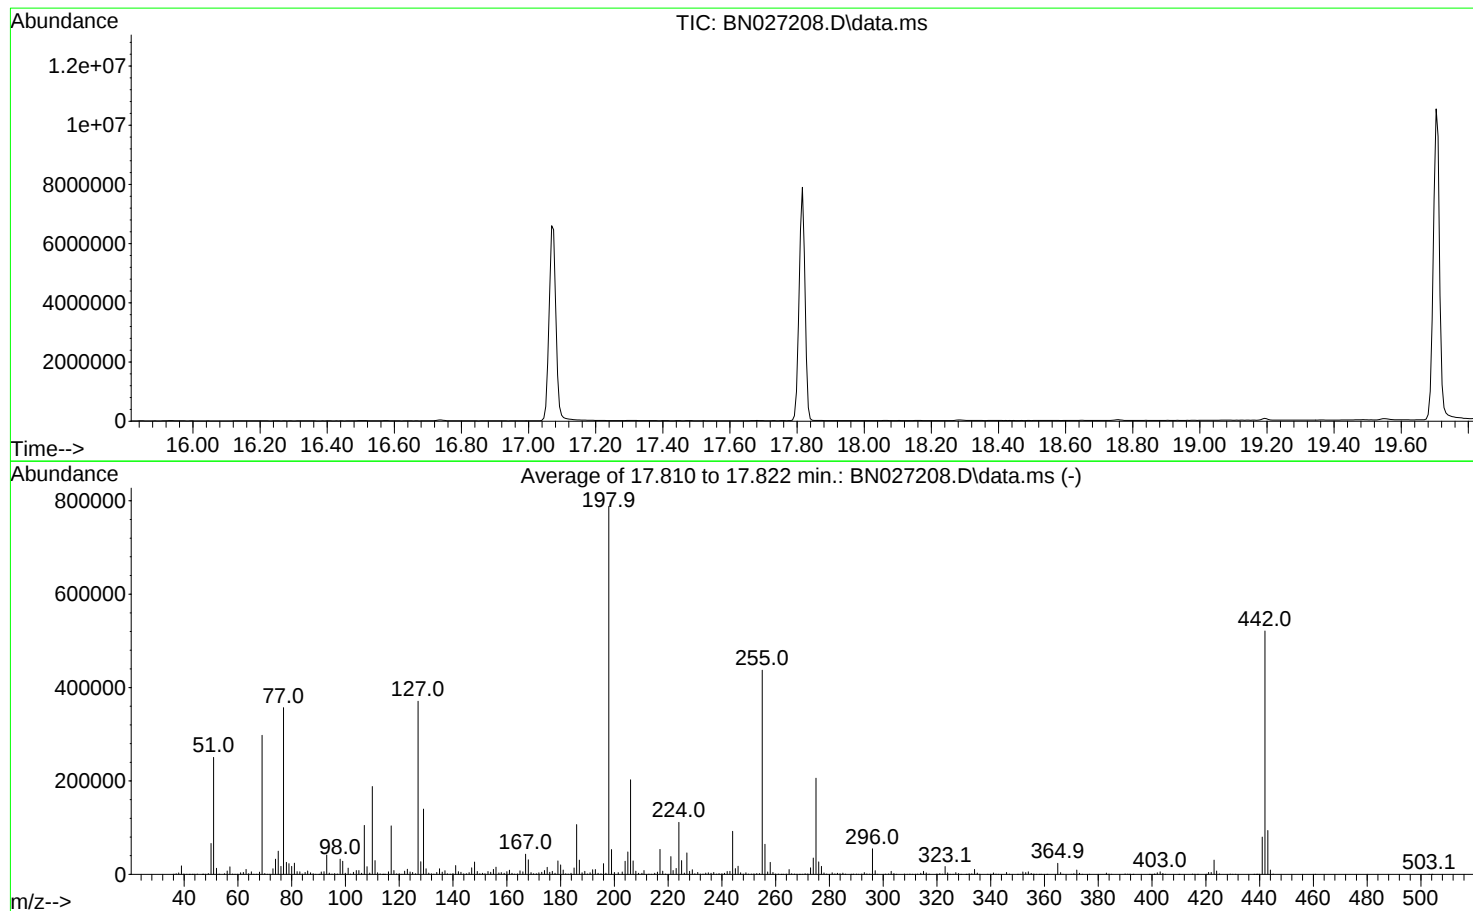




AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	250560	PASS
68	69	0.00	2	1.6	4900	PASS
69	198	0.00	100	37.8	297600	PASS
70	69	0.00	2	0.5	1599	PASS
127	198	10	80	47.1	370624	PASS
197	198	0.00	2	0.3	2453	PASS
198	198	100	100	100.0	787712	PASS
199	198	5	9	6.7	53069	PASS
275	198	10	60	26.1	205867	PASS
365	198	1	100	3.0	23808	PASS
441	198	0.01	100	10.1	79688	PASS
442	442	50	100	100.0	520960	PASS
443	442	15	24	18.0	93768	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082823\
Data File : BN027208.D
Acq On : 28 Aug 2023 08:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 29 03:48:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 03:48:36 2023
Response via : Initial Calibration

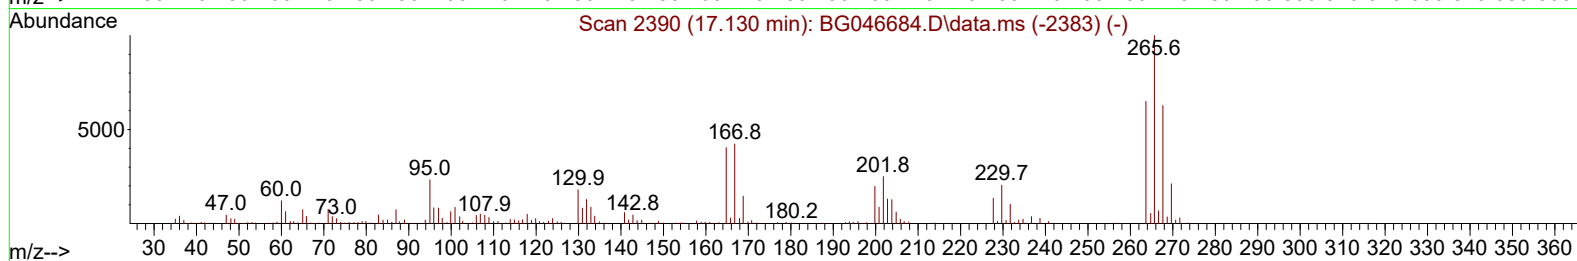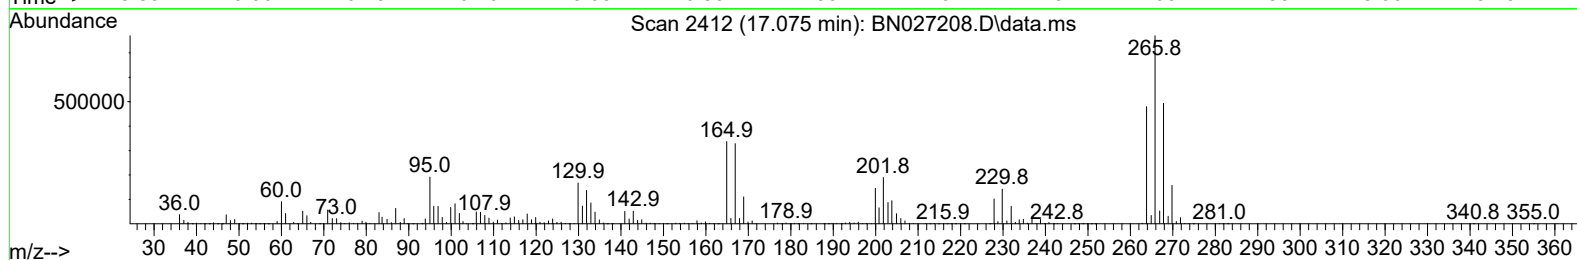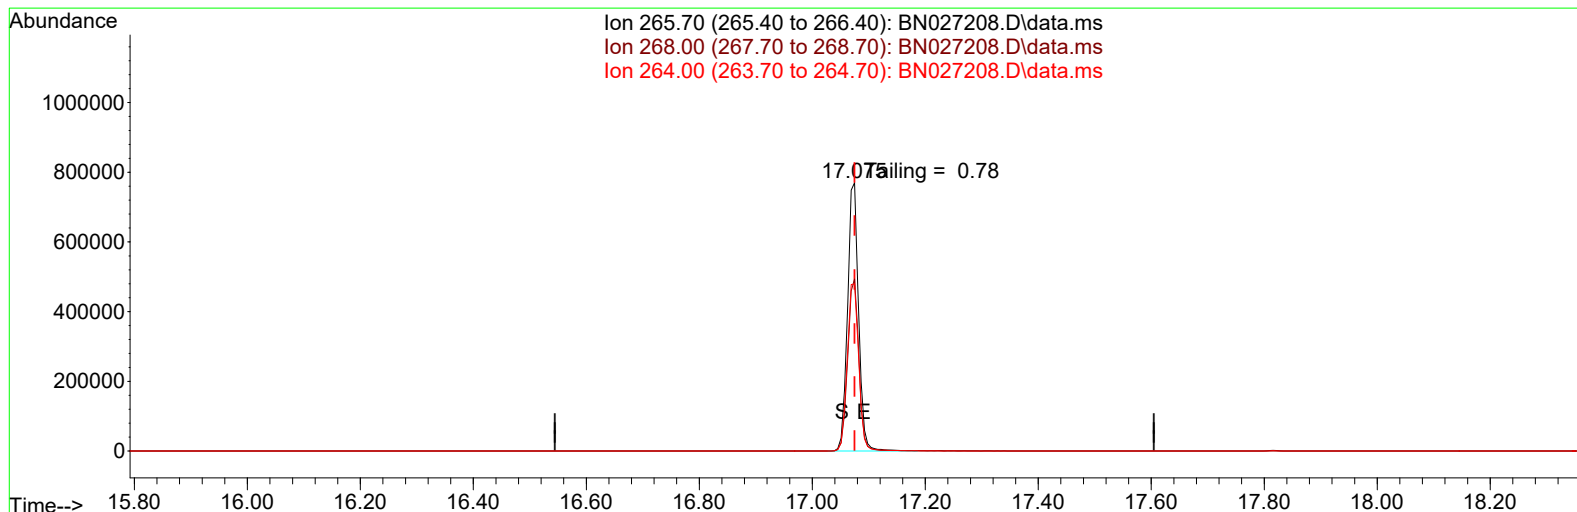

TIC: BN027208.D\data.ms

(70) Pentachlorophenol (C)

17.075min (0.000) 27435.58 ng




response 1047471

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.12
264.00	61.60	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082823\
Data File : BN027208.D
Acq On : 28 Aug 2023 08:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 29 03:48:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 03:48:36 2023
Response via : Initial Calibration

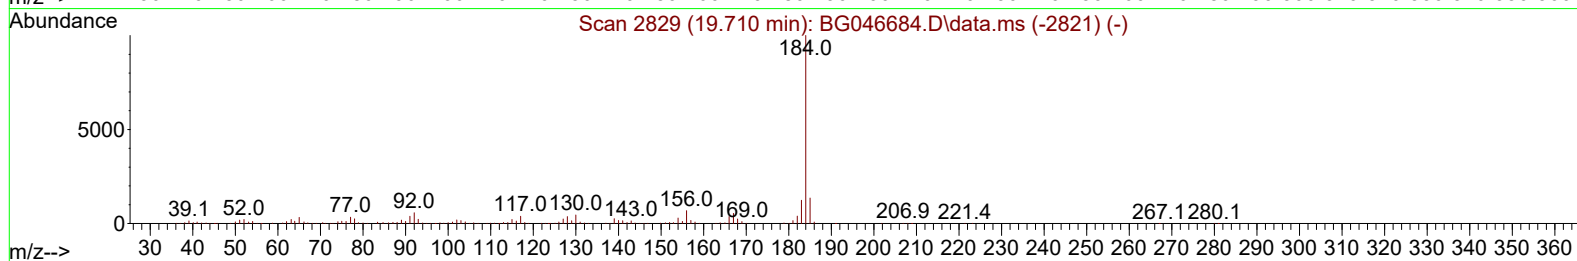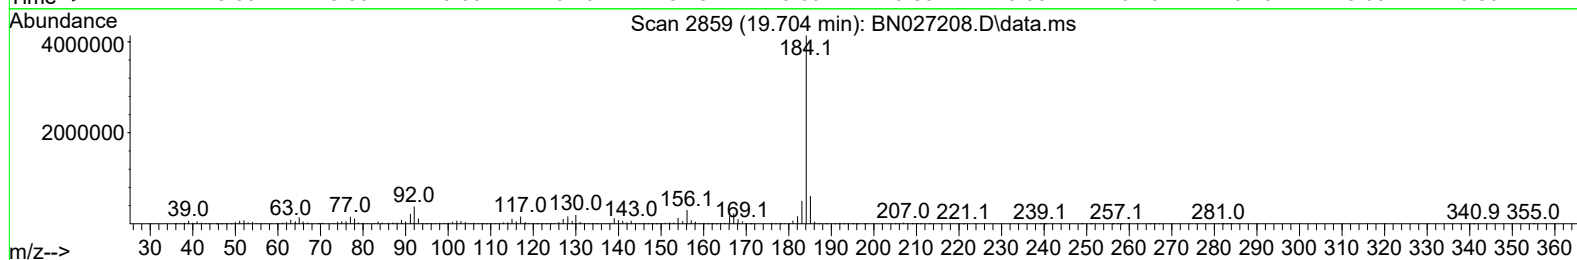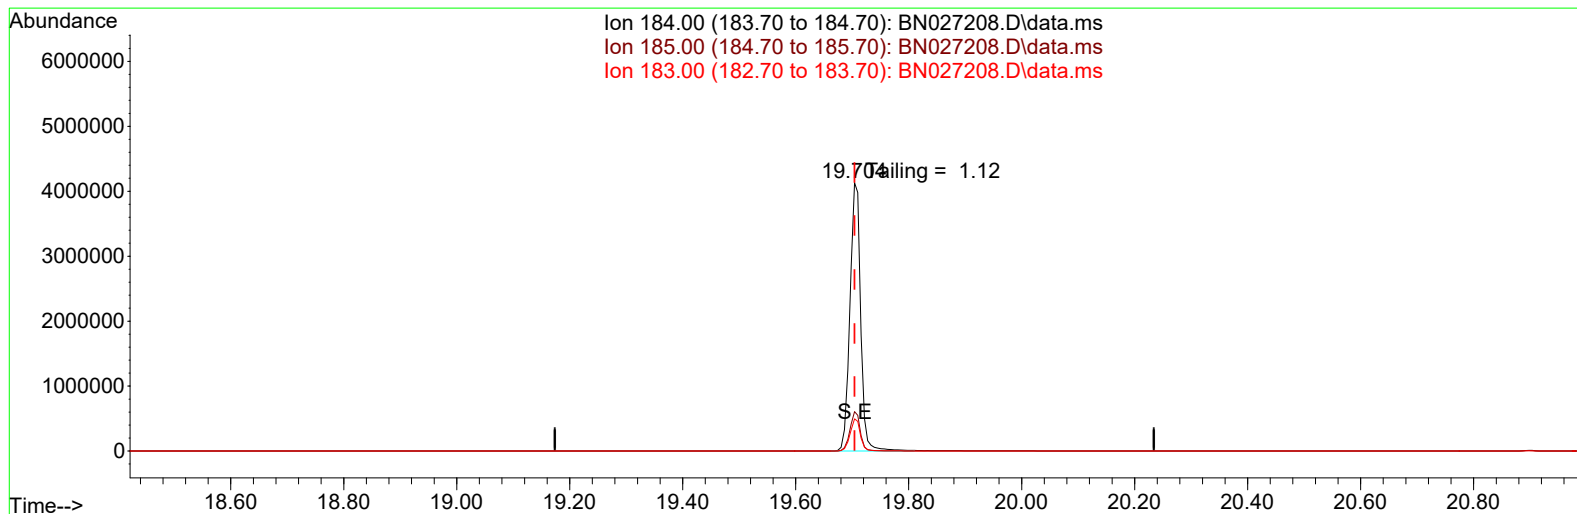

TIC: BN027208.D\data.ms

(77) Benzidine

19.704min (0.000) 212862.32 ng

response 5446095

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/28/2023	BNA_N	<u>BN027208.D</u>
Compound Name	Response	Retention Time
DDT	2737117	20.898
DDD	40642	20.457
DDE	1754	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42396	2779513	1.53

Instrument :
BNA_N
ClientSampleId :
DFTPP