

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
 Data File : BN033641.D
 Acq On : 28 Aug 2024 12:20
 Operator : MA/JU
 Sample : P3711-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E24A0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

Quant Time: Aug 28 15:00:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 27 23:48:09 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.540	152	4711	0.400	ng/u1	0.00
4) Naphthalene-d8	10.299	136	13140	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.174	164	7063	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.927	188	14996m	0.400	ng/u1	0.00
17) Chrysene-d12	21.136	240	11606m	0.400	ng/u1	0.00
23) Perylene-d12	23.301	264	12105m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	27730	5.726	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.894	152	6979	0.370	ng/u1	0.00
18) Fluoranthene-d10	18.966	212	17054	0.493	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.585	266	4202m	0.891	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
Data File : BN033641.D
Acq On : 28 Aug 2024 12:20
Operator : MA/JU
Sample : P3711-08
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E24A0

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024


Quant Time: Aug 28 15:00:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 23:48:09 2024
Response via : Initial Calibration

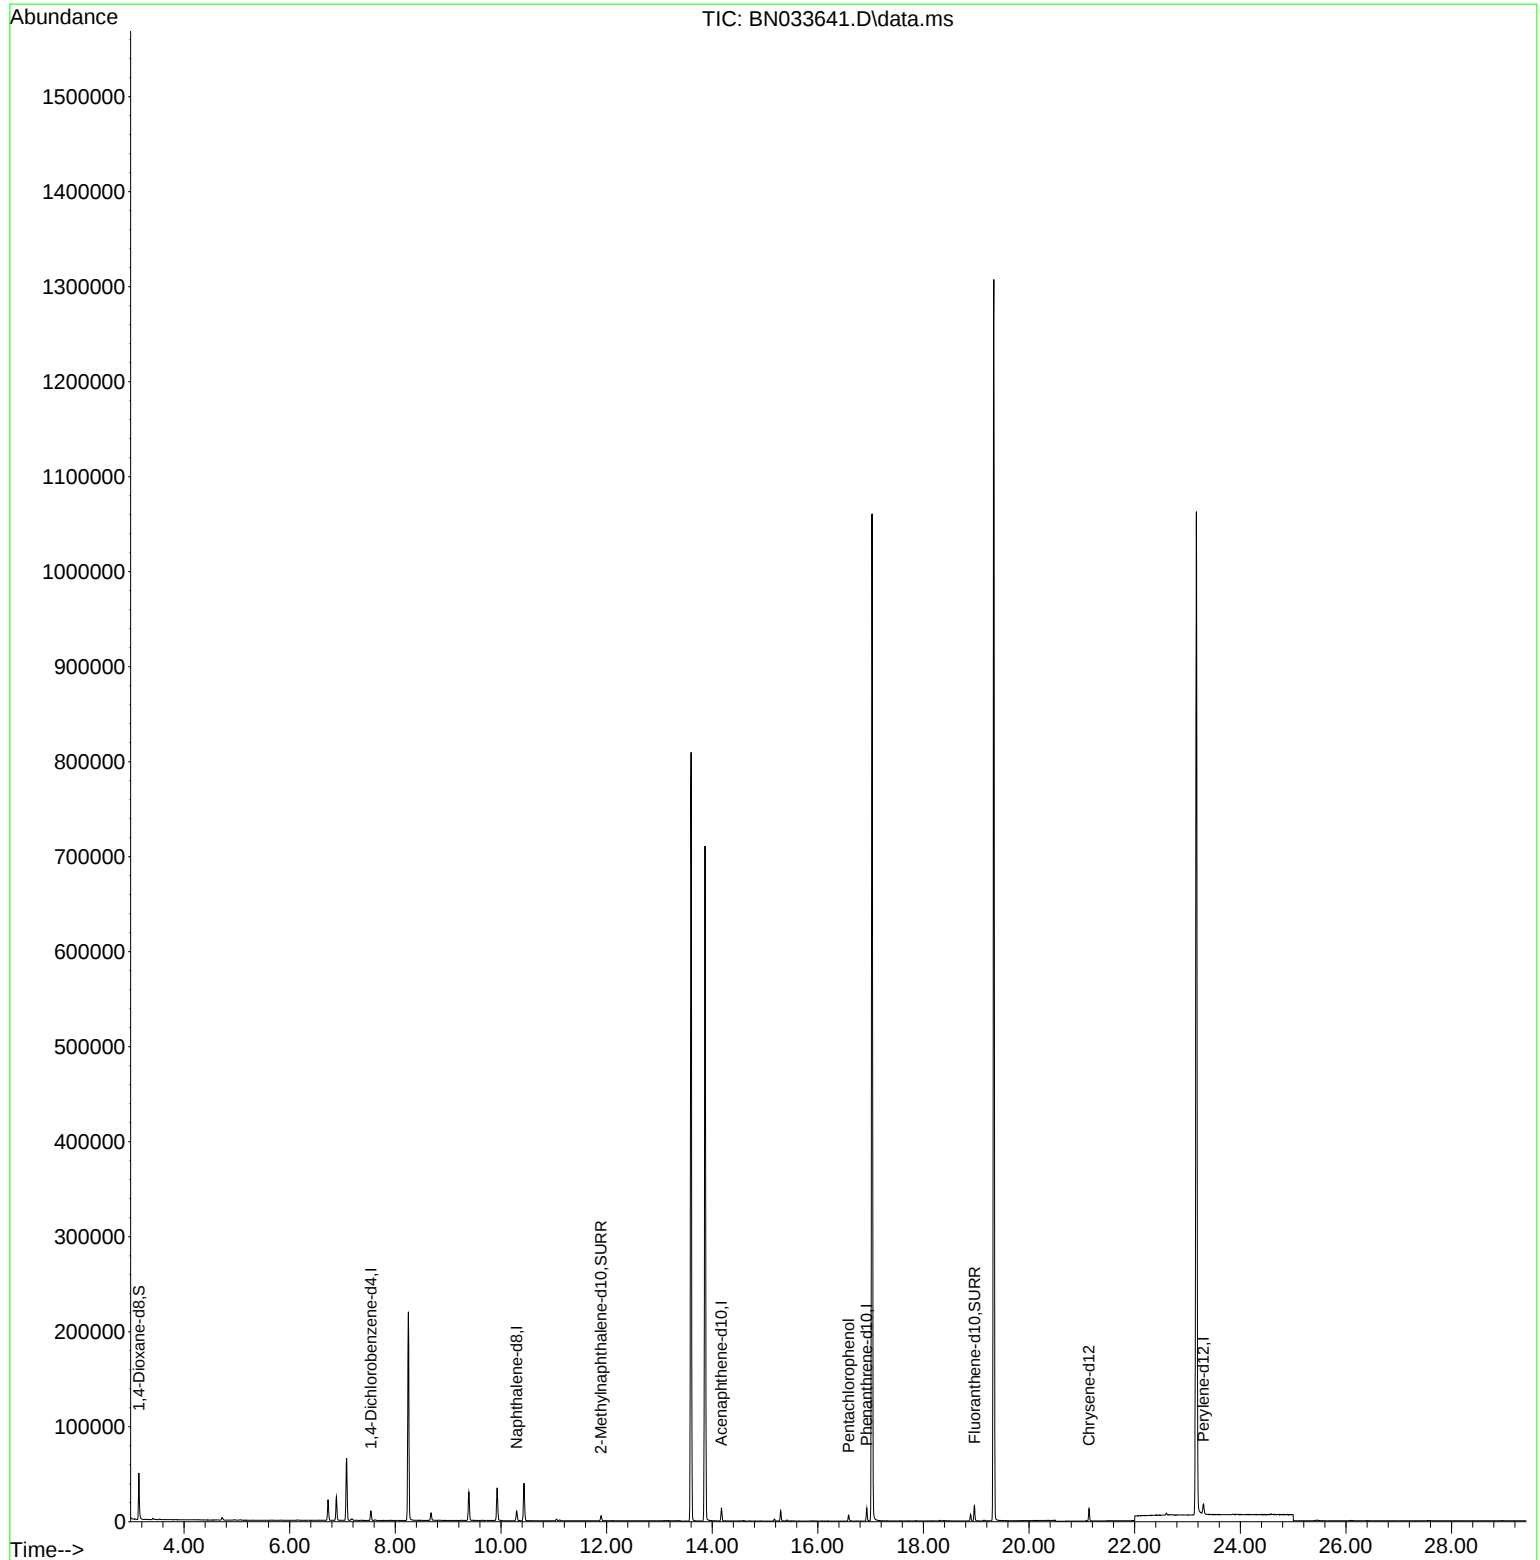

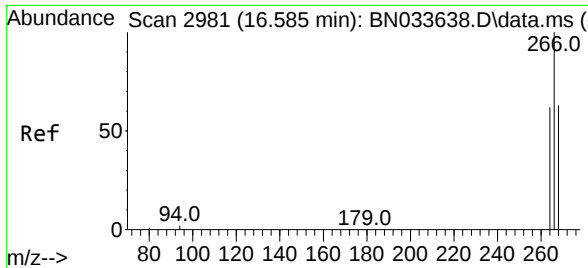

#14
 Pentachlorophenol
 Concen: 0.891 ng/ul m
 RT: 16.585 min Scan# 2981
 Delta R.T. 0.001 min
 Lab File: BN033641.D
 Acq: 28 Aug 2024 12:20

Instrument : BNA_N
 ClientSampleId : E24A0

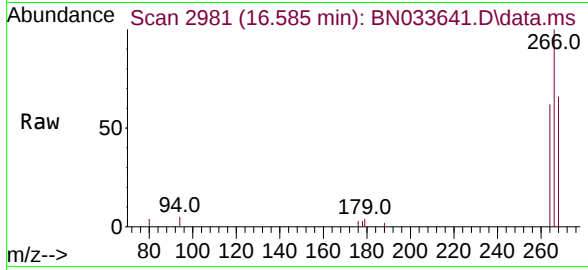

Tgt Ion:	266	Resp:	420
Ion Ratio	Lower	Upper	
266	100		
264	0.0	50.3	75.5
268	0.0	51.7	77.5

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

