

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
 Data File : BN033646.D
 Acq On : 28 Aug 2024 15:21
 Operator : MA/JU
 Sample : P3711-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2499

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

Quant Time: Aug 28 16:25:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 27 23:48:09 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.536	152	4999	0.400	ng/u1	0.00
4) Naphthalene-d8	10.299	136	14176	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.174	164	7952	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.927	188	16685m	0.400	ng/u1	0.00
17) Chrysene-d12	21.138	240	12713m	0.400	ng/u1	0.00
23) Perylene-d12	23.304	264	13468m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	23669	4.605	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.894	152	7182	0.353	ng/u1	0.00
18) Fluoranthene-d10	18.966	212	18639	0.492	ng/u1	0.00
Target Compounds						
14) Pentachlorophenol	16.585	266	957m	0.182	ng/u1	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
Data File : BN033646.D
Acq On : 28 Aug 2024 15:21
Operator : MA/JU
Sample : P3711-07
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2499

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024


Quant Time: Aug 28 16:25:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 23:48:09 2024
Response via : Initial Calibration

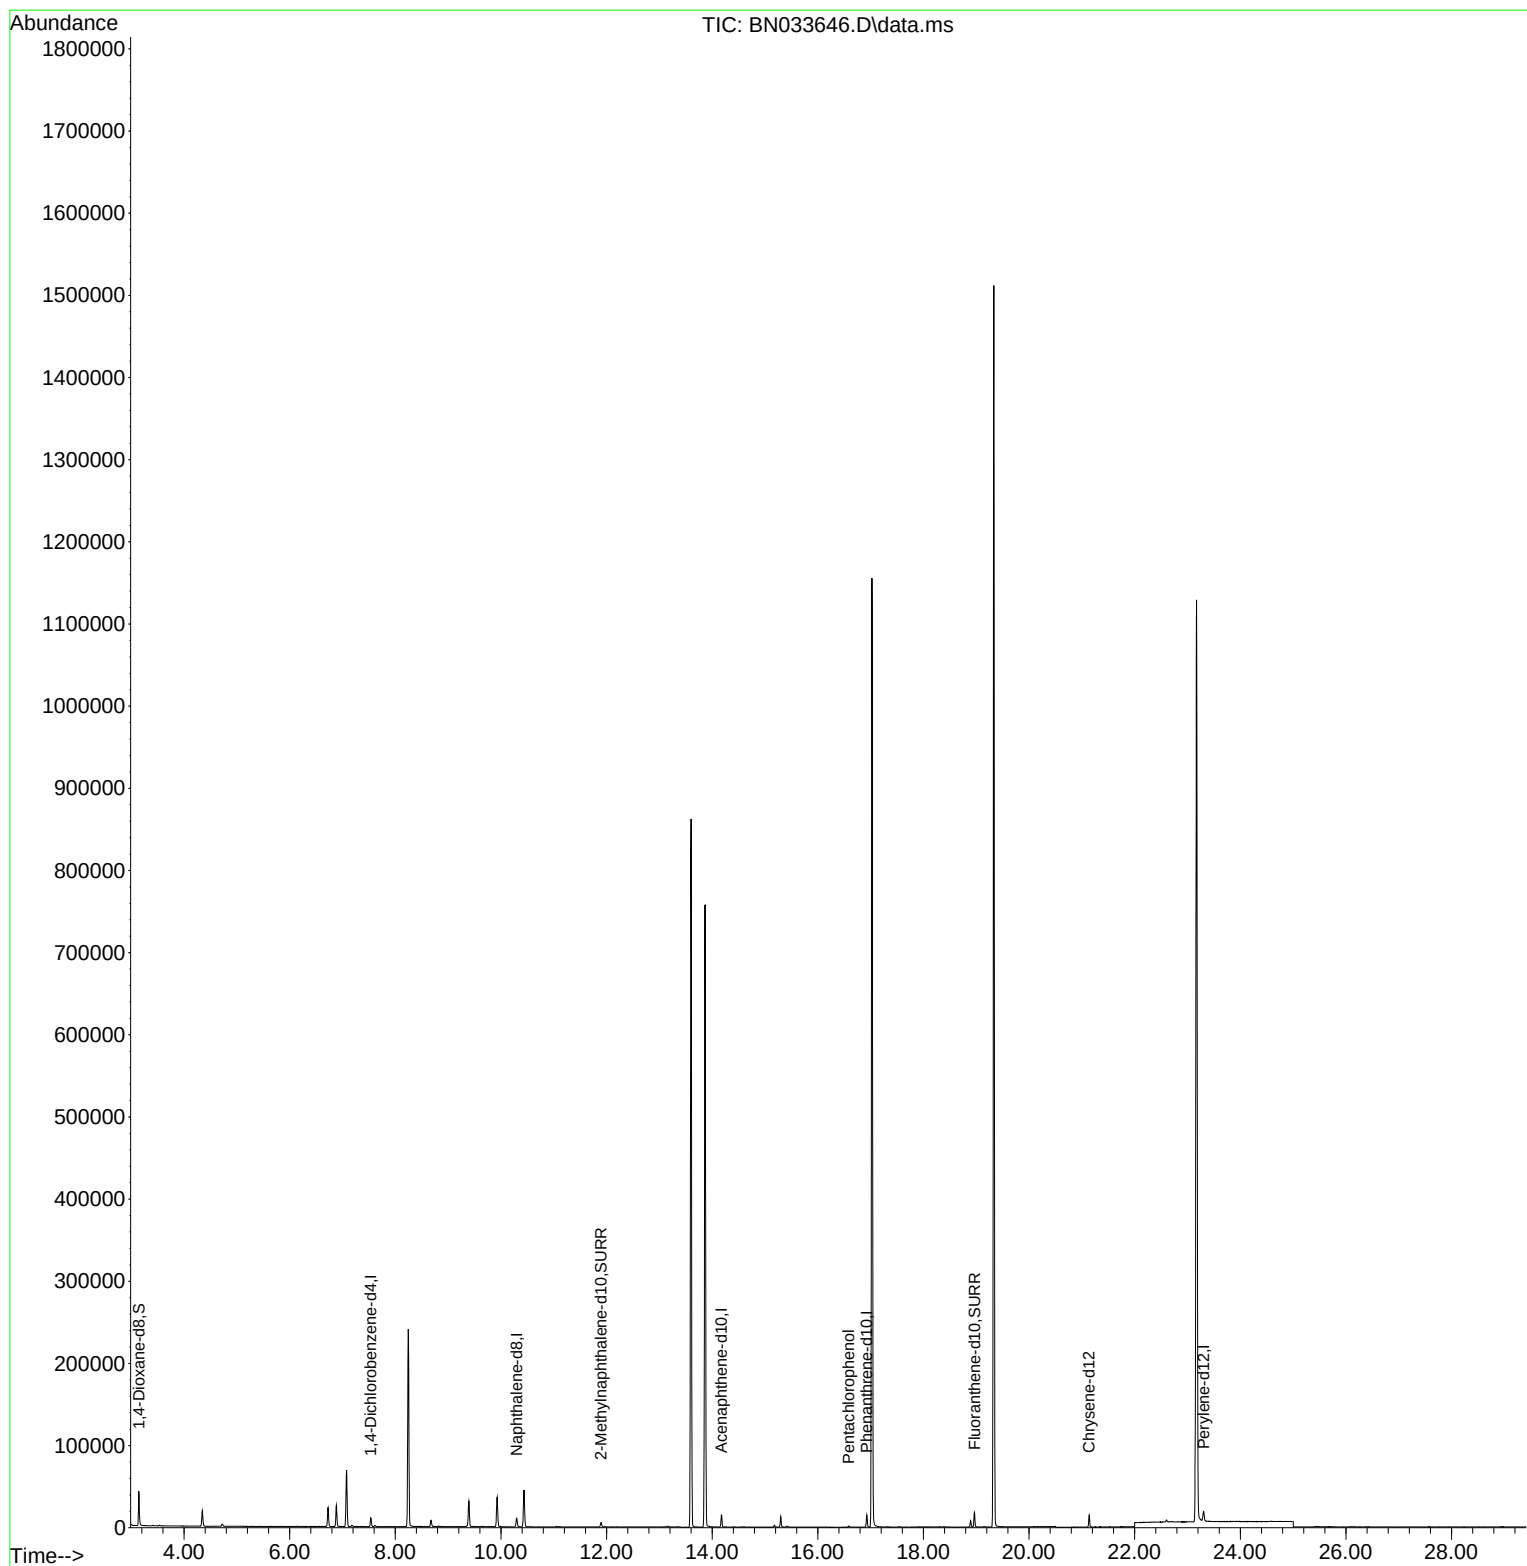

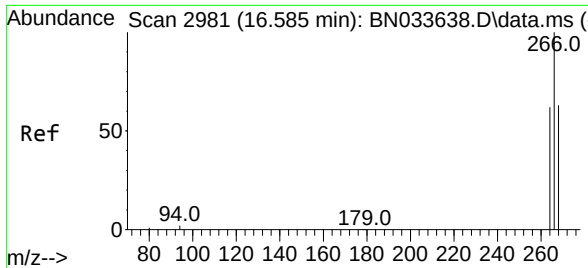

#14
Pentachlorophenol
Concen: 0.182 ng/ul m
RT: 16.585 min Scan# 2981
Delta R.T. 0.001 min
Lab File: BN033646.D
Acq: 28 Aug 2024 15:21

Instrument :
BNA_N
ClientSampleId :
E2499

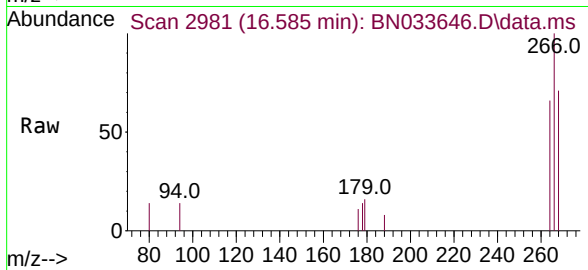

Tgt Ion:266 Resp: 95
Ion Ratio Lower Upper
266 100
264 0.0 50.3 75.5
268 0.0 51.7 77.5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

