

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
 Data File : BN033648.D
 Acq On : 28 Aug 2024 16:33
 Operator : MA/JU
 Sample : P3711-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E24A2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

Quant Time: Aug 28 18:14:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 27 23:48:09 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.536	152	5311	0.400	ng/ul	0.00
4) Naphthalene-d8	10.299	136	15040	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.174	164	8109	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.927	188	17213m	0.400	ng/ul	0.00
17) Chrysene-d12	21.141	240	13347m	0.400	ng/ul	0.00
23) Perylene-d12	23.307	264	13788m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	28220	5.168	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.894	152	6919	0.321	ng/ul	0.00
18) Fluoranthene-d10	18.966	212	18679	0.469	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.177	88	1530	0.253	ng/ul#	84
14) Pentachlorophenol	16.581	266	165m	0.030	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
Data File : BN033648.D
Acq On : 28 Aug 2024 16:33
Operator : MA/JU
Sample : P3711-12
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E24A2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024


Quant Time: Aug 28 18:14:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 23:48:09 2024
Response via : Initial Calibration

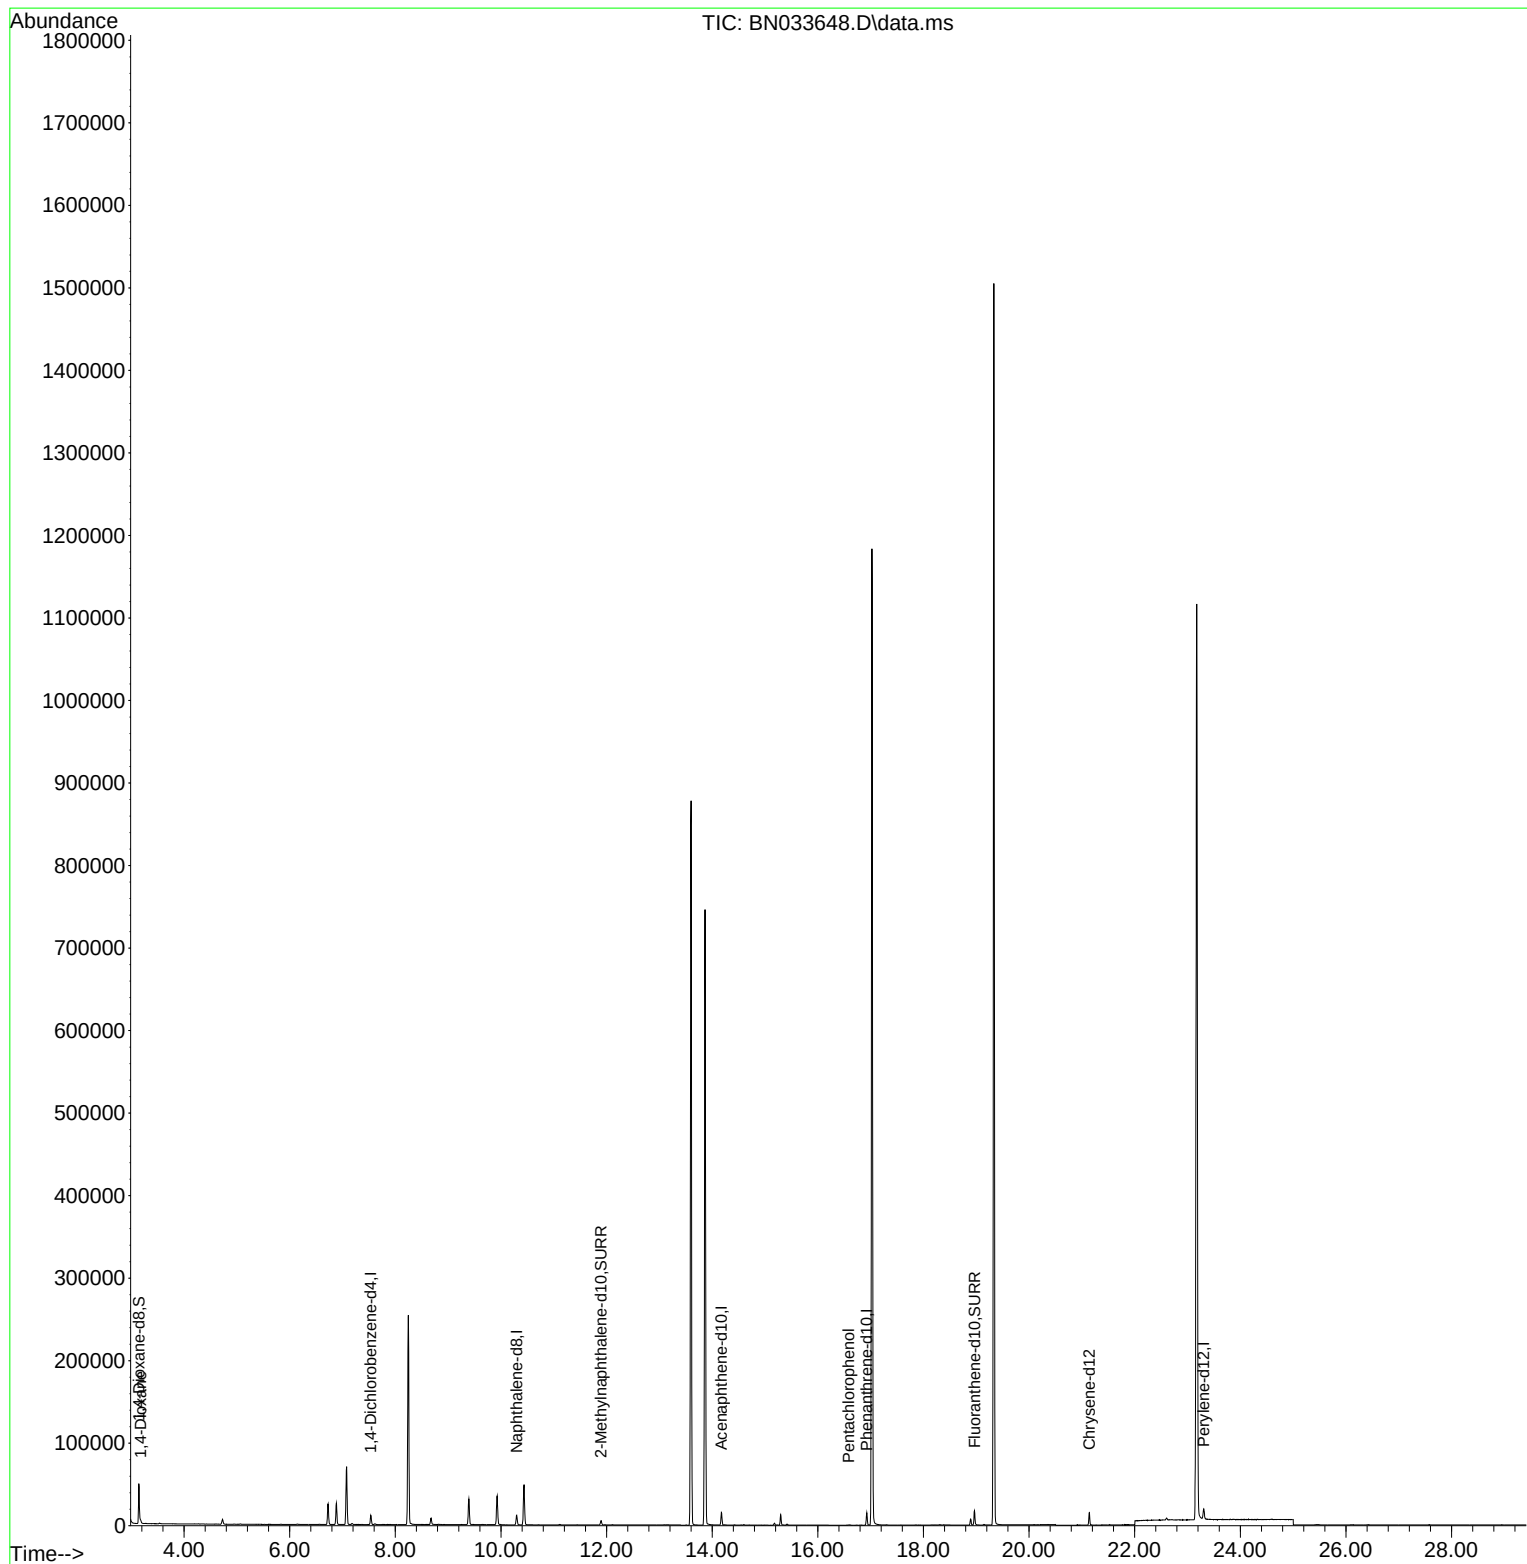

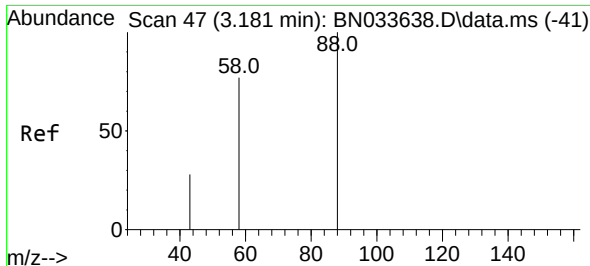

#2
1,4-Dioxane
Concen: 0.253 ng/ul
RT: 3.177 min Scan# 41
Delta R.T. 0.000 min
Lab File: BN033648.D
Acq: 28 Aug 2024 16:33




Instrument :
BNA_N
ClientSampleId :
E24A2

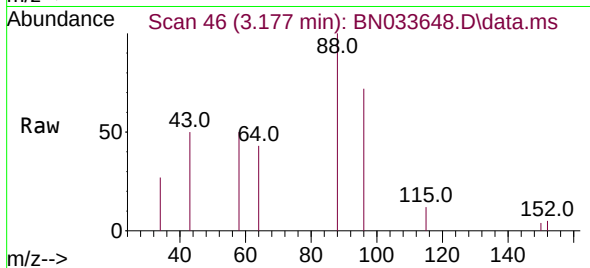


Tgt Ion: 88 Resp: 1530
Ion Ratio Lower Upper
88 100
43 50.4 47.0 70.4
58 50.0 53.0 79.4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

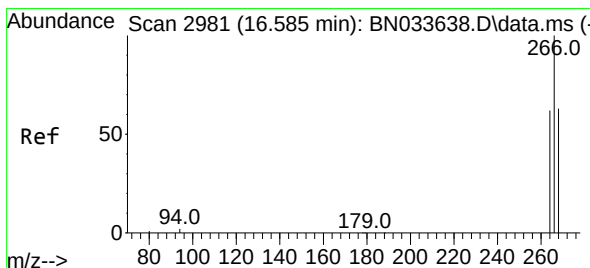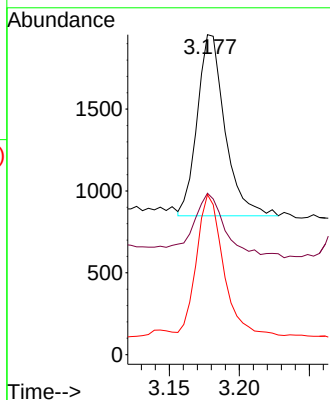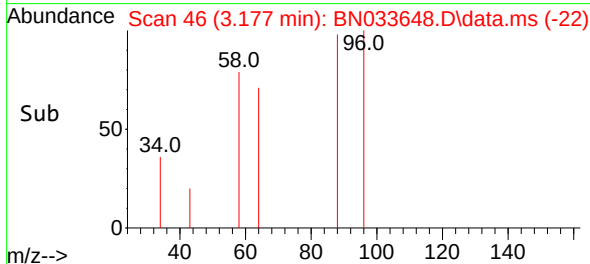

#14
Pentachlorophenol
Concen: 0.030 ng/ul m
RT: 16.581 min Scan# 2980
Delta R.T. -0.003 min
Lab File: BN033648.D
Acq: 28 Aug 2024 16:33

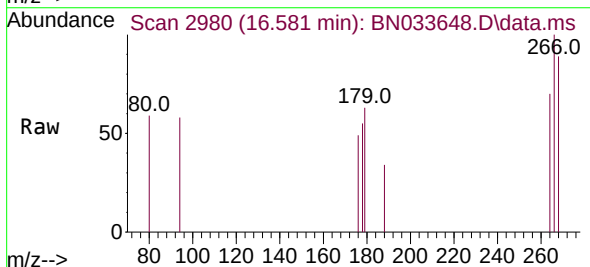

Tgt Ion:266 Resp: 165
Ion Ratio Lower Upper
266 100
264 0.0 50.3 75.5#
268 1.8 51.7 77.5#

