

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
 Data File : BN033649.D
 Acq On : 28 Aug 2024 17:10
 Operator : MA/JU
 Sample : P3711-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2494

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

Quant Time: Aug 28 18:17:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 27 23:48:09 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.536	152	5137	0.400	ng/u1	0.00
4) Naphthalene-d8	10.299	136	14159	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.174	164	7466	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.927	188	15650m	0.400	ng/u1	0.00
17) Chrysene-d12	21.138	240	11811m	0.400	ng/u1	0.00
23) Perylene-d12	23.304	264	12380m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	29462	5.579	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.894	152	7633	0.376	ng/u1	0.00
18) Fluoranthene-d10	18.962	212	17595	0.500	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.581	266	2134m	0.433	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
Data File : BN033649.D
Acq On : 28 Aug 2024 17:10
Operator : MA/JU
Sample : P3711-02
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2494

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024


Quant Time: Aug 28 18:17:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 23:48:09 2024
Response via : Initial Calibration

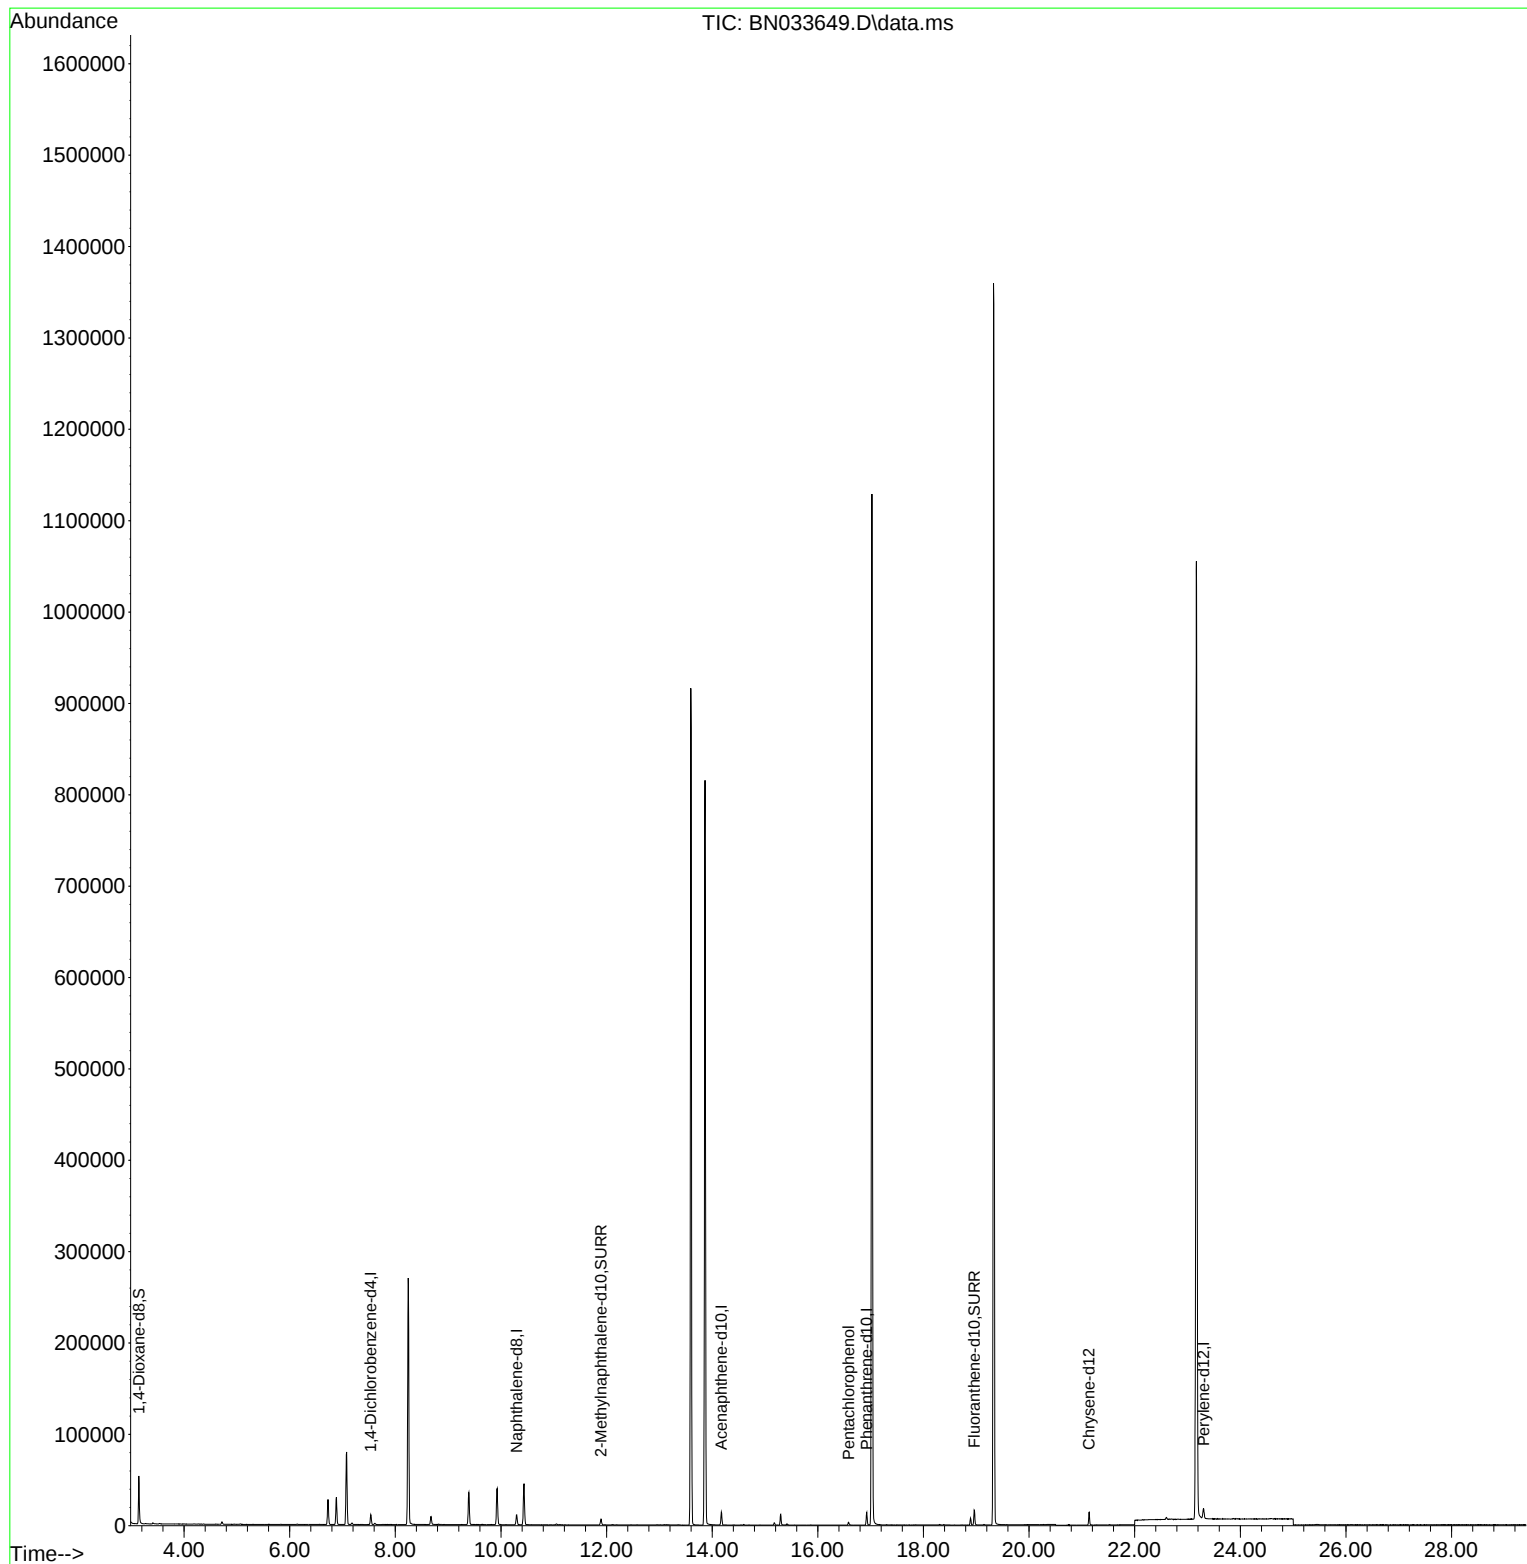

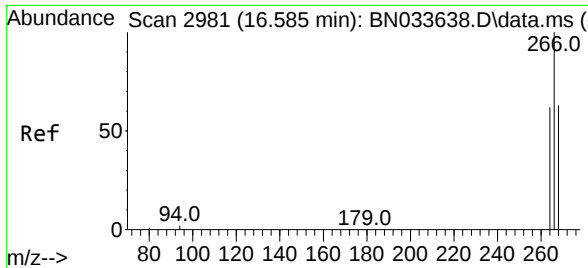

#14
 Pentachlorophenol
 Concen: 0.433 ng/ul m
 RT: 16.581 min Scan# 2980
 Delta R.T. -0.003 min
 Lab File: BN033649.D
 Acq: 28 Aug 2024 17:10

Instrument :
 BNA_N
 ClientSampleId :
 E2494

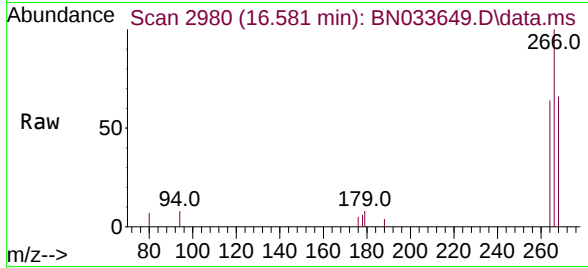

Tgt Ion:266 Resp: 2134
 Ion Ratio Lower Upper
 266 100
 264 0.0 50.3 75.5
 268 0.0 51.7 77.5

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

