

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
 Data File : BN033661.D
 Acq On : 29 Aug 2024 01:00
 Operator : MA/JU
 Sample : P3711-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E24A9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

Quant Time: Aug 29 02:05:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 27 23:48:09 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.536	152	5585	0.400	ng/ul	0.00
4) Naphthalene-d8	10.294	136	15945	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.174	164	8913	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.923	188	18424m	0.400	ng/ul	0.00
17) Chrysene-d12	21.130	240	14163m	0.400	ng/ul	0.00
23) Perylene-d12	23.289	264	14432m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	31860	5.549	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.894	152	8903	0.389	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	20735	0.491	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.343	128	1016	0.024	ng/ul#	Qvalue 80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082824\
Data File : BN033661.D
Acq On : 29 Aug 2024 01:00
Operator : MA/JU
Sample : P3711-17
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E24A9

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024


Quant Time: Aug 29 02:05:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 23:48:09 2024
Response via : Initial Calibration

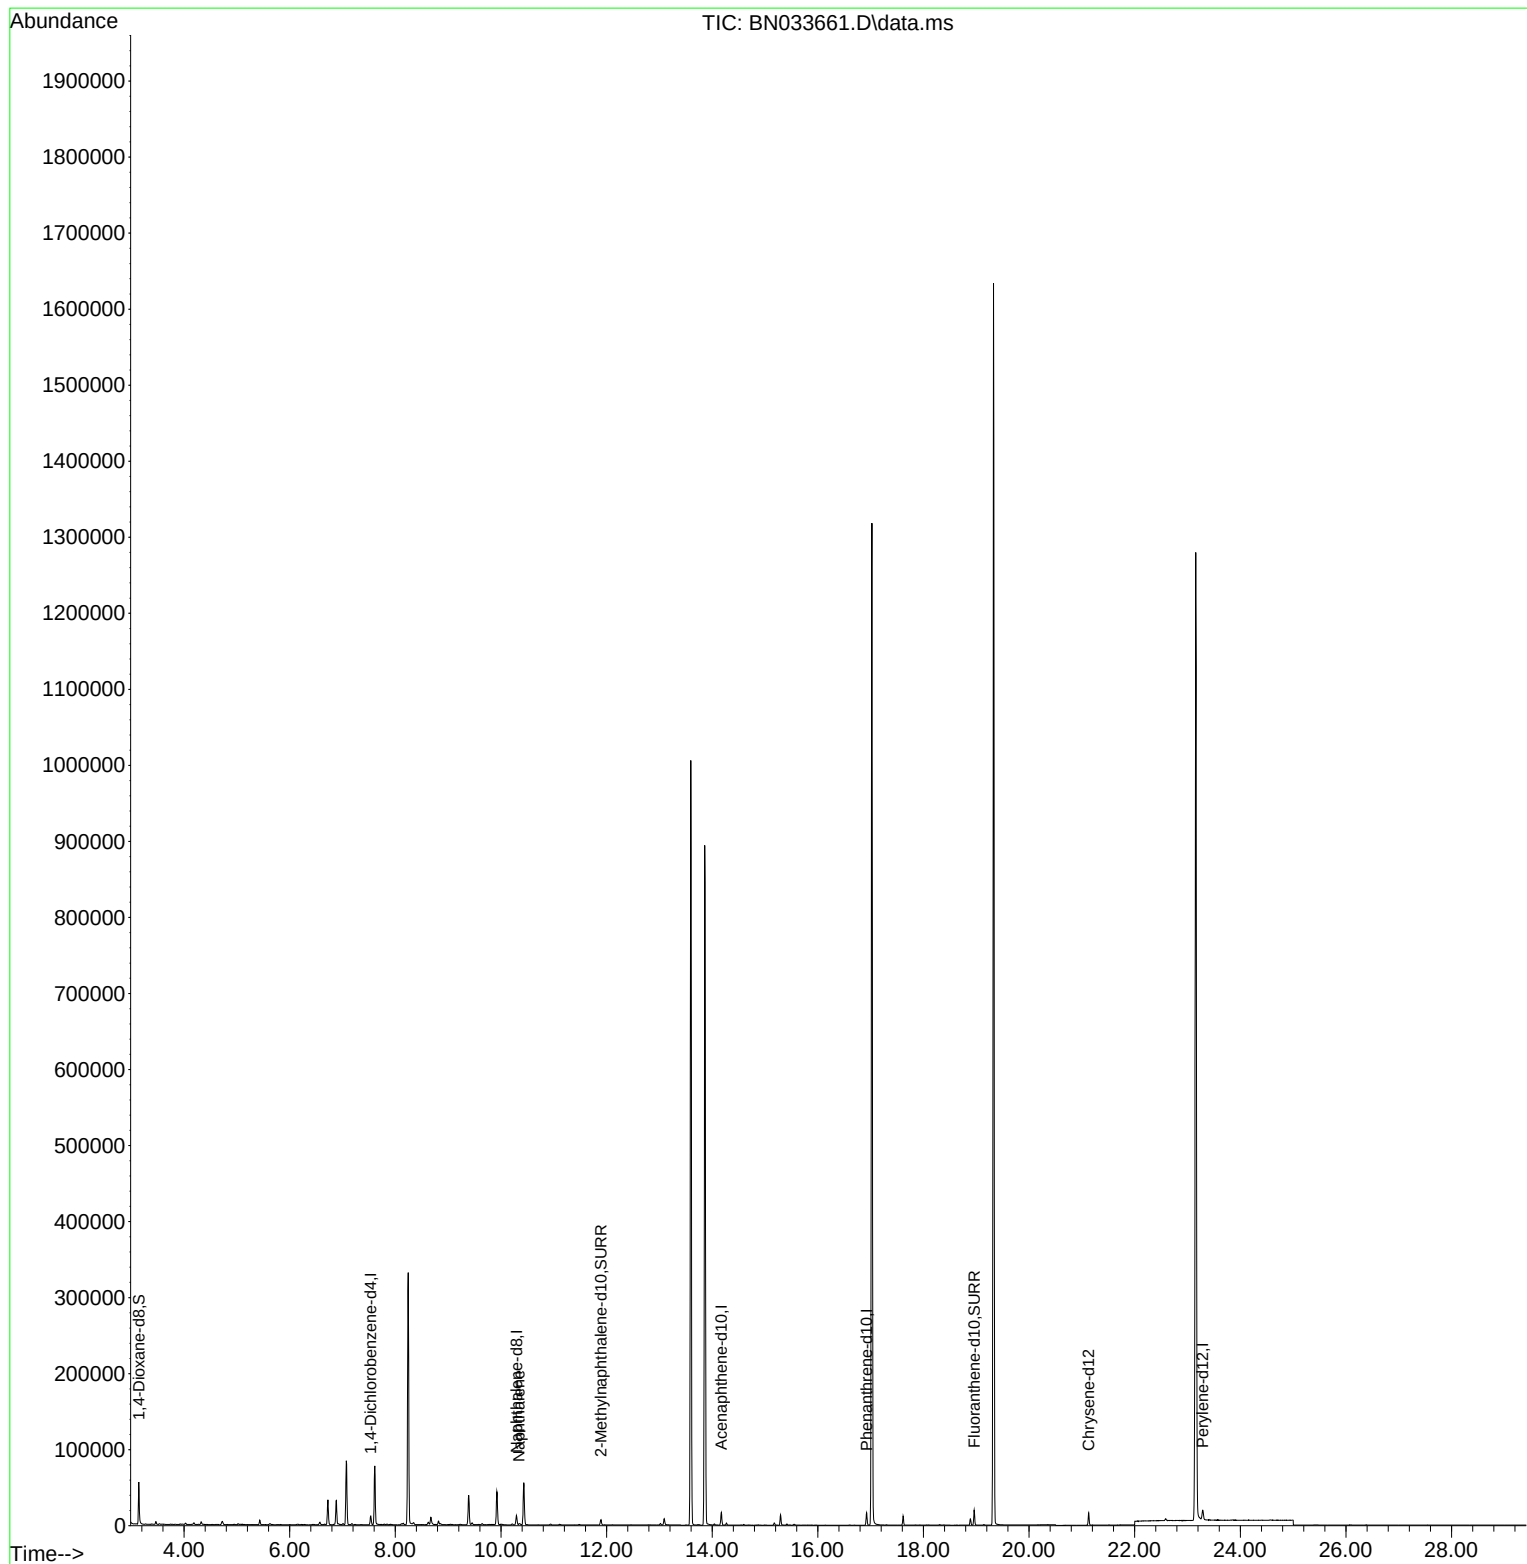

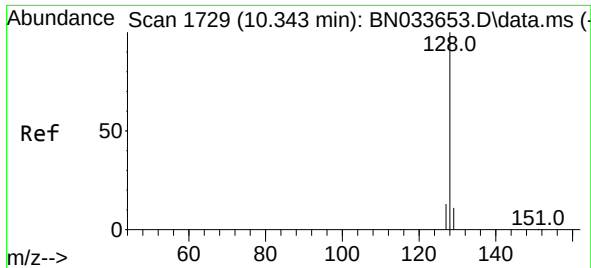

#5
Naphthalene
Concen: 0.024 ng/ul
RT: 10.343 min Scan# 1729
Delta R.T. -0.004 min
Lab File: BN033661.D
Acq: 29 Aug 2024 01:00

Instrument :
BNA_N
ClientSampleId :
E24A9

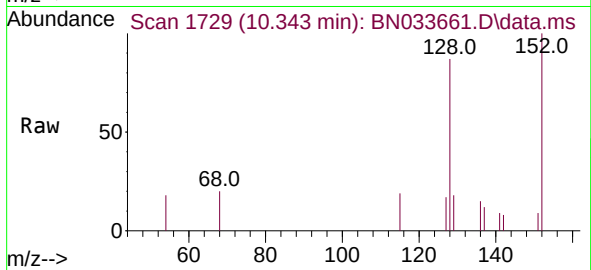

Tgt Ion:128 Resp: 1010
Ion Ratio Lower Upper
128 100
129 20.8 9.3 13.9
127 19.9 10.8 16.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

