
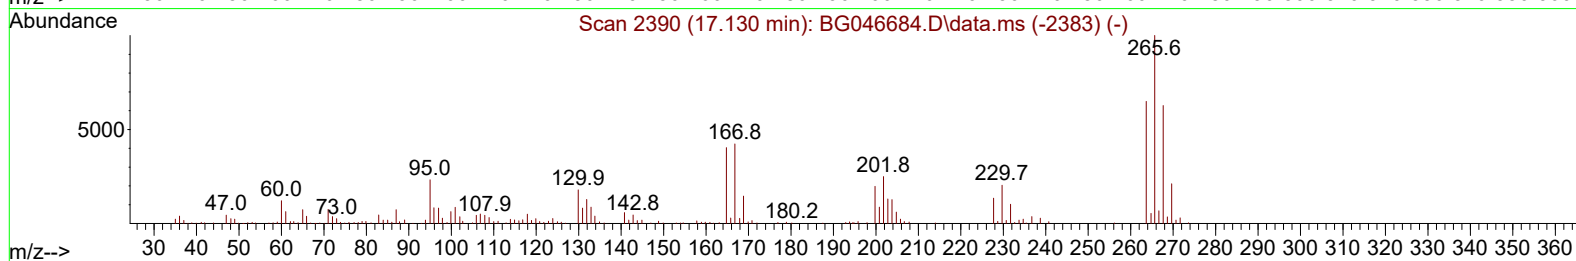
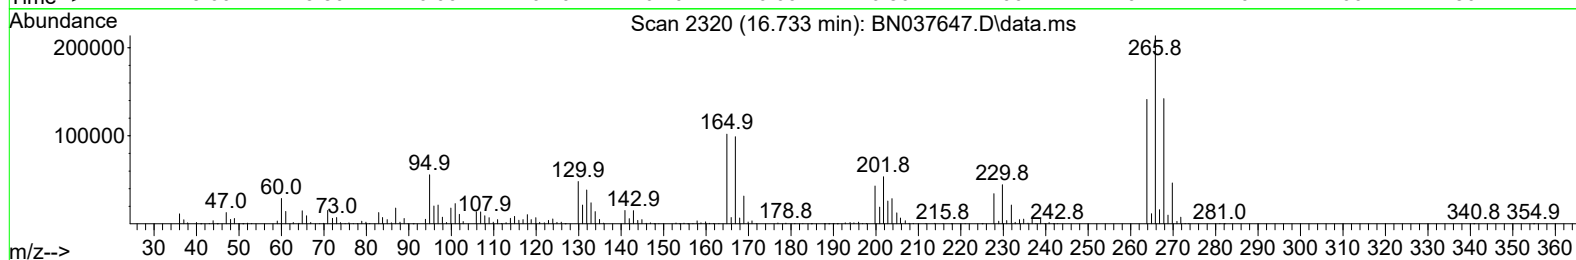


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082825\
Data File : BN037647.D
Acq On : 28 Aug 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 04:47:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

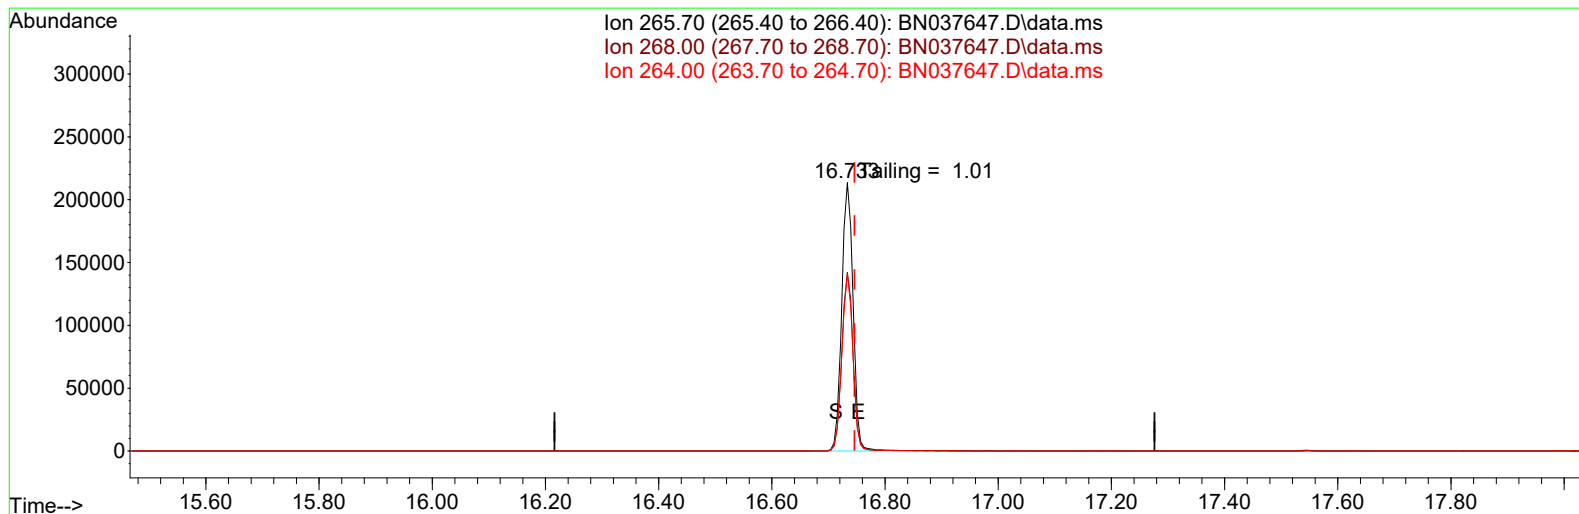

TIC: BN037647.D\data.ms

(70) Pentachlorophenol (C)




16.733min (-0.013) 27093.45 ng

response 295758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.56
264.00	61.60	66.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082825\
Data File : BN037647.D
Acq On : 28 Aug 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 04:47:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

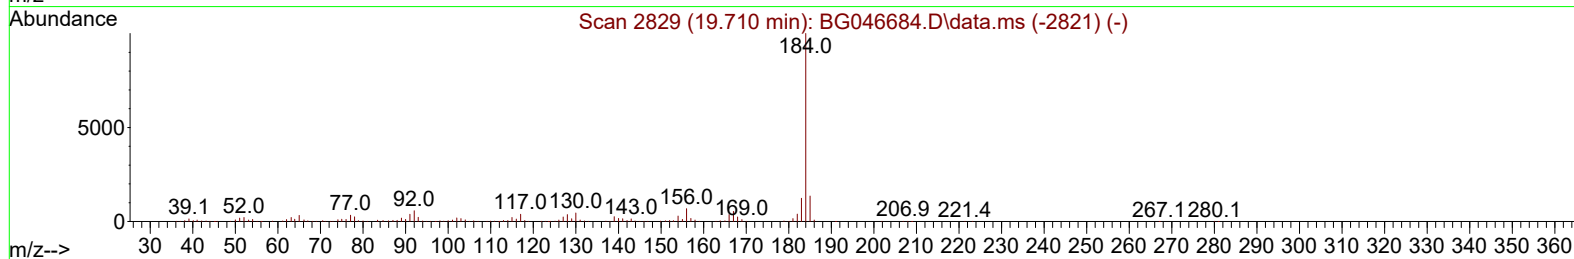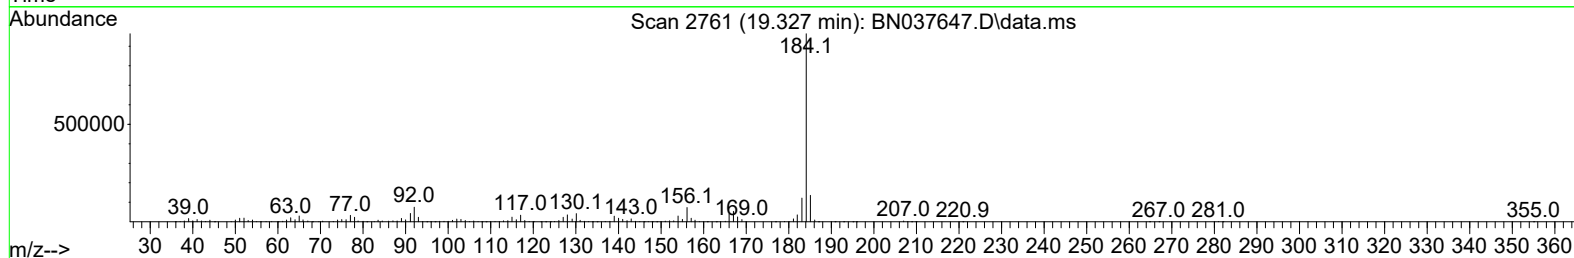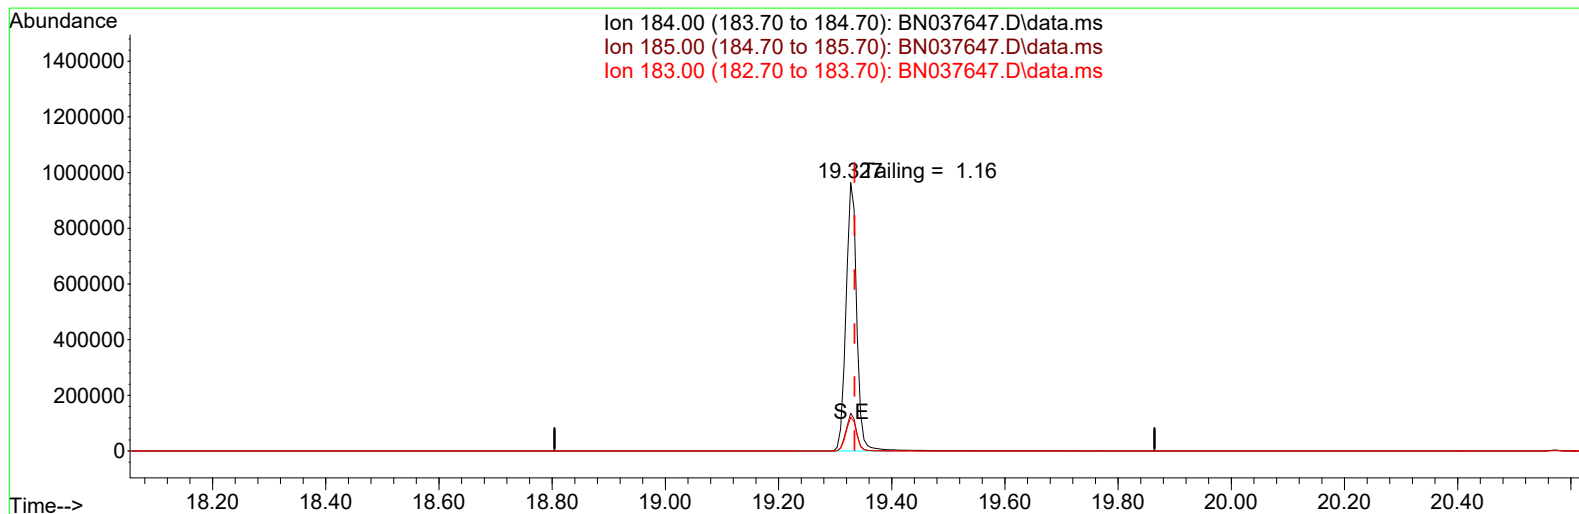

TIC: BN037647.D\data.ms

(77) Benzidine**19.327min (-0.007) 0.00 ng****response 1266888**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	12.62
0.00	0.00	0.00