

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082918\
 Data File : BN002542.D
 Acq On : 29 Aug 2018 13:15
 Operator : JU/SJ
 Sample : J4596-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z30

Quant Time: Aug 29 17:40:33 2018
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 25 04:34:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	160185	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	741045	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	446812	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1027946	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1125278	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1144536	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.23	96	20461	6.03	ng/uL	0.00
5) Phenol-d5	6.85	99	444846	30.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	304107	32.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	366987	32.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	374857	31.92	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	180454	30.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	198624	32.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	384075	33.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	522219	42.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1368428	36.94	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1719197	37.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	193753	27.67	ng/ul	0.00
57) Fluorene-d10	15.30	176	1211668	37.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	158871	24.27	ng/ul	0.00
70) Anthracene-d10	17.15	188	1903894	38.77	ng/ul	0.00
78) Pyrene-d10	19.45	212	2091609	38.85	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	2304611	38.51	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.88	94	19293	1.290	ng/ul#	88
44) Dimethylphthalate	13.76	163	334804	9.216	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082918\
Data File : BN002542.D
Acq On : 29 Aug 2018 13:15
Operator : JU/SJ
Sample : J4596-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z30

Quant Time: Aug 29 17:40:33 2018
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 25 04:34:18 2018
Response via : Initial Calibration

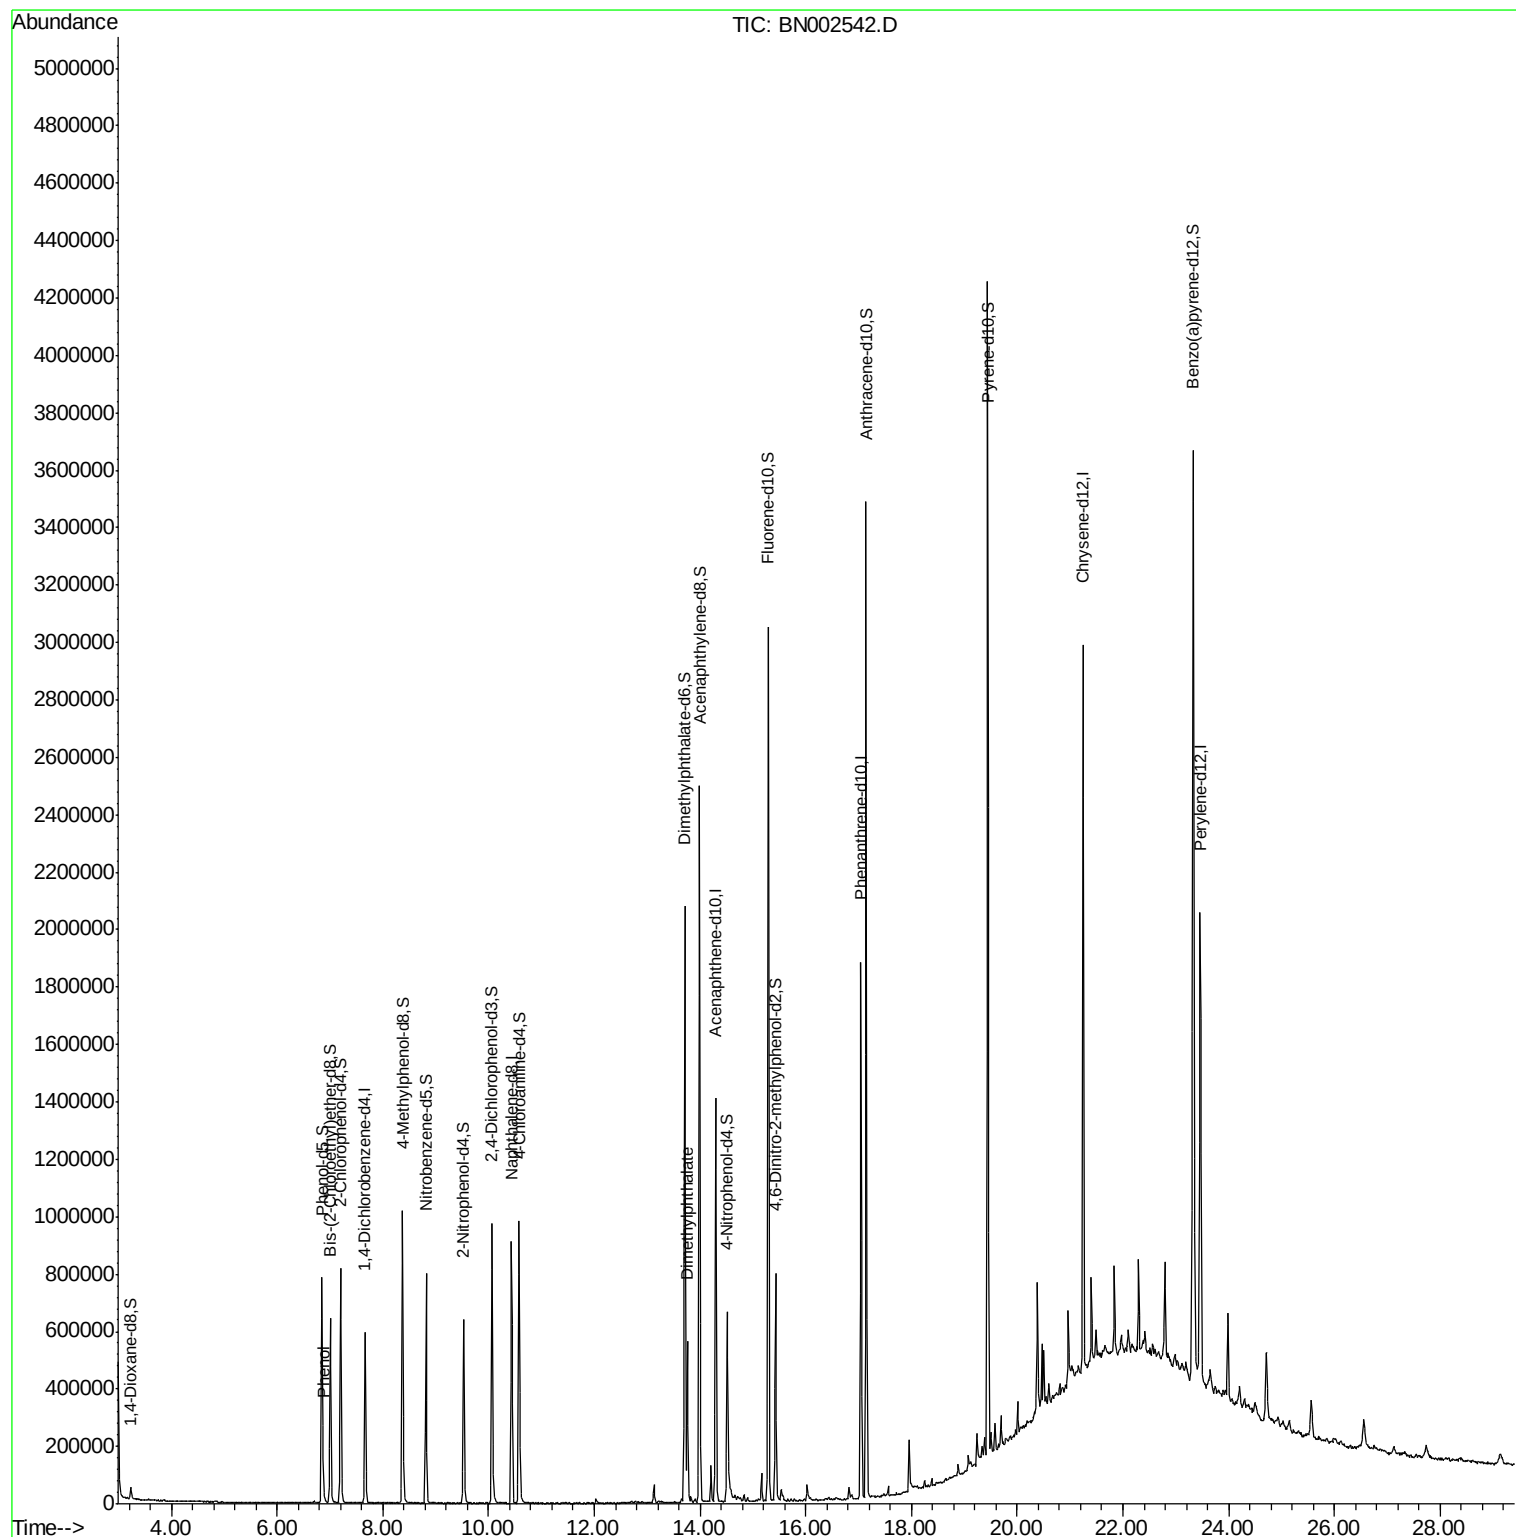

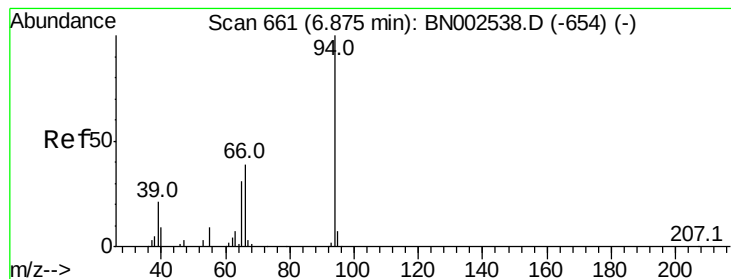





#6

Phenol

Concen: 1.290 ng/ul
 RT: 6.88 min Scan# 661
 Delta R.T. -0.00 min
 Lab File: BN002542.D
 Acq: 29 Aug 2018 13:15

Instrument :
 BNA_N
 ClientSampleId :
 A3Z30

Tot Ion: 94 Resp: 19293
 Ion Ratio Lower Upper
 94 100
 65 30.1 21.0 31.6
 66 45.7 29.3 43.9#

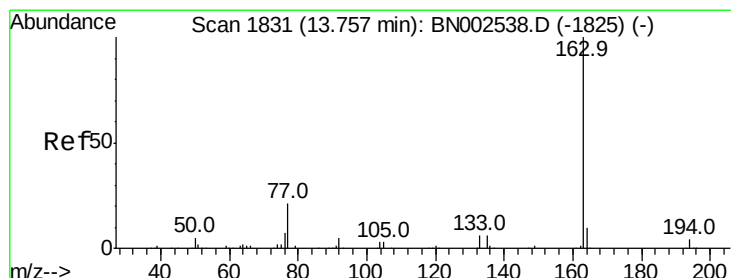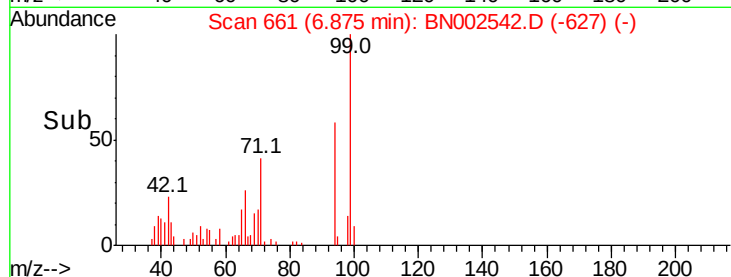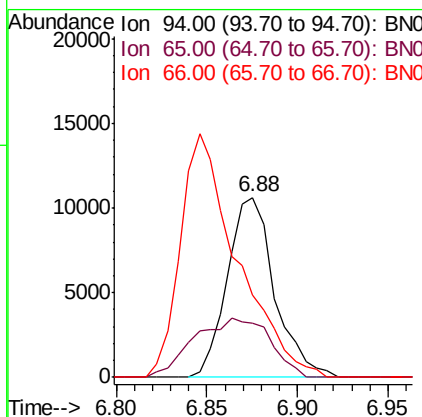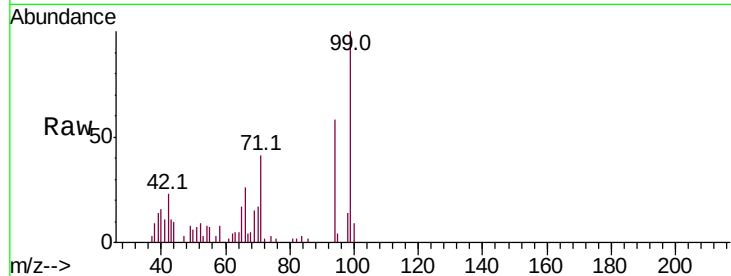

#44

Dimethylphthalate

Concen: 9.216 ng/ul
 RT: 13.76 min Scan# 1831
 Delta R.T. -0.01 min
 Lab File: BN002542.D
 Acq: 29 Aug 2018 13:15

Tgt Ion:163 Resp: 334804
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.2 4.8
 164 10.1 7.8 11.8

