

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082918\
 Data File : BN002543.D
 Acq On : 29 Aug 2018 13:50
 Operator : JU/SJ
 Sample : J4596-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z29

Quant Time: Aug 29 17:42:00 2018
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 25 04:34:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	141636	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	649577	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	410753	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	989975	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1110067	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1100706	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	9269	3.09	ng/uL	0.00
5) Phenol-d5	6.85	99	218447	16.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	138358	16.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	173756	17.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	170662	16.44	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	75545	14.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	83309	15.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	172454	17.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	205517	19.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	609379	17.90	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	732961	17.55	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	71461	11.10	ng/ul	0.00
57) Fluorene-d10	15.29	176	555261	18.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	58238	9.24	ng/ul	0.00
70) Anthracene-d10	17.15	188	866944	18.33	ng/ul	0.00
78) Pyrene-d10	19.45	212	1006973	18.96	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	1059312	18.41	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.76	163	259137	7.760	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082918\
Data File : BN002543.D
Acq On : 29 Aug 2018 13:50
Operator : JU/SJ
Sample : J4596-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z29

Quant Time: Aug 29 17:42:00 2018
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 25 04:34:18 2018
Response via : Initial Calibration

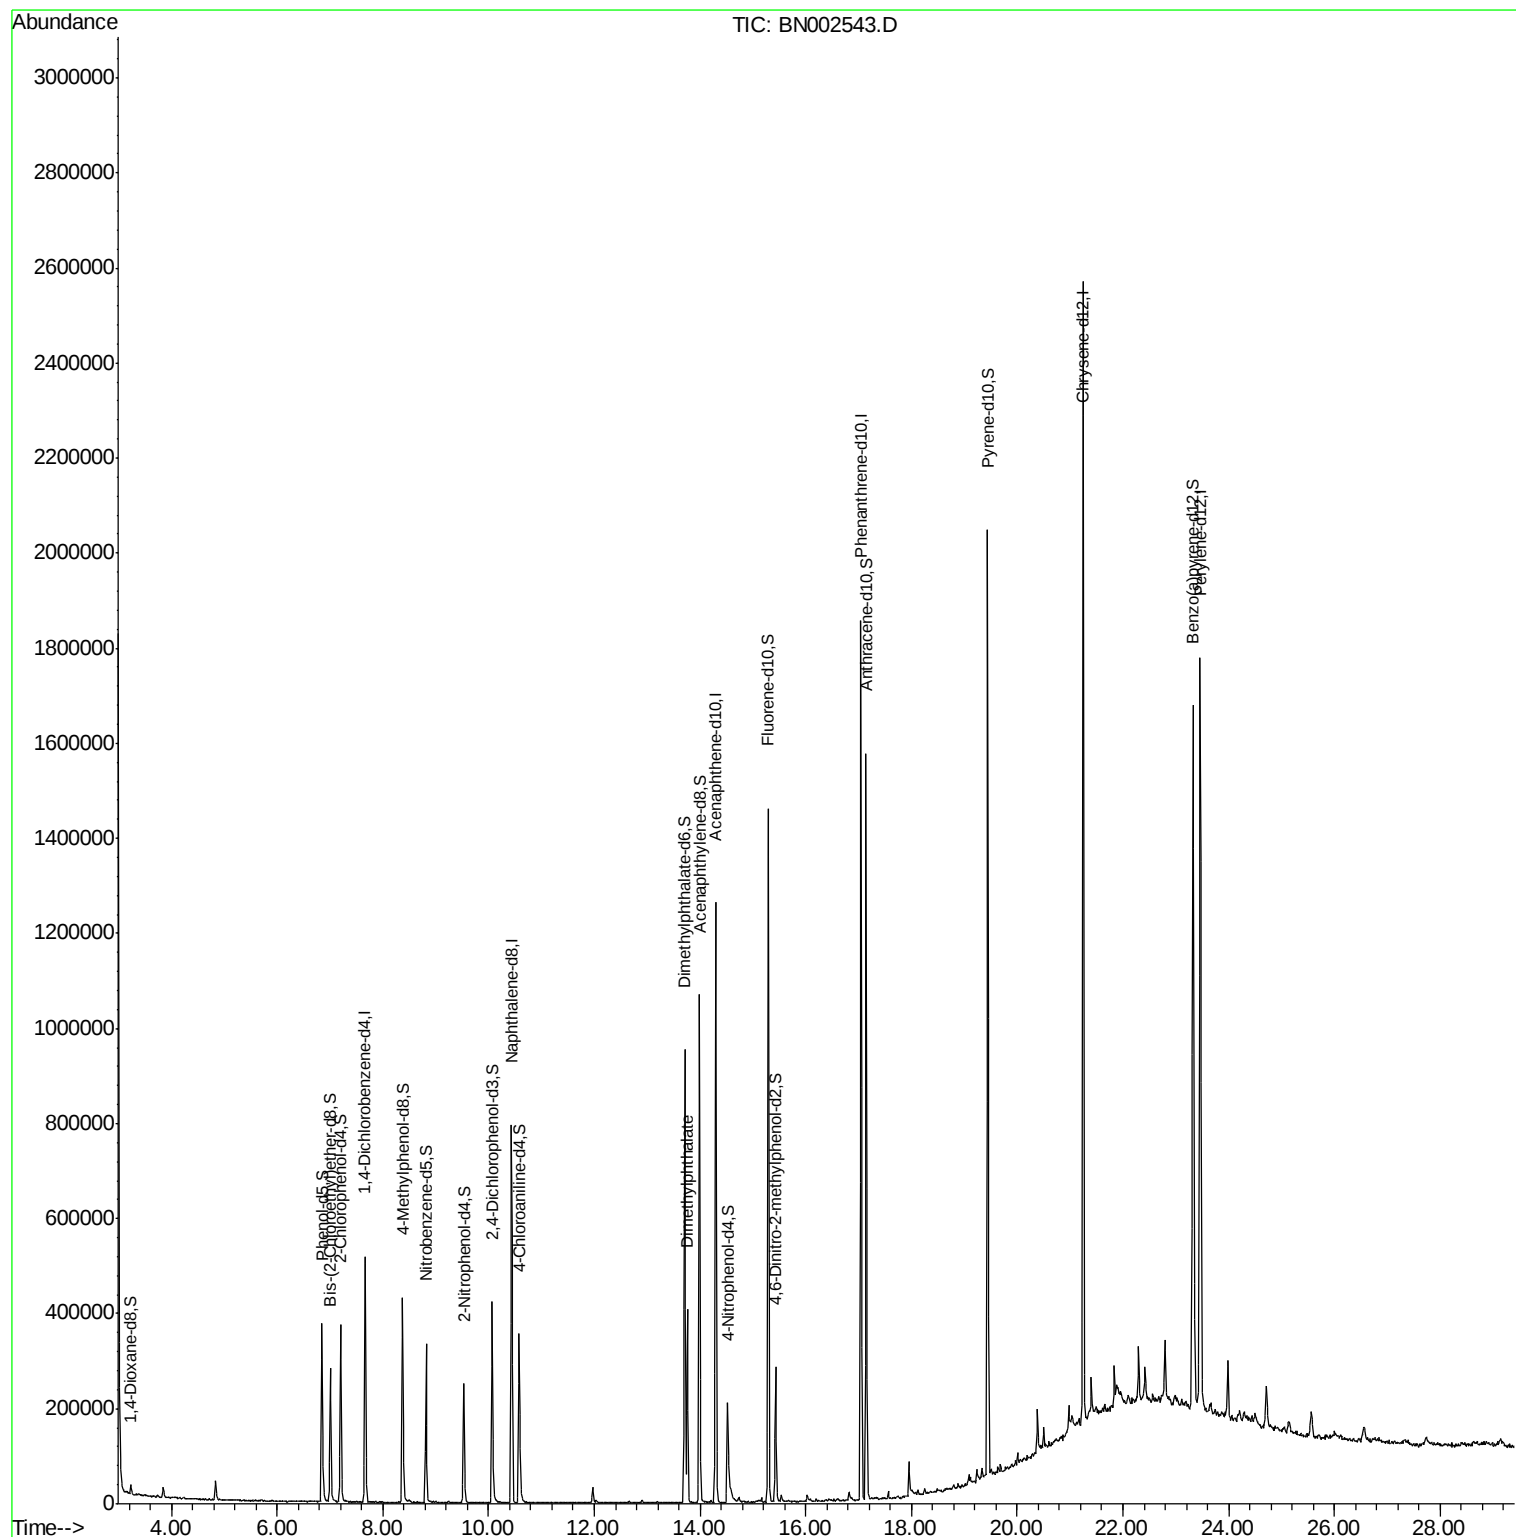

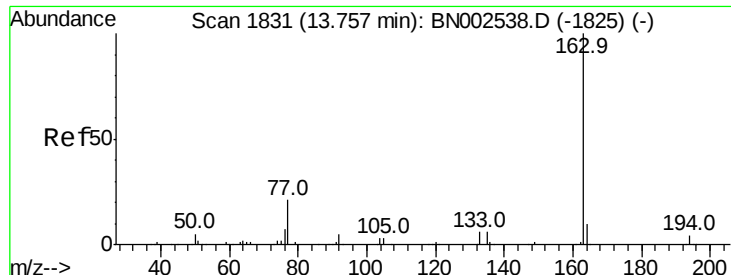

#44

Dimethylphthalate

Concen: 7.760 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. -0.01 min

Lab File: BN002543.D

Acq: 29 Aug 2018 13:50

Instrument :

BNA_N

ClientSampleId :

A3Z29


Tot Ion:163 Resp: 259137

Ion Ratio Lower Upper

163 100

194 4.4 3.2 4.8

164 10.1 7.8 11.8

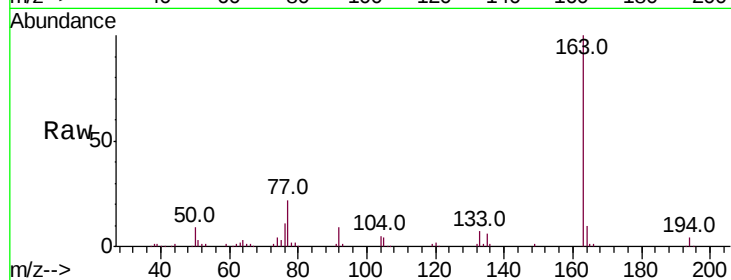

Abundance Ion 163.00 (162.70 to 163.70): E
250000
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

