


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083019\
 Data File : BN007519.D
 Acq On : 30 Aug 2019 10:06
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 29 12:18:45 2019

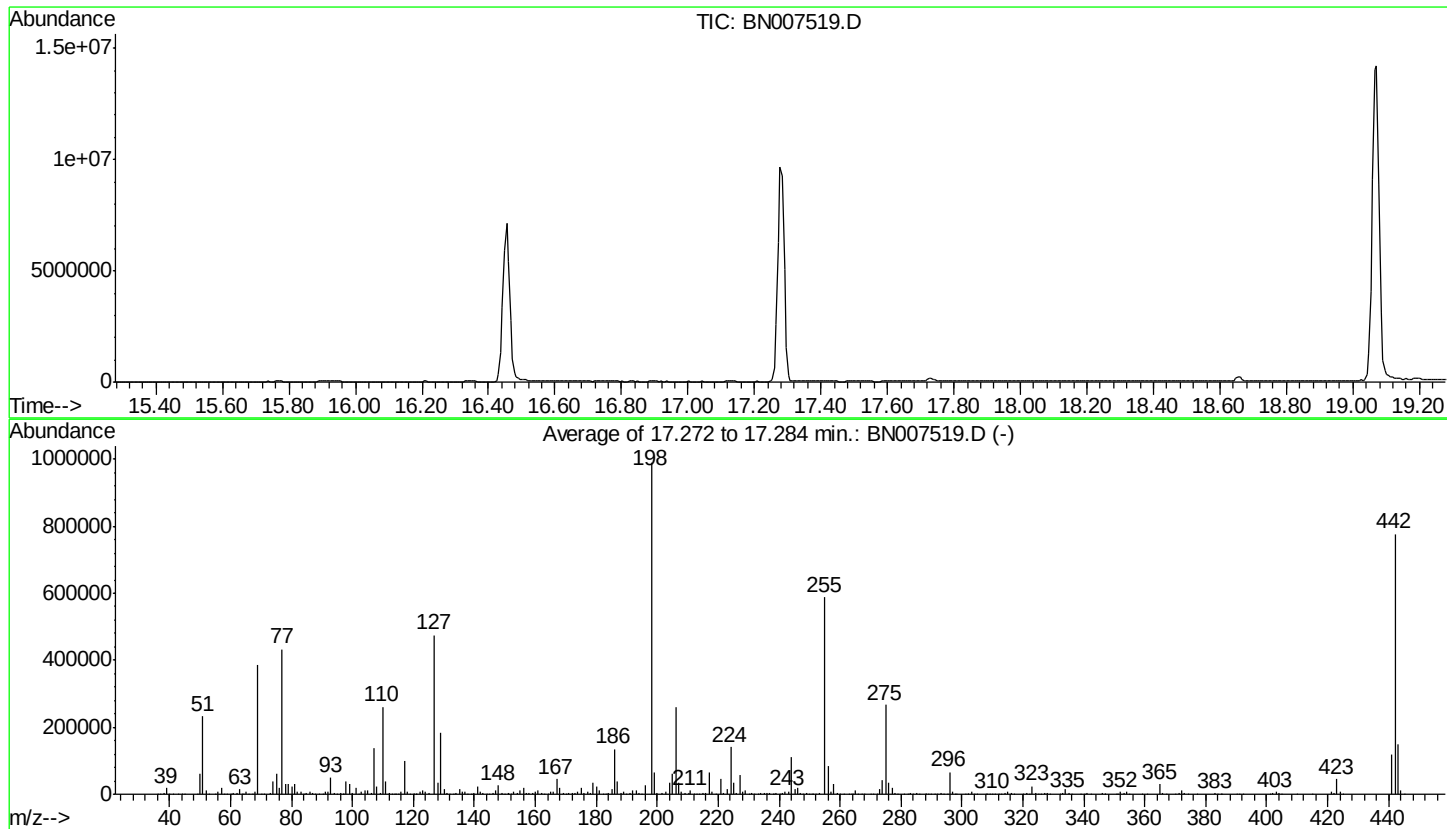

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	231637	PASS
68	69	0.00	2	1.9	7289	PASS
69	198	0.00	100	39.1	386915	PASS
70	69	0.00	2	0.5	1777	PASS
127	198	10	80	48.0	474752	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	989930	PASS
199	198	5	9	6.5	64800	PASS
275	198	10	60	26.9	266773	PASS
365	198	1	100	3.0	29293	PASS
441	198	0.01	100	12.0	119077	PASS
442	198	50	100	78.5	776725	PASS
443	442	15	24	19.3	150064	PASS