
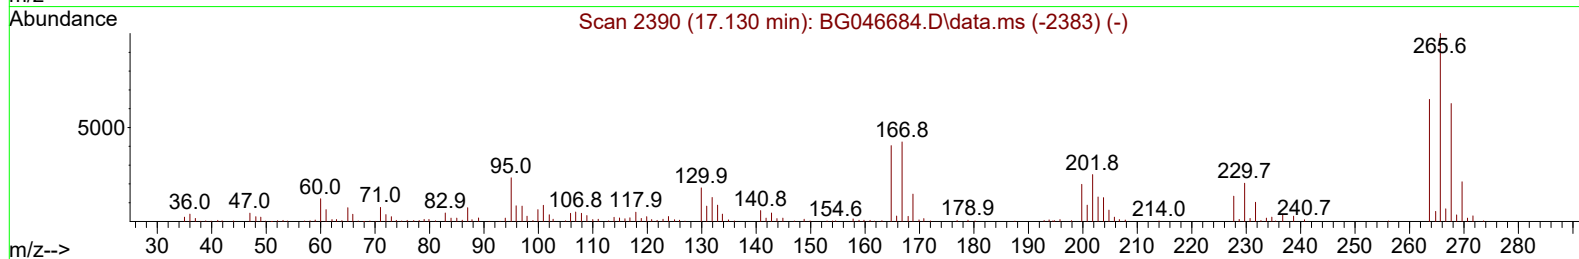
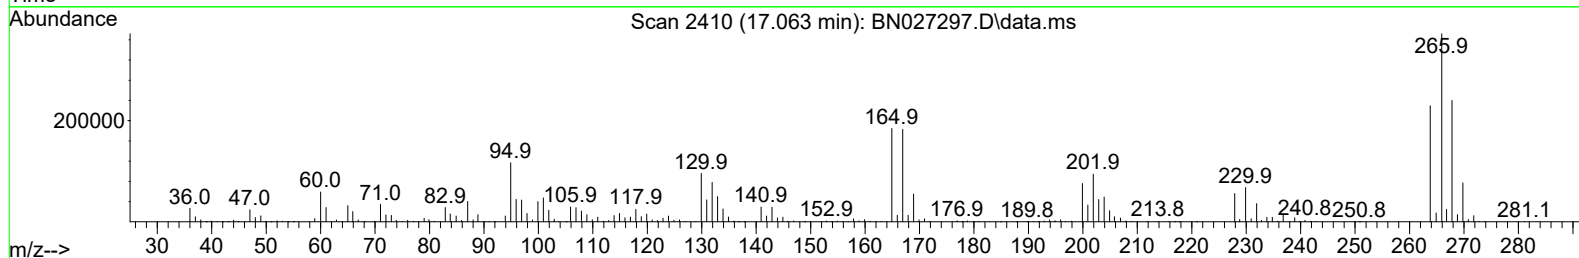


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027297.D
Acq On : 31 Aug 2023 06:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 77 Sample Multiplier: 1

Quant Time: Aug 31 07:53:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 07:53:42 2023
Response via : Initial Calibration

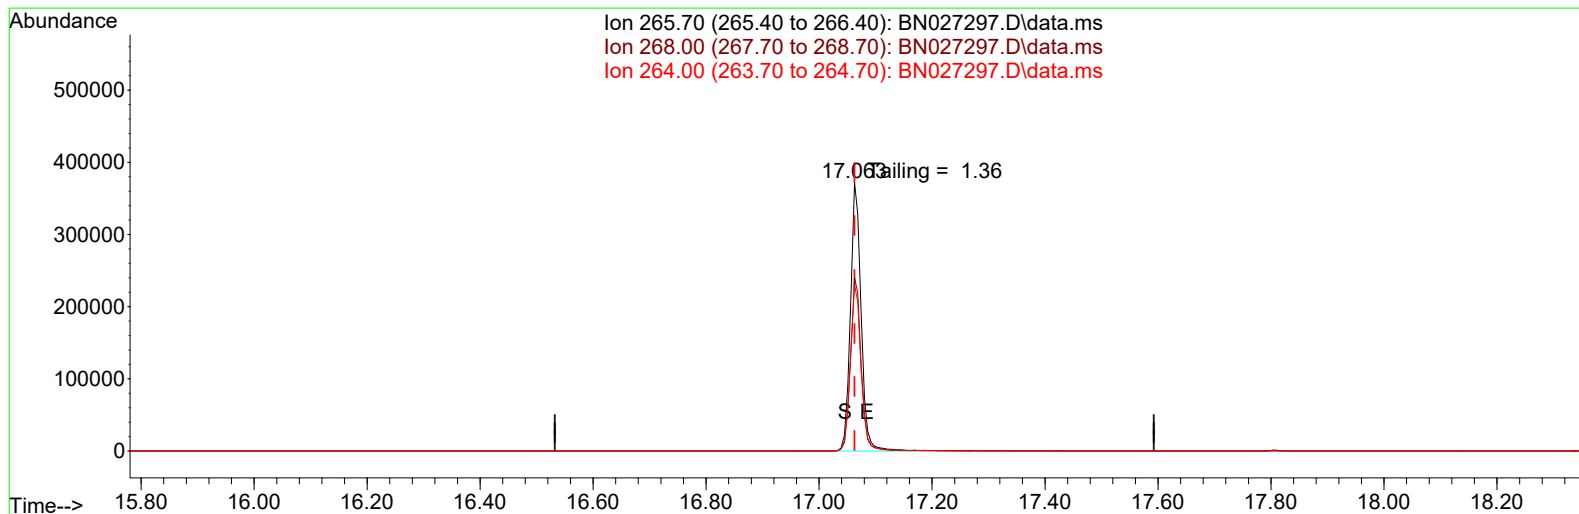

TIC: BN027297.D\data.ms

(70) Pentachlorophenol (C)




17.063min (0.000) 19323.70 ng

response 488305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.53
264.00	61.60	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027297.D
Acq On : 31 Aug 2023 06:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 77 Sample Multiplier: 1

Quant Time: Aug 31 07:53:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 07:53:42 2023
Response via : Initial Calibration

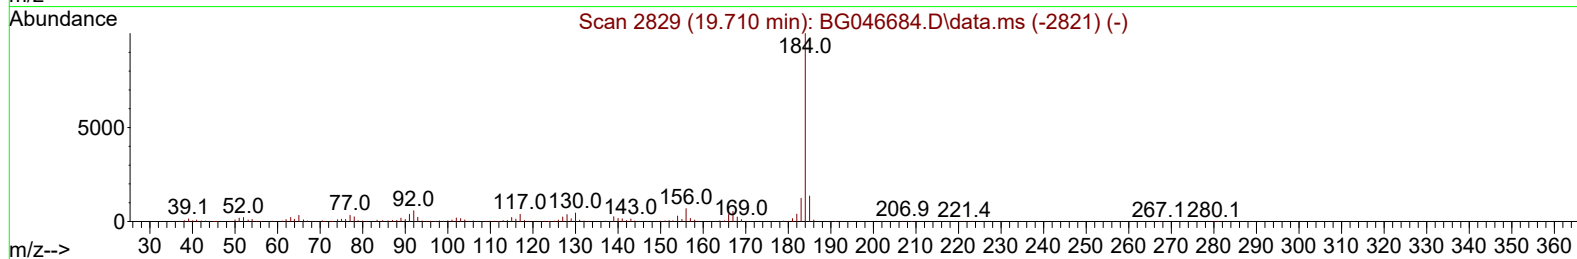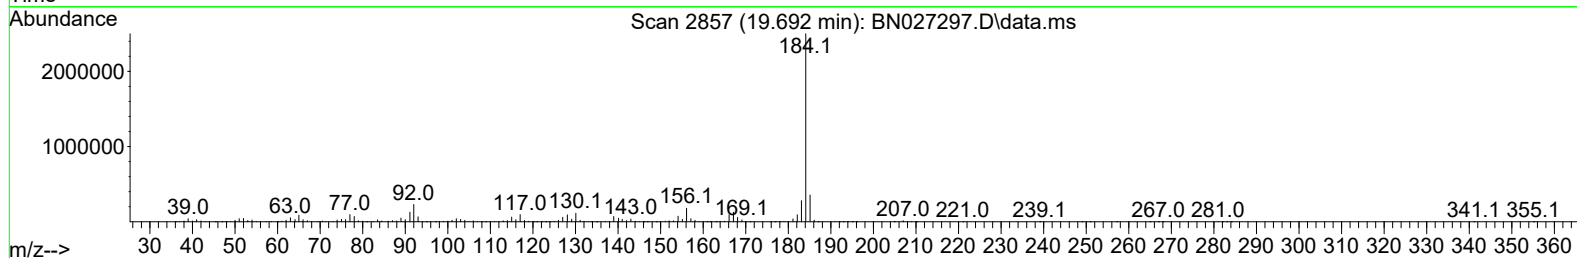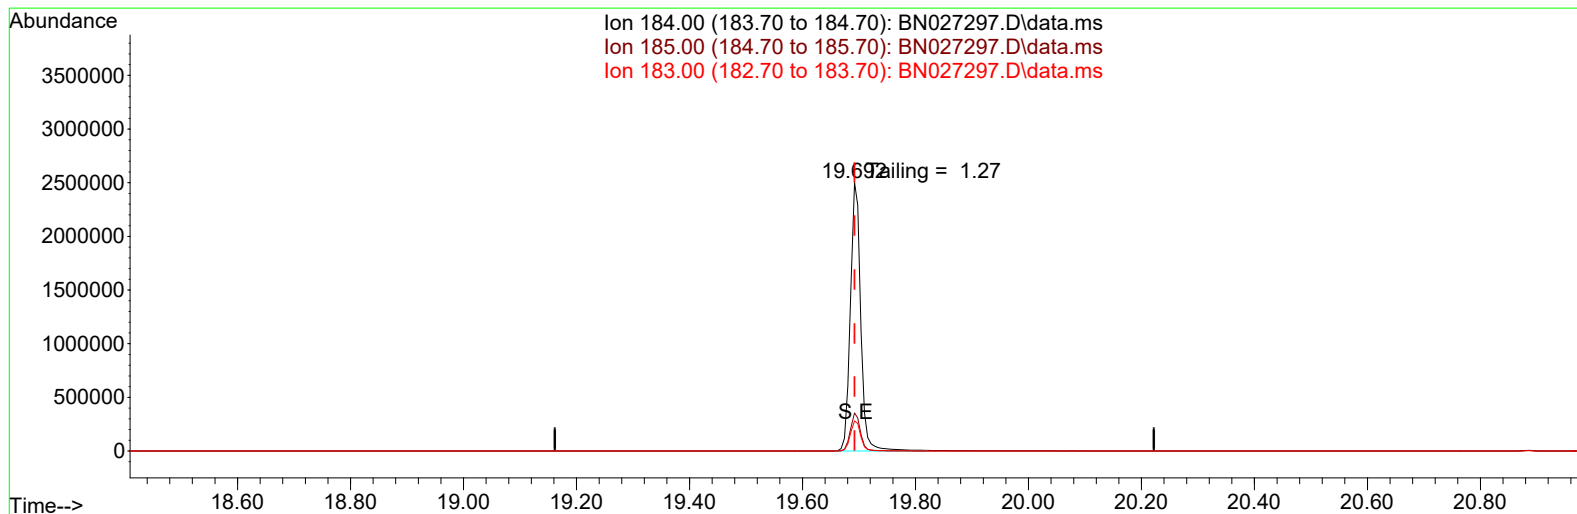

TIC: BN027297.D\data.ms

(77) Benzidine

19.692min (0.000) 0.00 ng

response 3226036

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.19
183.00	13.20	11.22
0.00	0.00	0.00