
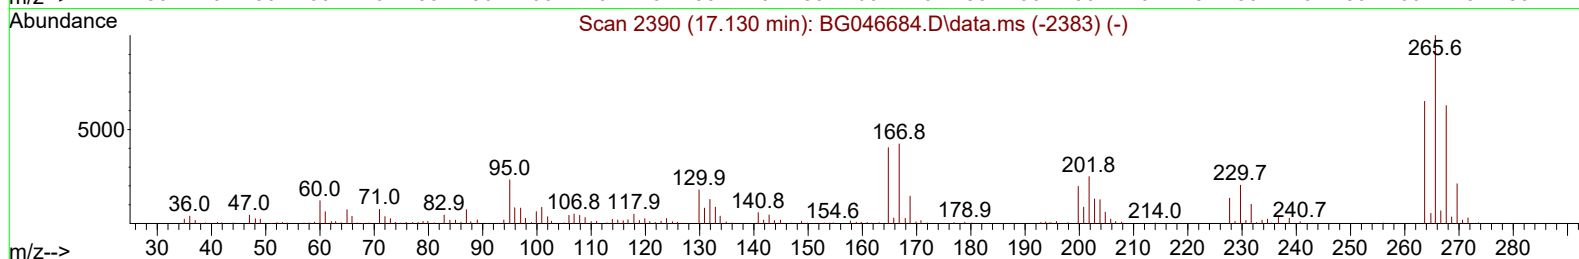
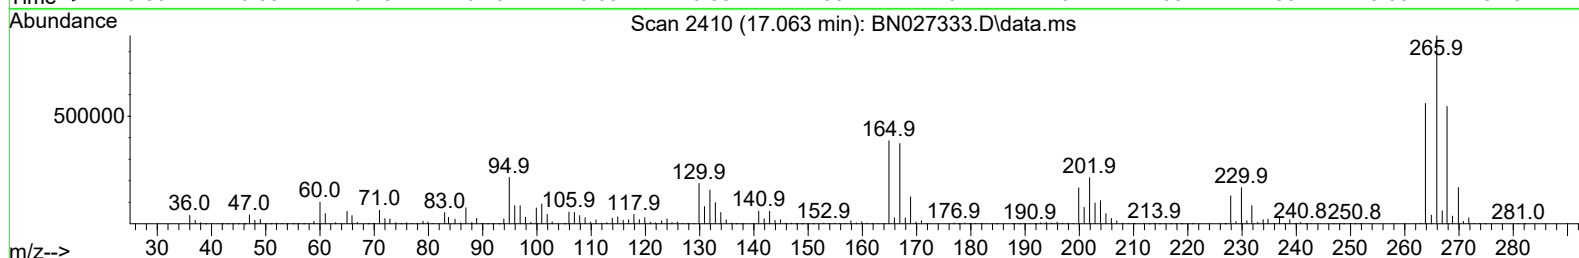


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027333.D
Acq On : 01 Sep 2023 07:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 114 Sample Multiplier: 1

Quant Time: Sep 01 07:35:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 01 07:34:32 2023
Response via : Initial Calibration

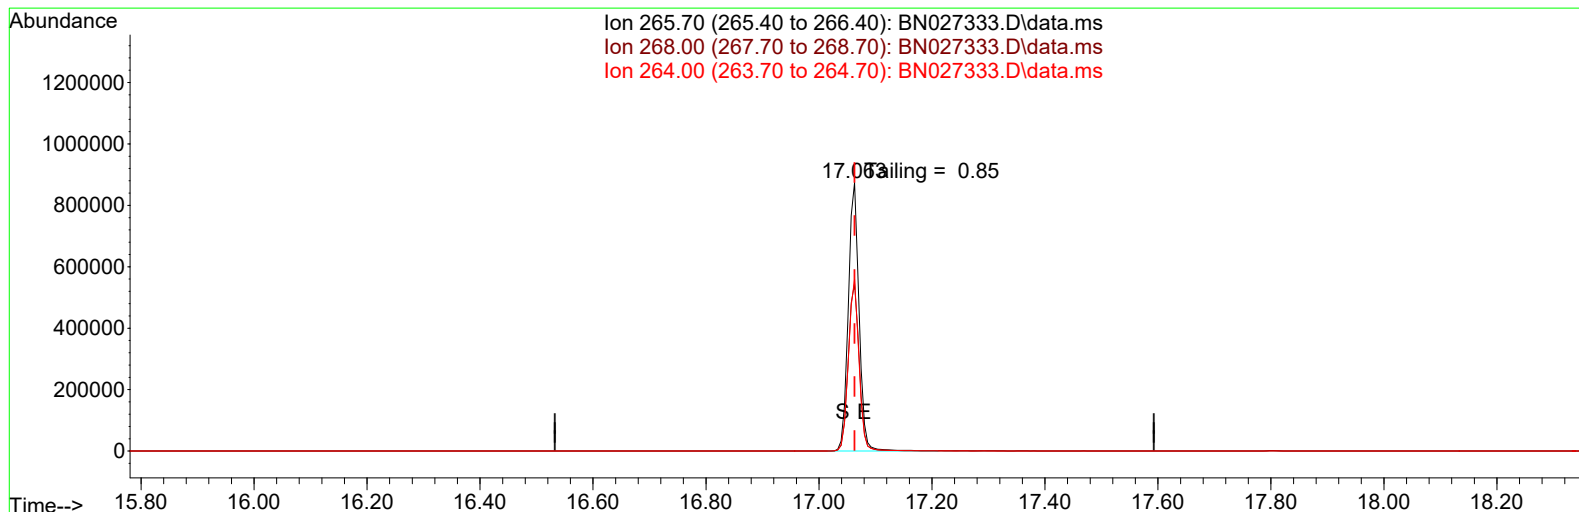

TIC: BN027333.D\data.ms

(70) Pentachlorophenol (C)




17.063min (-0.000) 32188.41 ng

response 1161485

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.35
264.00	61.60	63.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027333.D
Acq On : 01 Sep 2023 07:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 114 Sample Multiplier: 1

Quant Time: Sep 01 07:35:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 01 07:34:32 2023
Response via : Initial Calibration

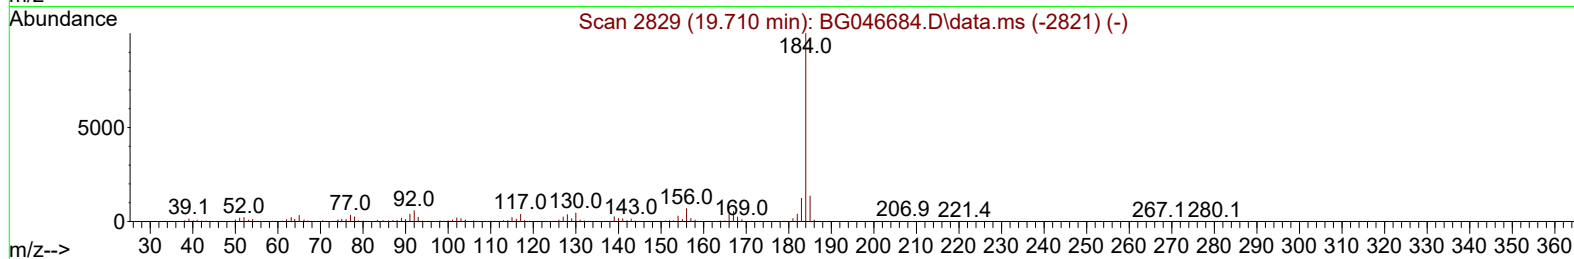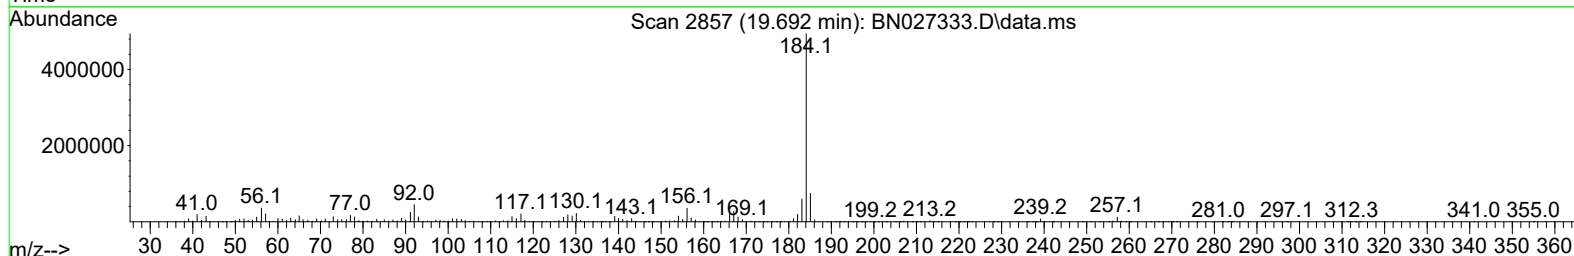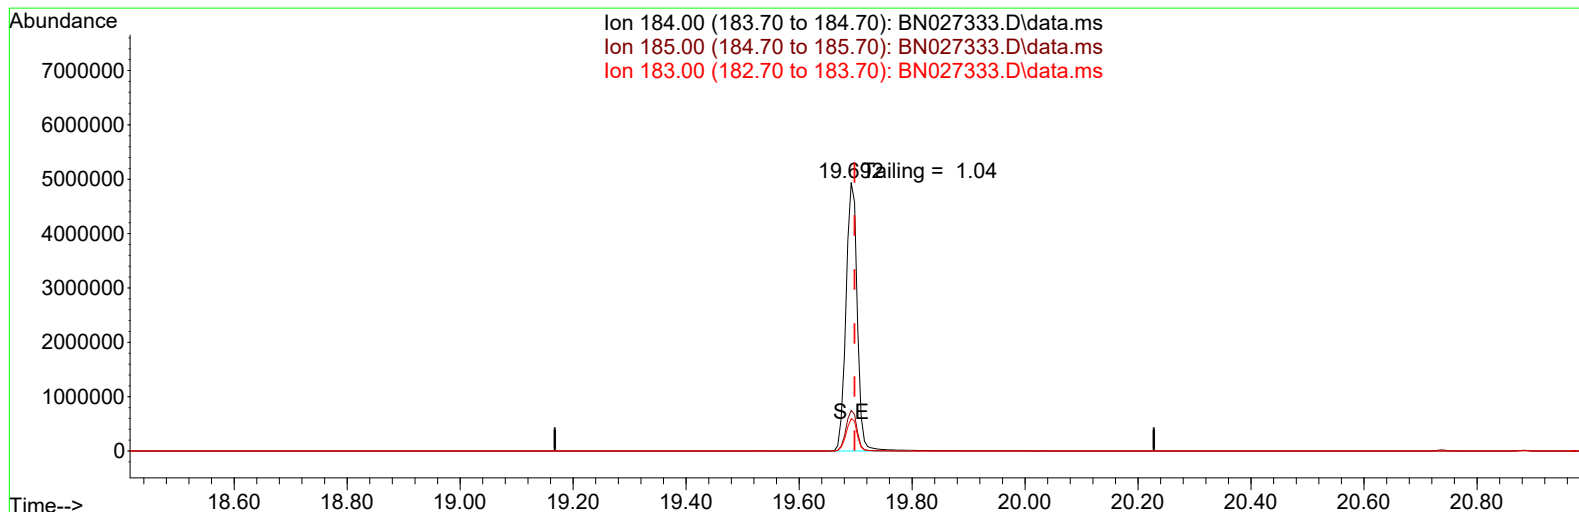

TIC: BN027333.D\data.ms

(77) Benzidine**19.692min (-0.006) 328028.85 ng****response 6815226**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.17
183.00	13.20	12.10
0.00	0.00	0.00