
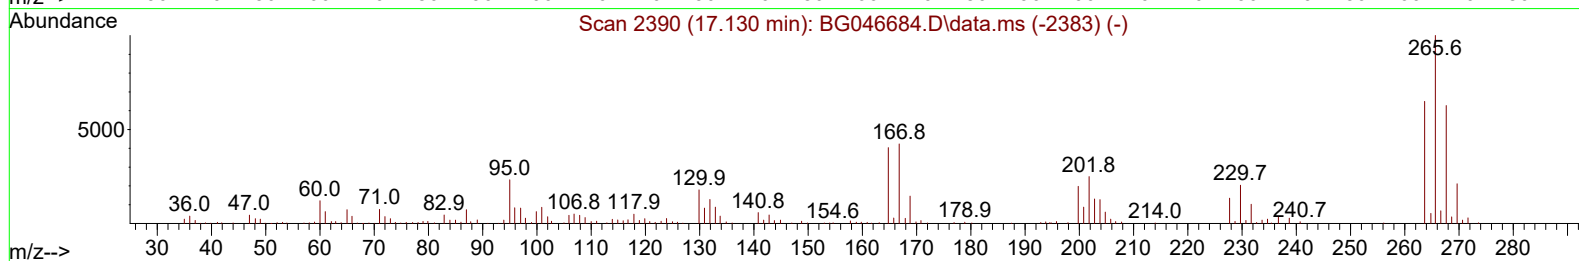
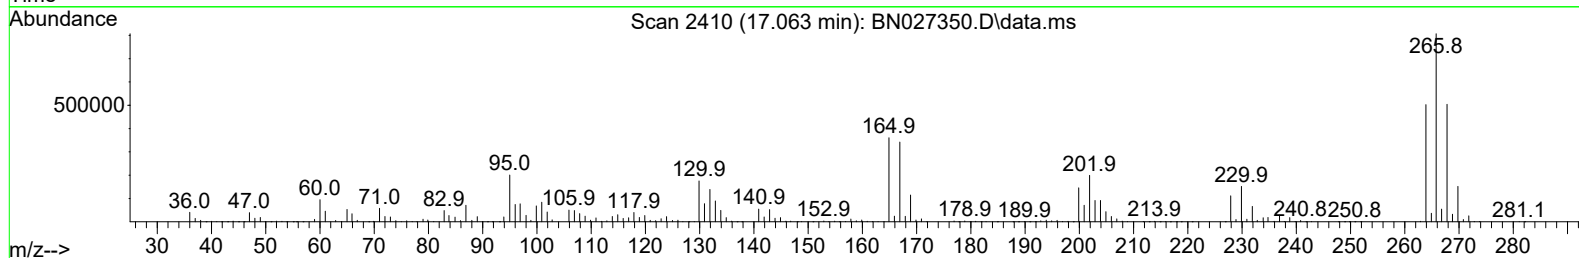


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027350.D
Acq On : 01 Sep 2023 17:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 131 Sample Multiplier: 1

Quant Time: Sep 02 04:36:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 04:36:41 2023
Response via : Initial Calibration

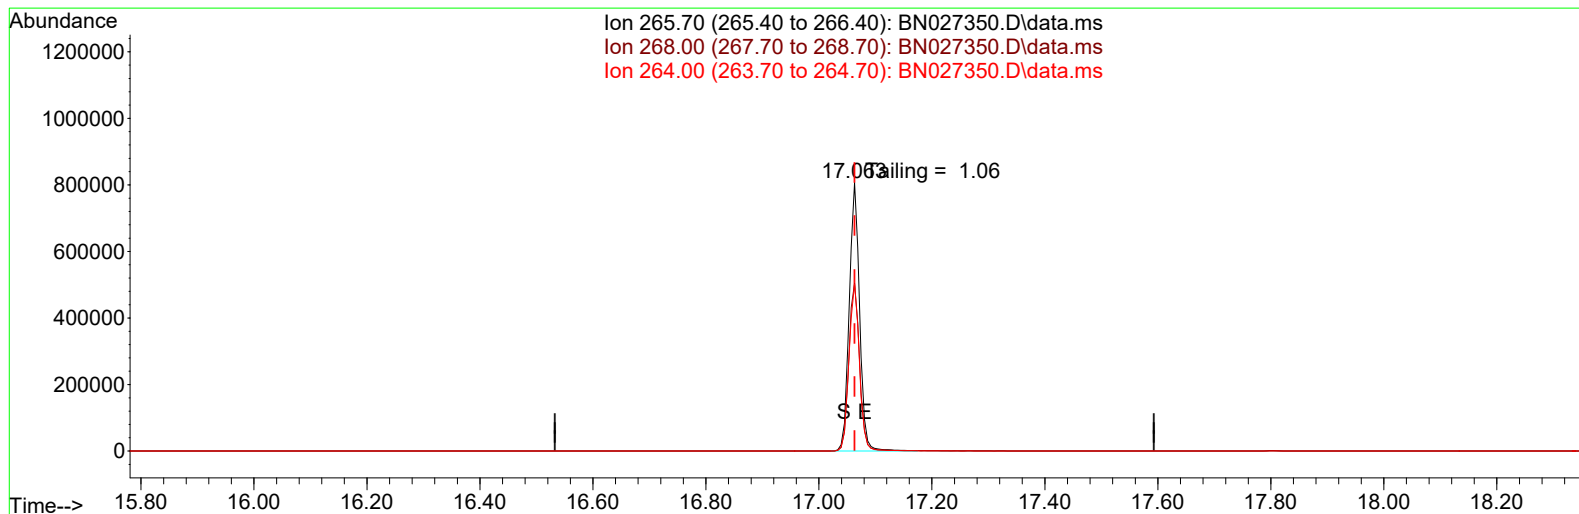

TIC: BN027350.D\data.ms

(70) Pentachlorophenol (C)




17.063min (0.000) 32606.02 ng

response 1033003

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.47
264.00	61.60	62.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027350.D
Acq On : 01 Sep 2023 17:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 131 Sample Multiplier: 1

Quant Time: Sep 02 04:36:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 04:36:41 2023
Response via : Initial Calibration

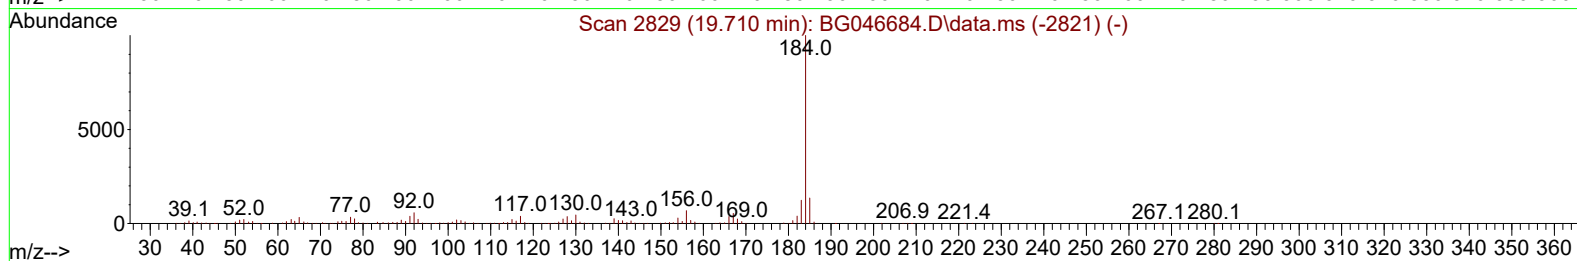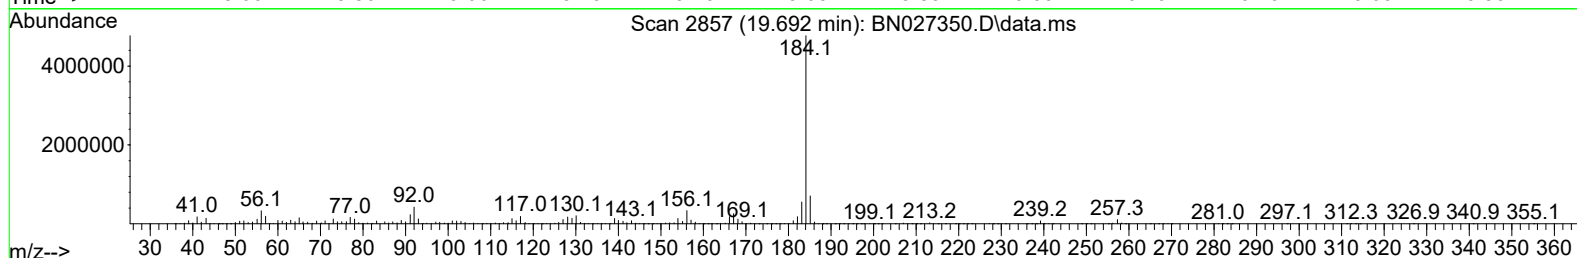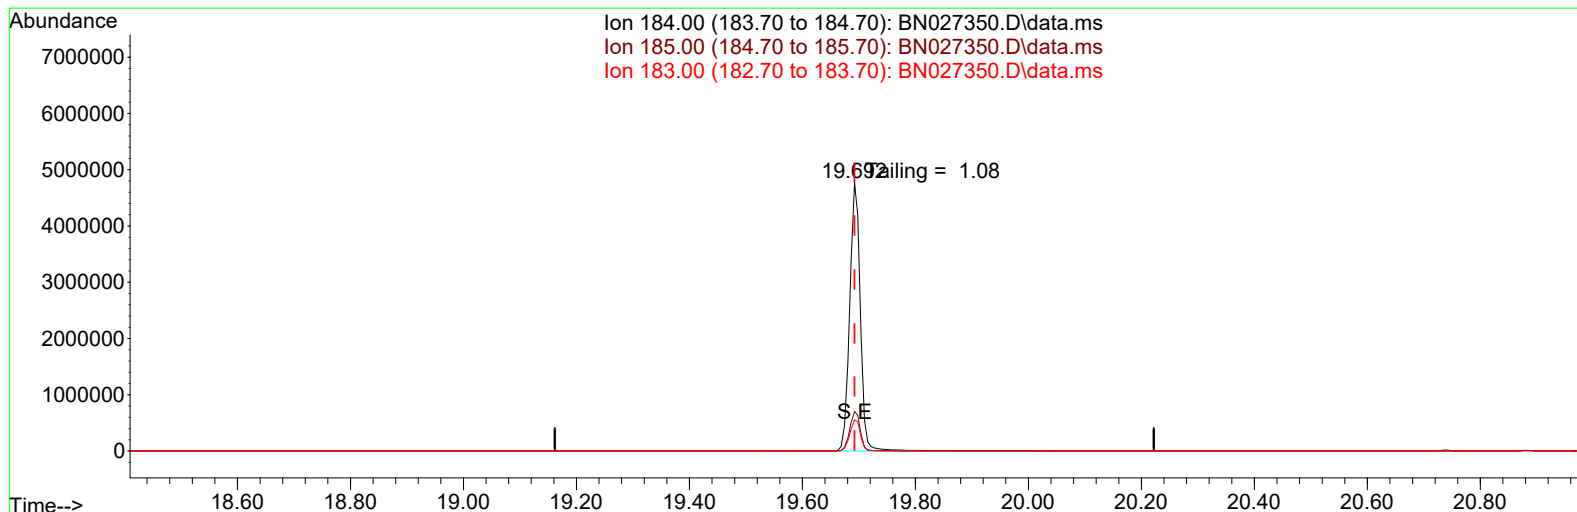

TIC: BN027350.D\data.ms

(77) Benzidine**19.692min (0.000) 296839.97 ng****response 6194687**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.81
183.00	13.20	11.62
0.00	0.00	0.00