

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
 Data File : BN027317.D
 Acq On : 31 Aug 2023 20:04
 Operator : MA/JU
 Sample : PB155046BL
 Misc :
 ALS Vial : 98 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB155046BL

Quant Time: Sep 01 04:03:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 29 05:37:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.066	152	4621	0.400	ng	0.00
7) Naphthalene-d8	10.885	136	12191	0.400	ng	-0.01
13) Acenaphthene-d10	14.694	164	5354	0.400	ng	0.00
19) Phenanthrene-d10	17.443	188	14550	0.400	ng	0.00
29) Chrysene-d12	21.623	240	8573	0.400	ng	0.00
35) Perylene-d12	24.154	264	1912	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.582	112	8230	0.683	ng	0.00
5) Phenol-d6	7.199	99	8726	0.596	ng	0.00
8) Nitrobenzene-d5	9.251	82	4255	0.479	ng	-0.01
11) 2-Methylnaphthalene-d10	12.460	152	9082	0.507	ng	-0.01
14) 2,4,6-Tribromophenol	16.189	330	1371	0.692	ng	0.00
15) 2-Fluorobiphenyl	13.326	172	11229	0.552	ng	0.00
27) Fluoranthene-d10	19.463	212	19133	0.529	ng	0.00
31) Terphenyl-d14	20.048	244	12301	0.714	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027317.D
Acq On : 31 Aug 2023 20:04
Operator : MA/JU
Sample : PB155046BL
Misc :
ALS Vial : 98 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB155046BL


Quant Time: Sep 01 04:03:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 05:37:30 2023
Response via : Initial Calibration

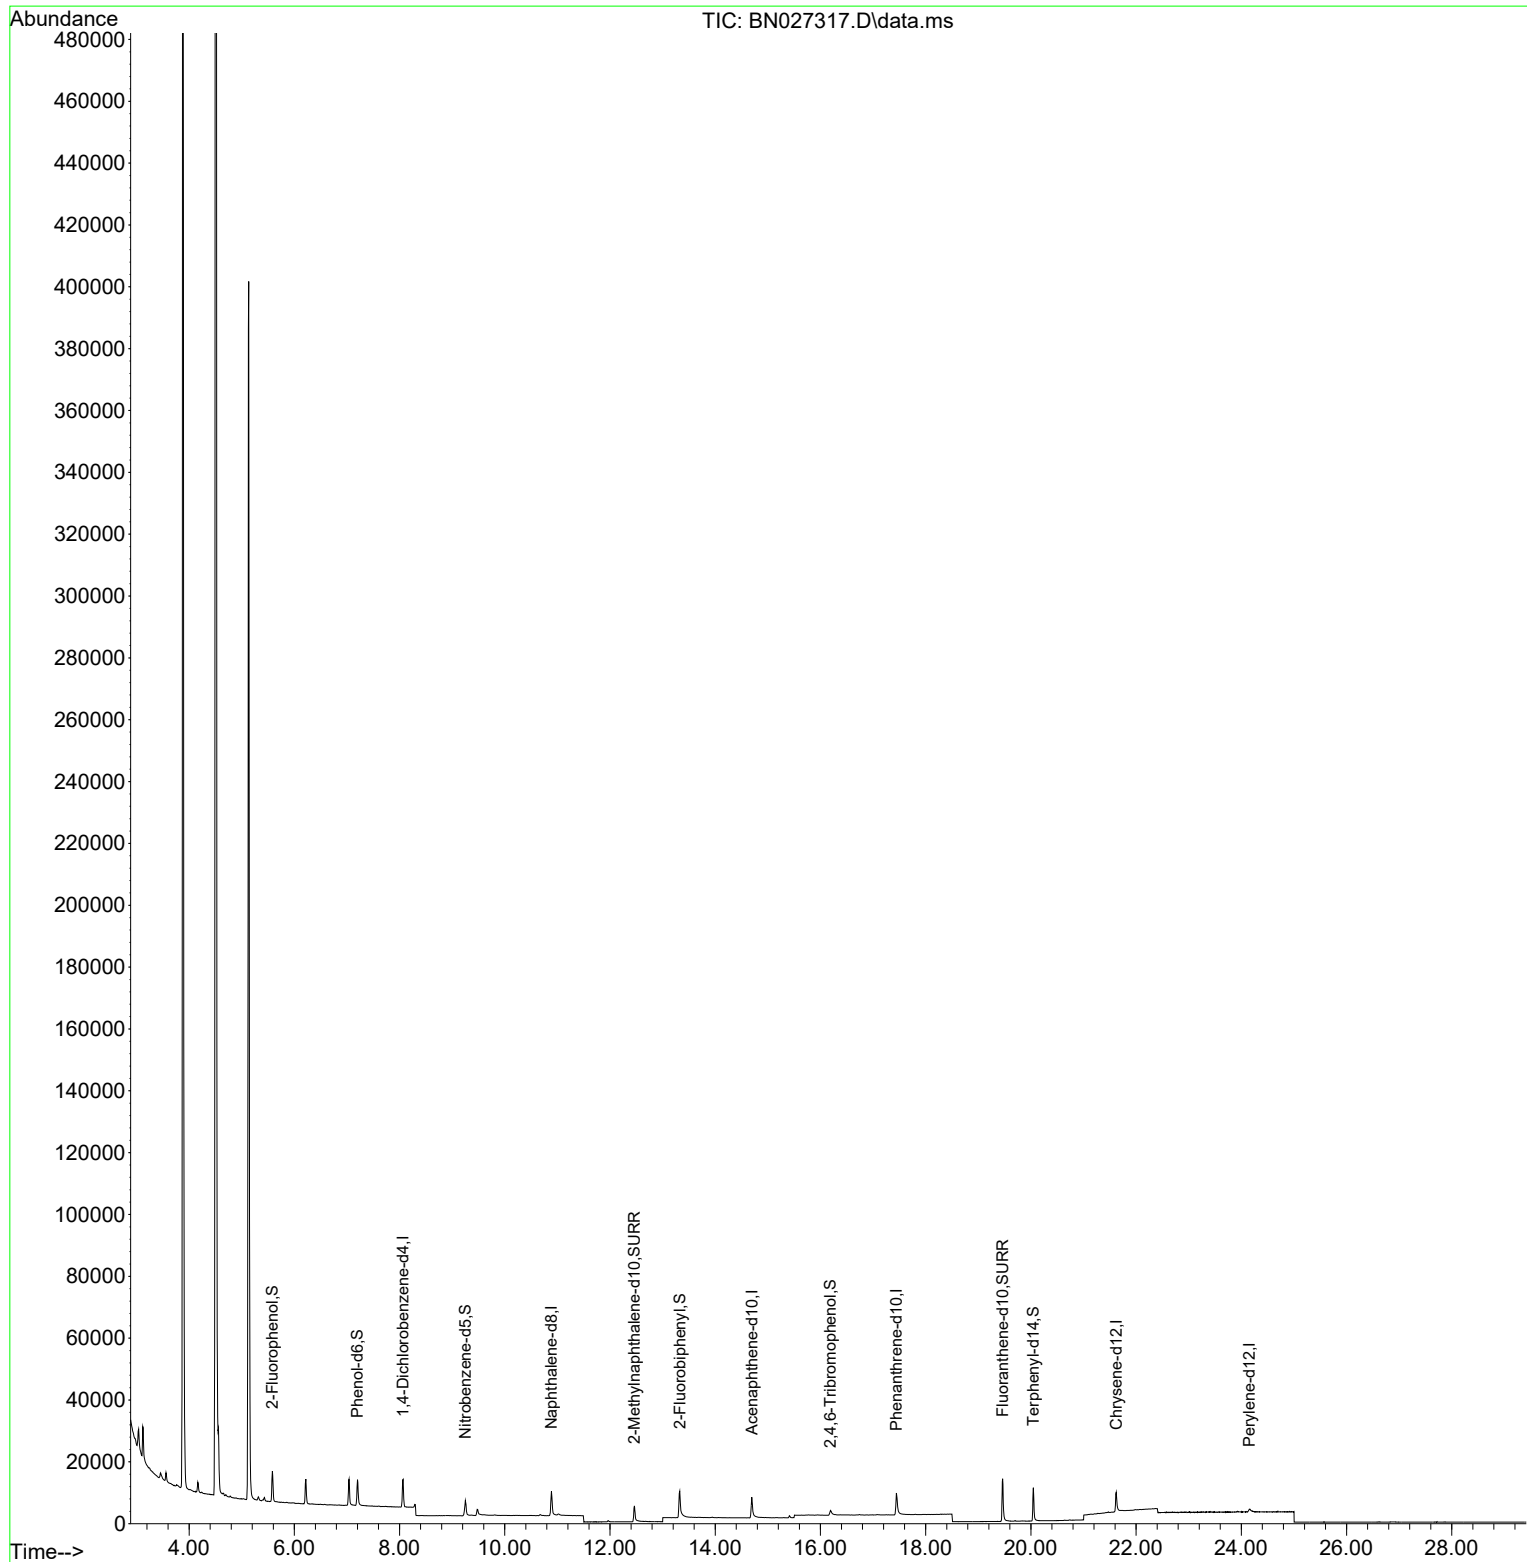






#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.066 min Scan# 719
Delta R.T. -0.007 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04

Instrument :
BNA_N
ClientSampleId :
PB155046BL







Tgt Ion:152 Resp: 4621
Ion Ratio Lower Upper
152 100
150 150.2 122.7 184.1
115 62.4 48.6 73.0

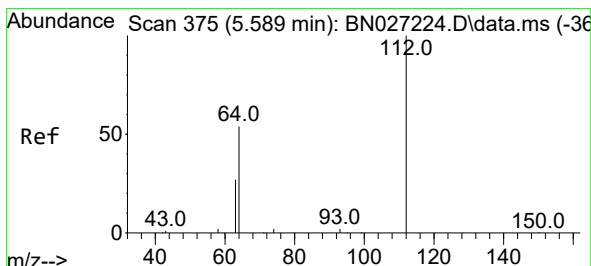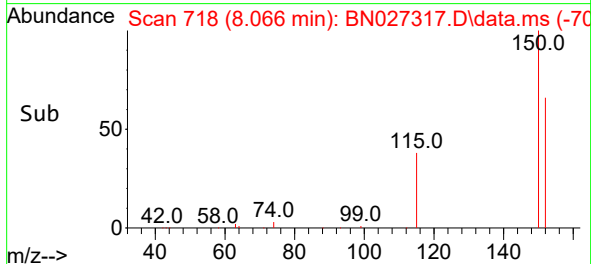

#4
2-Fluorophenol
Concen: 0.683 ng
RT: 5.582 min Scan# 374
Delta R.T. -0.007 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04

Tgt Ion:112 Resp: 8230
Ion Ratio Lower Upper
112 100
64 55.8 44.4 66.6
63 29.8 23.1 34.7


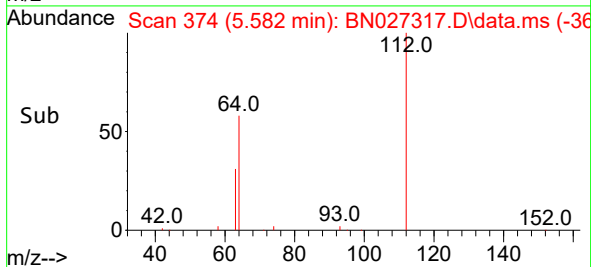

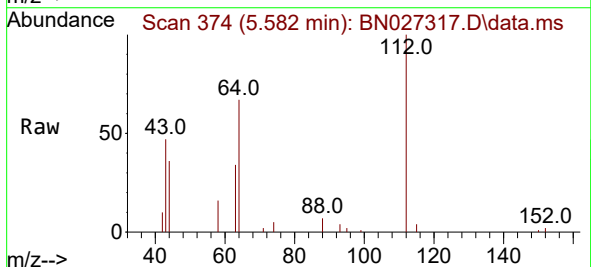


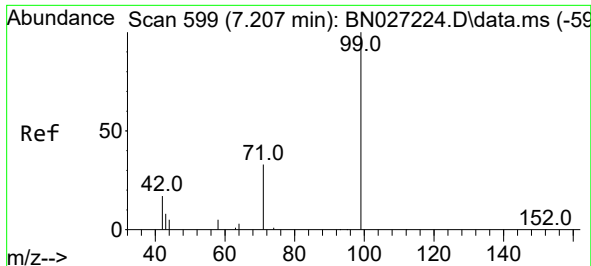

#5
Phenol-d6
Concen: 0.596 ng
RT: 7.199 min Scan# 598
Delta R.T. -0.007 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04




Instrument :
BNA_N
ClientSampleId :
PB155046BL


Tgt Ion: 99 Resp: 8726
Ion Ratio Lower Upper
99 100
42 19.2 14.5 21.7
71 33.2 25.8 38.6

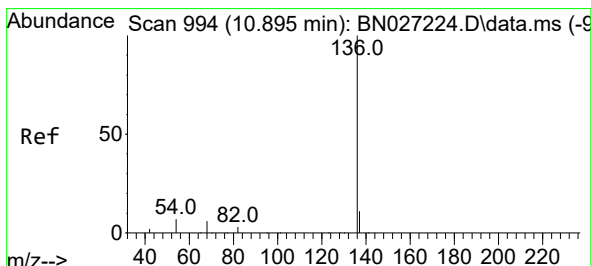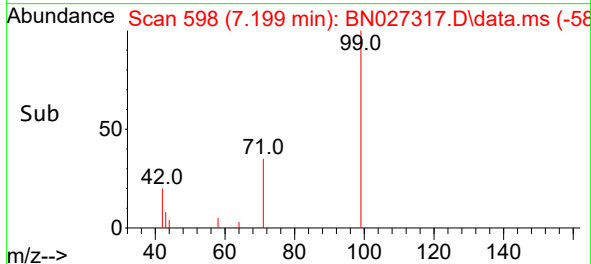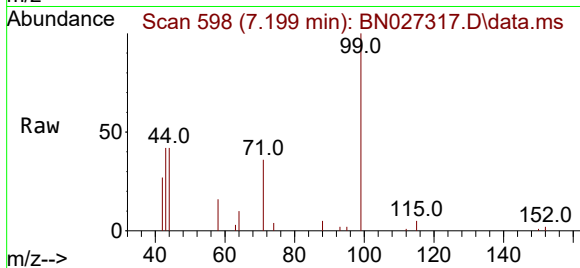

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.885 min Scan# 993
Delta R.T. -0.011 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04

Tgt Ion: 136 Resp: 12191
Ion Ratio Lower Upper
136 100
137 13.0 9.3 13.9
54 8.9 6.7 10.1
68 8.1 6.1 9.1


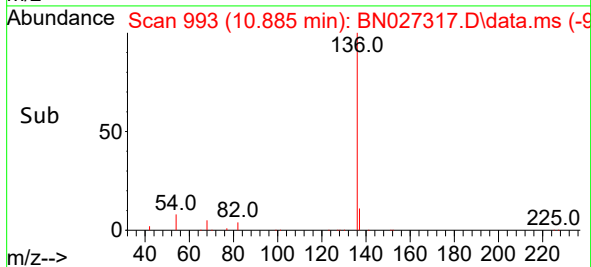

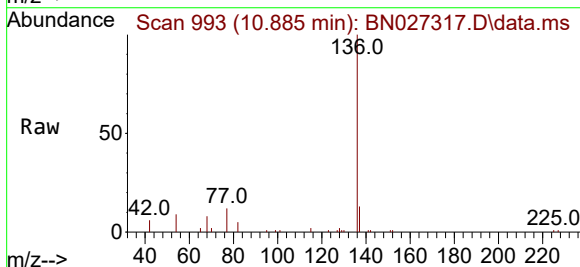


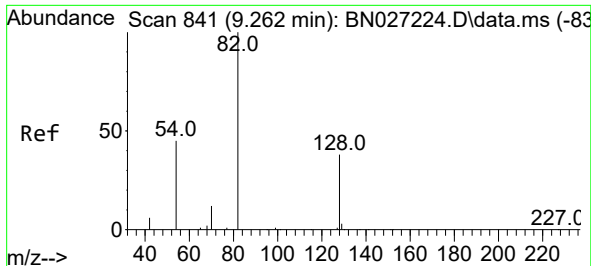

#8
Nitrobenzene-d5
Concen: 0.479 ng
RT: 9.251 min Scan# 841
Delta R.T. -0.011 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04




Instrument :
BNA_N
ClientSampleId :
PB155046BL


Tgt Ion: 82 Resp: 4255
Ion Ratio Lower Upper
82 100
128 38.0 33.4 50.0
54 50.4 37.7 56.5

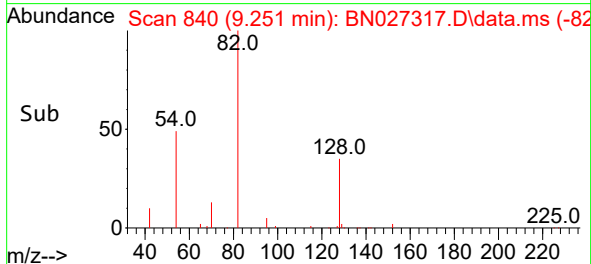

#11
2-Methylnaphthalene-d10
Concen: 0.507 ng
RT: 12.460 min Scan# 1304
Delta R.T. -0.011 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04

Tgt Ion: 152 Resp: 9082
Ion Ratio Lower Upper
152 100
151 21.3 16.6 25.0

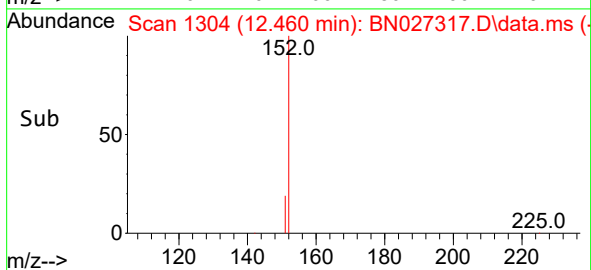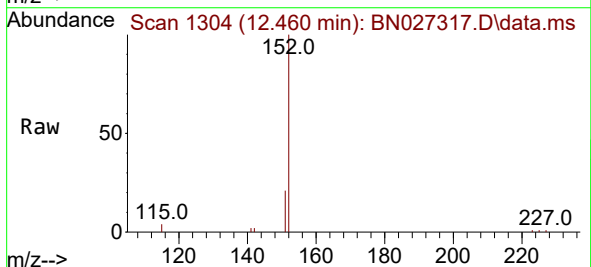



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.694 min Scan# 1606

Delta R.T. 0.000 min

Lab File: BN027317.D

Acq: 31 Aug 2023 20:04

Instrument :

BNA_N

ClientSampleId :

PB155046BL





Tgt Ion:164 Resp: 5354

Ion Ratio Lower Upper

164 100

162 105.4 85.8 128.8

160 55.7 44.2 66.2

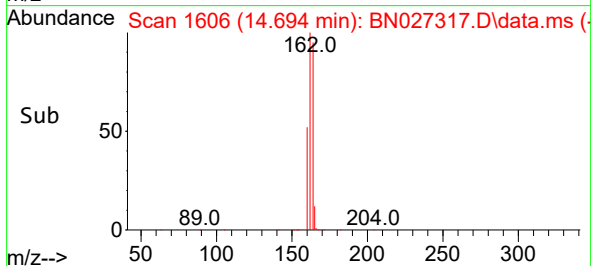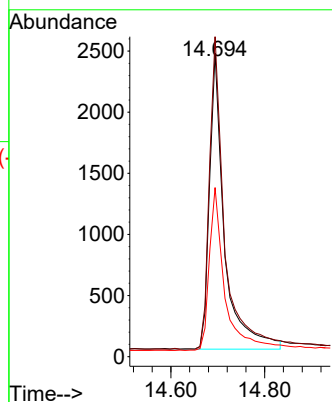

#14

2,4,6-Tribromophenol

Concen: 0.692 ng

RT: 16.189 min Scan# 1737

Delta R.T. 0.000 min

Lab File: BN027317.D

Acq: 31 Aug 2023 20:04




Tgt Ion:330 Resp: 1371


Ion Ratio Lower Upper

330 100

332 96.3 75.2 112.8

141 49.6 36.2 54.4


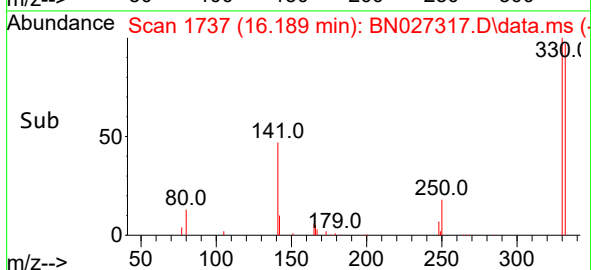

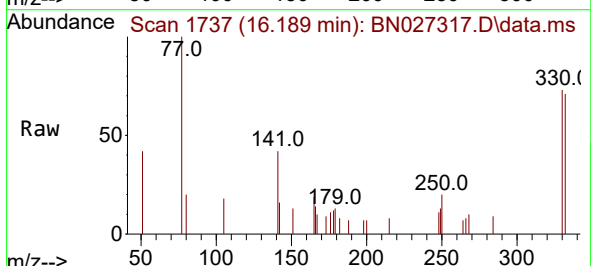


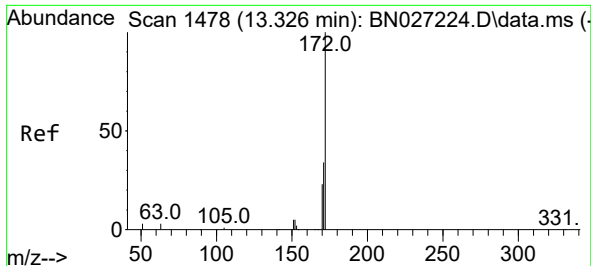

#15
2-Fluorobiphenyl
Concen: 0.552 ng
RT: 13.326 min Scan# 1478
Delta R.T. 0.000 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04




Instrument :
BNA_N
ClientSampleId :
PB155046BL


Tgt Ion:172 Resp: 11229
Ion Ratio Lower Upper
172 100
171 34.2 27.8 41.8
170 24.0 19.3 28.9

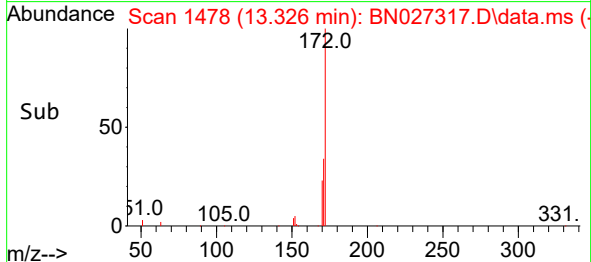

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.443 min Scan# 1838
Delta R.T. 0.000 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04

Tgt Ion:188 Resp: 14550
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.4 11.0 16.6


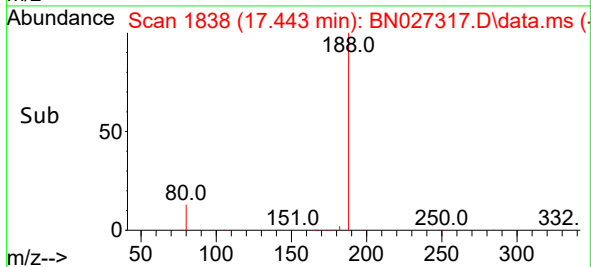

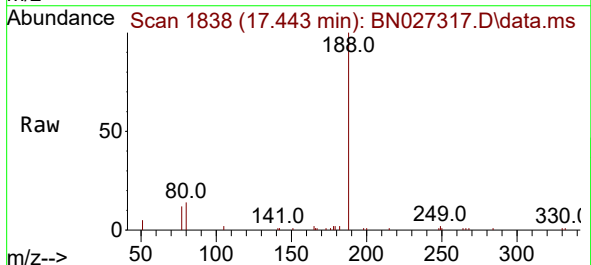


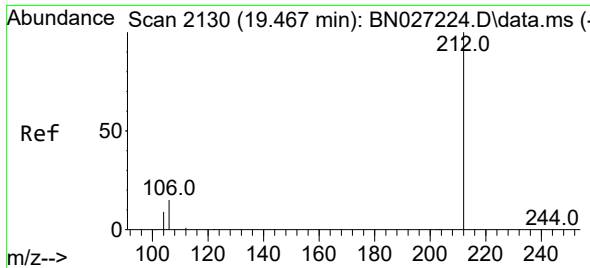

#27
Fluoranthene-d10
Concen: 0.529 ng
RT: 19.463 min Scan# 2130
Delta R.T. -0.005 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04




Instrument :
BNA_N
ClientSampleId :
PB155046BL


Tgt Ion:212 Resp: 19133
Ion Ratio Lower Upper
212 100
106 15.6 12.1 18.1
104 8.6 6.9 10.3

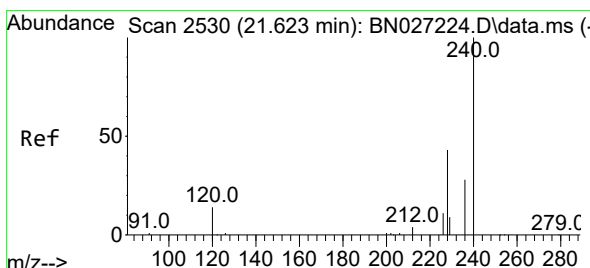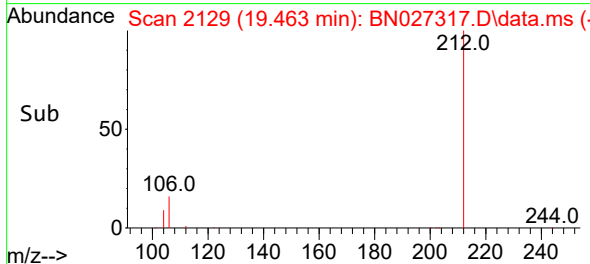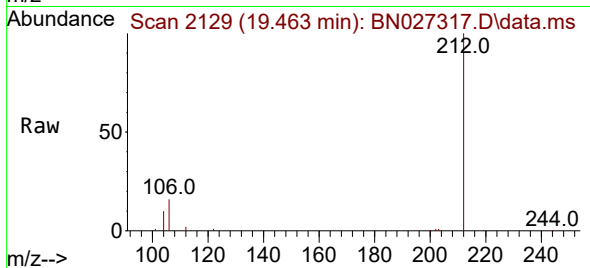

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.623 min Scan# 2530
Delta R.T. 0.000 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04

Tgt Ion:240 Resp: 8573
Ion Ratio Lower Upper
240 100
120 21.1 14.2 21.4
236 31.7 22.9 34.3


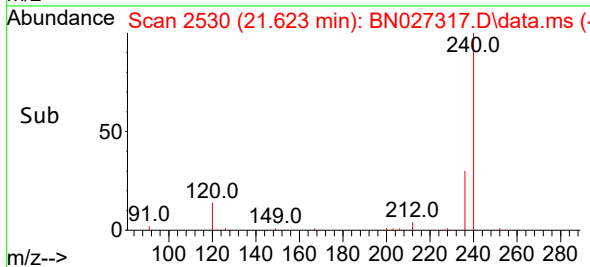

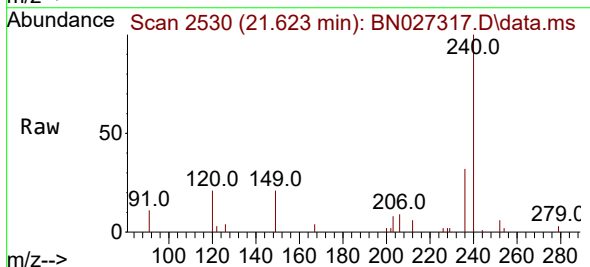




#31
Terphenyl-d14
Concen: 0.714 ng
RT: 20.048 min Scan# 21
Delta R.T. -0.005 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04

Instrument :
BNA_N
ClientSampleId :
PB155046BL

Tgt Ion:244 Resp: 12301
Ion Ratio Lower Upper
244 100
212 9.7 7.5 11.3
122 16.8 14.0 21.0

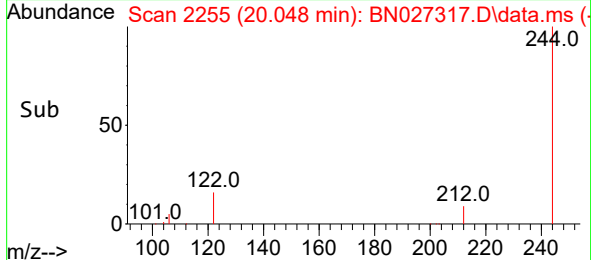

#35
Perylene-d12
Concen: 0.400 ng
RT: 24.154 min Scan# 3214
Delta R.T. -0.003 min
Lab File: BN027317.D
Acq: 31 Aug 2023 20:04

Tgt Ion:264 Resp: 1912
Ion Ratio Lower Upper
264 100
260 39.3 20.7 31.1#
265 372.7 53.3 79.9#

