


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027280.D
Acq On : 30 Aug 2023 18:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 29 05:37:30 2023

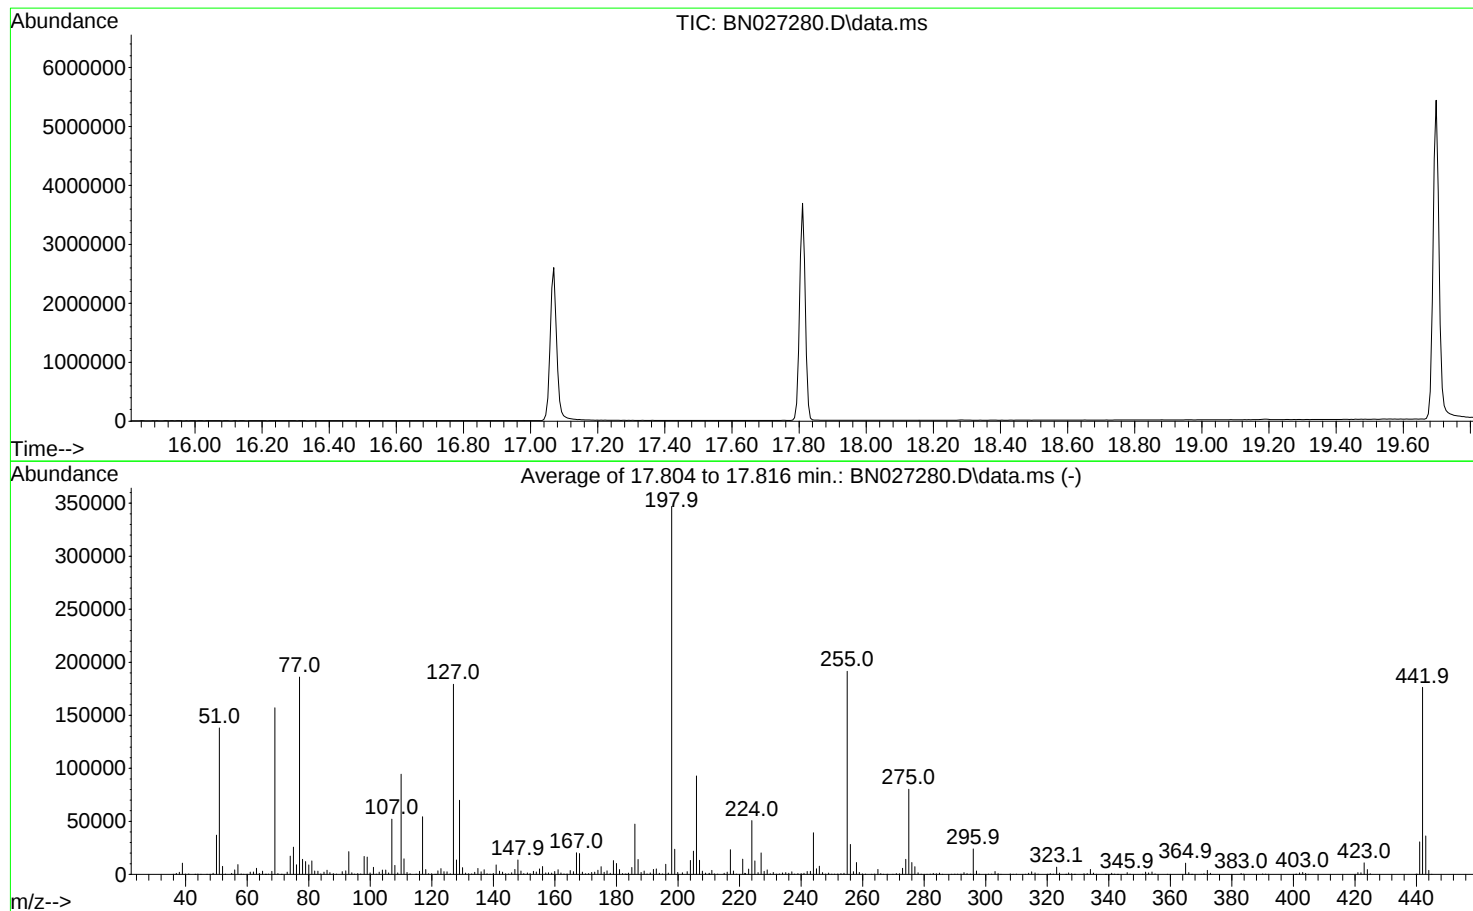




AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	138014	PASS
68	69	0.00	2	1.8	2856	PASS
69	198	0.00	100	45.3	157056	PASS
70	69	0.00	2	0.5	831	PASS
127	198	10	80	51.7	179243	PASS
197	198	0.00	2	0.4	1219	PASS
198	198	100	100	100.0	346901	PASS
199	198	5	9	6.8	23739	PASS
275	198	10	60	23.1	80208	PASS
365	198	1	100	3.0	10515	PASS
441	198	0.01	100	8.8	30696	PASS
442	442	50	100	100.0	176384	PASS
443	442	15	24	20.5	36187	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027280.D
Acq On : 30 Aug 2023 18:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 31 06:33:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 06:24:29 2023
Response via : Initial Calibration

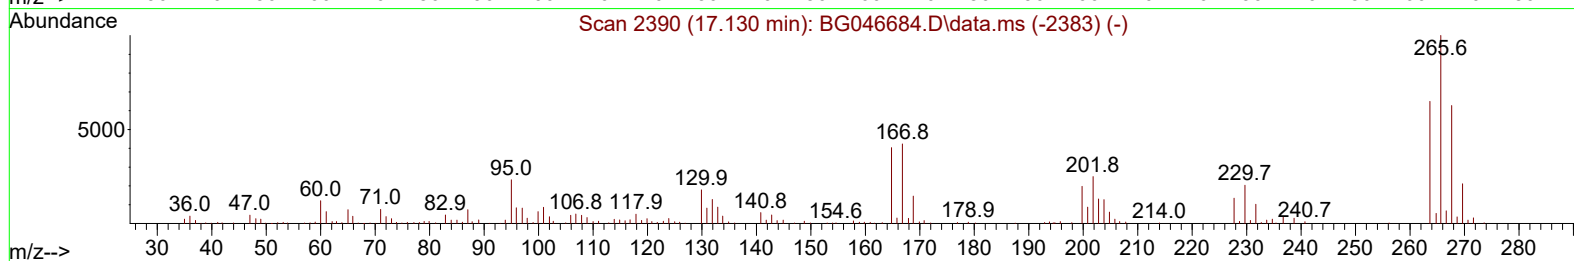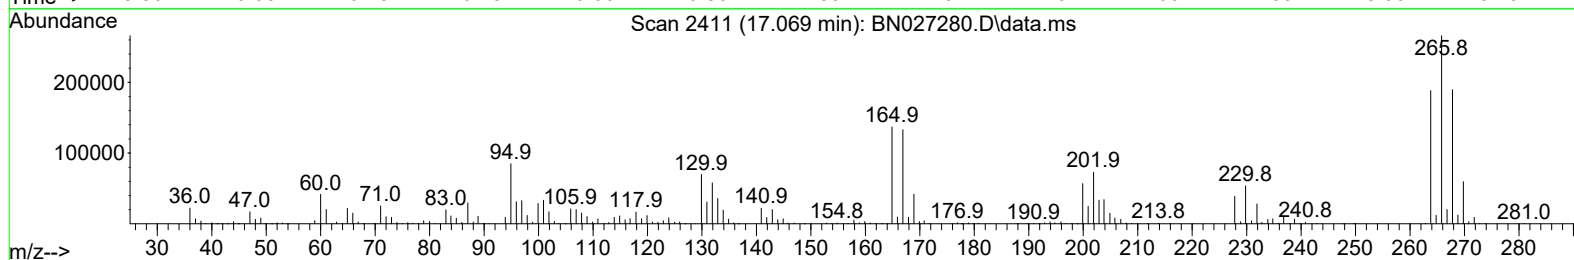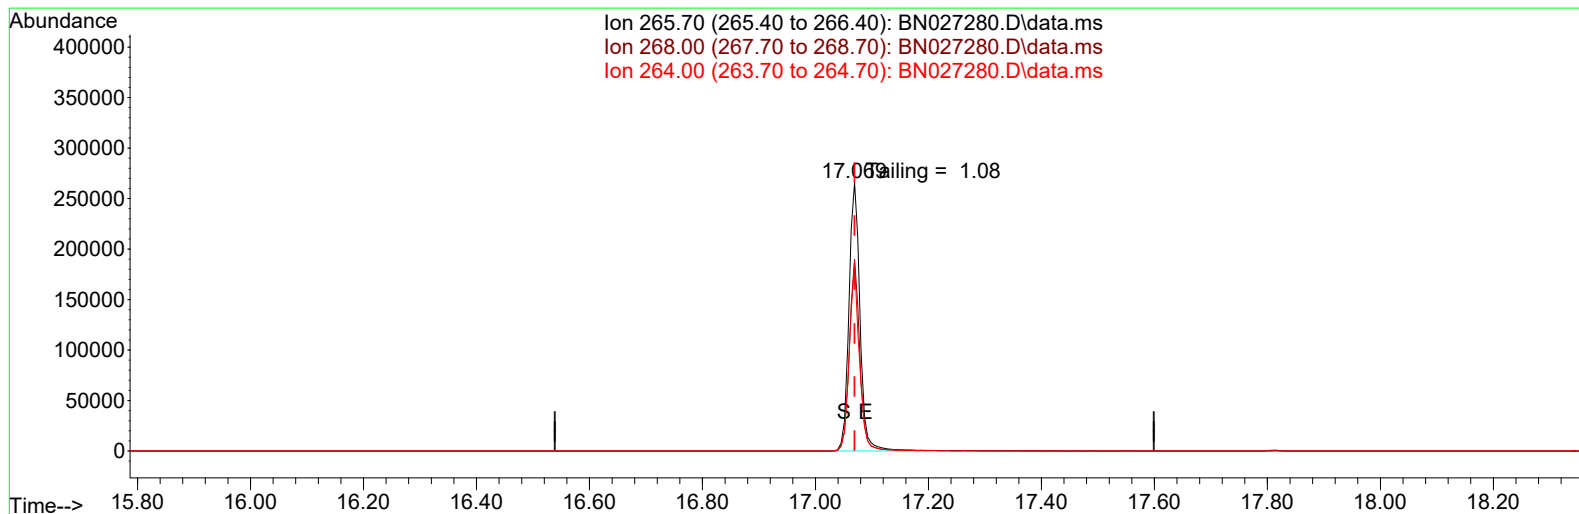

TIC: BN027280.D\data.ms

(70) Pentachlorophenol (C)

17.069min (+ 0.000) 19463.02 ng

response 363676

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.35
264.00	61.60	70.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/30/2023	BNA_N	<u>BN027280.D</u>
Compound Name	Response	Retention Time
DDT	1231744	20.892
DDD	17832	20.451
DDE	1090	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18922	1250666	1.51

Instrument :
BNA_N
ClientSampleId :
DFTPP