


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027297.D
Acq On : 31 Aug 2023 06:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 29 05:37:30 2023

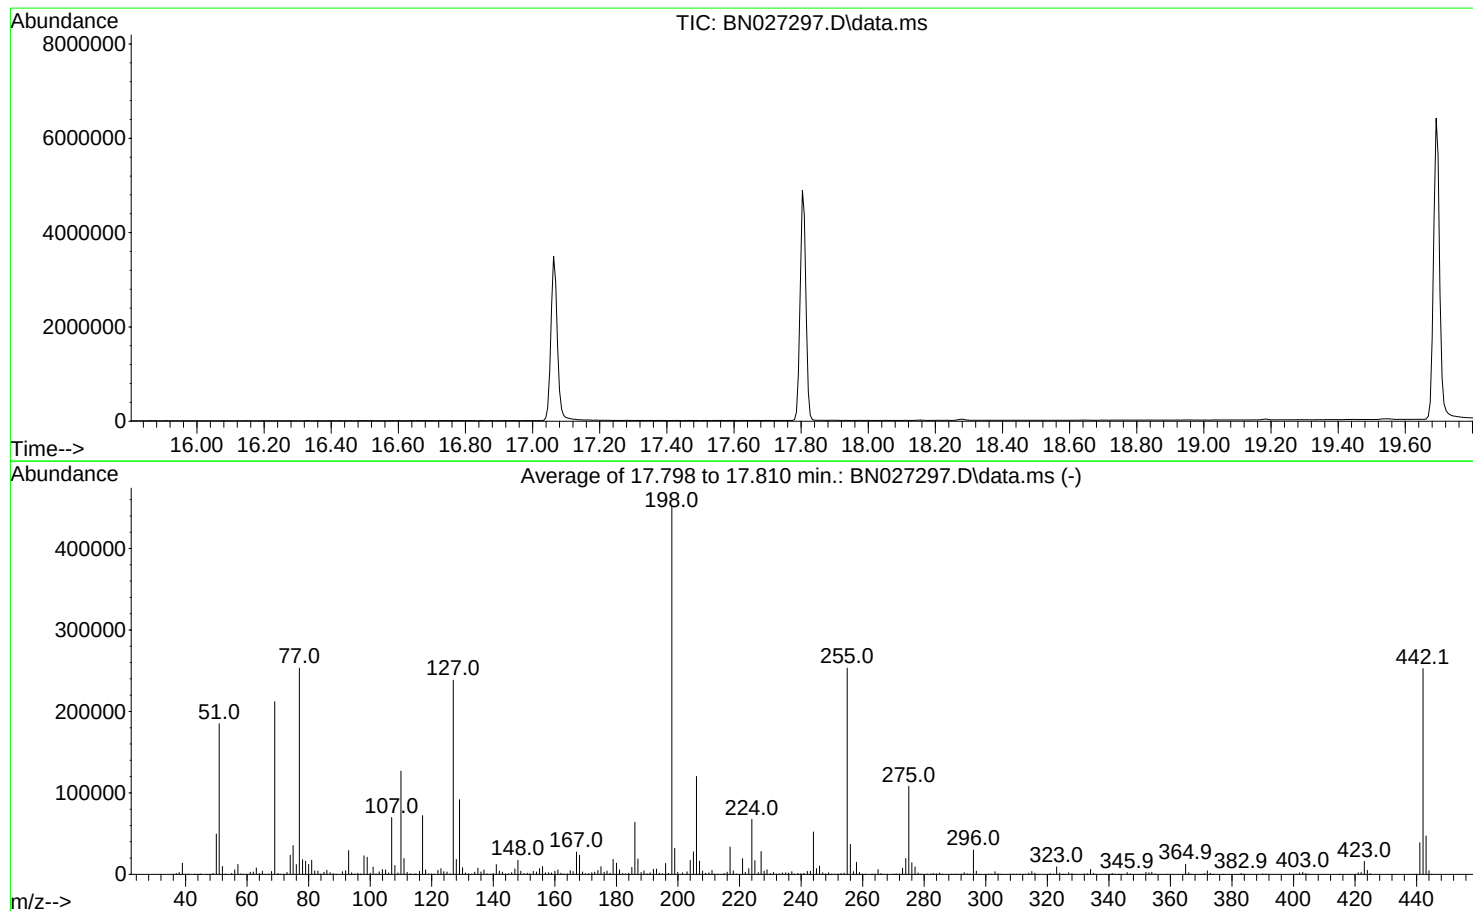




AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	184994	PASS
68	69	0.00	2	1.7	3542	PASS
69	198	0.00	100	46.9	211861	PASS
70	69	0.00	2	0.5	1110	PASS
127	198	10	80	52.8	238208	PASS
197	198	0.00	2	0.3	1463	PASS
198	198	100	100	100.0	451541	PASS
199	198	5	9	7.1	31941	PASS
275	198	10	60	23.9	107992	PASS
365	198	1	100	2.8	12454	PASS
441	198	0.01	100	8.6	38811	PASS
442	442	50	100	100.0	252496	PASS
443	442	15	24	18.7	47213	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
 Data File : BN027297.D
 Acq On : 31 Aug 2023 06:58
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 31 07:53:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 31 07:53:42 2023
 Response via : Initial Calibration

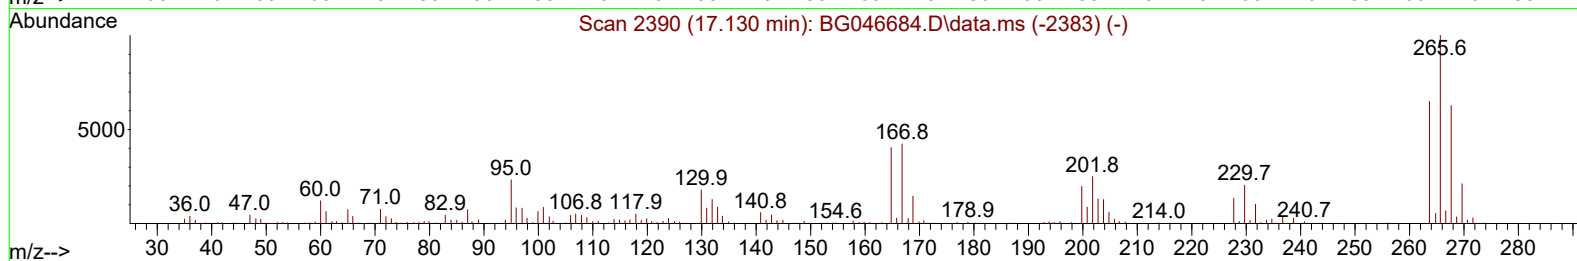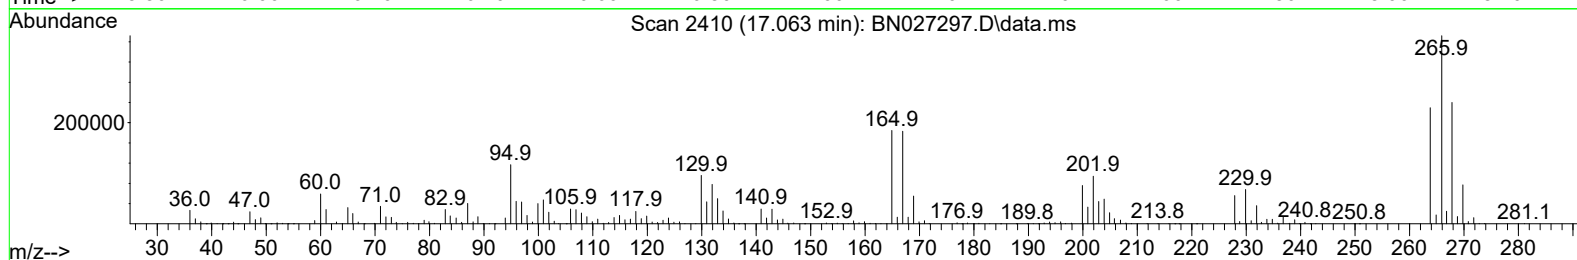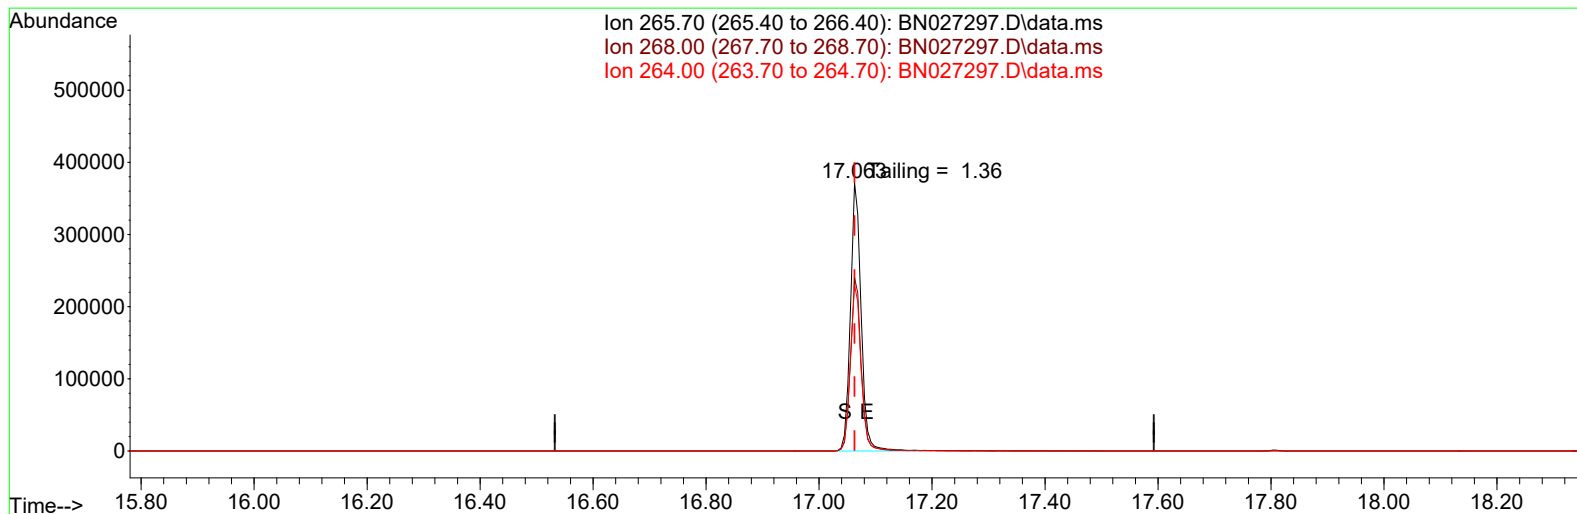

TIC: BN027297.D\data.ms

(70) Pentachlorophenol (C)

17.063min (0.000) 19323.70 ng




response 488305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.53
264.00	61.60	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
 Data File : BN027297.D
 Acq On : 31 Aug 2023 06:58
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 31 07:53:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 31 07:53:42 2023
 Response via : Initial Calibration

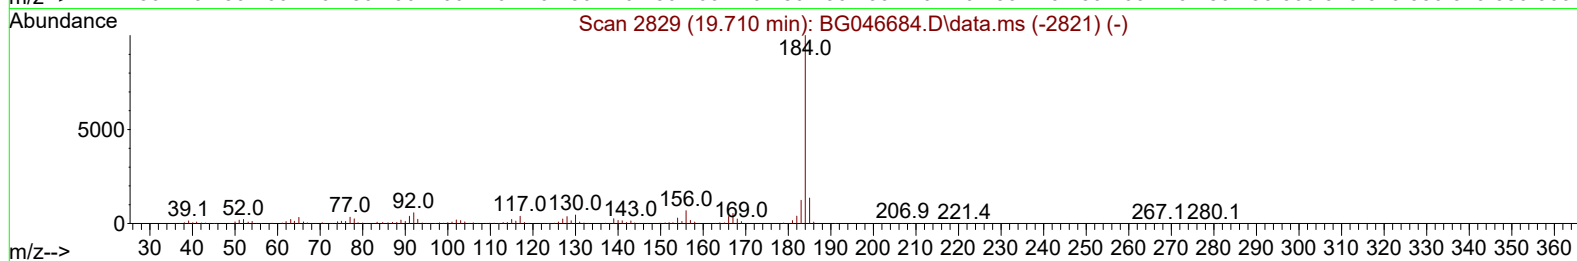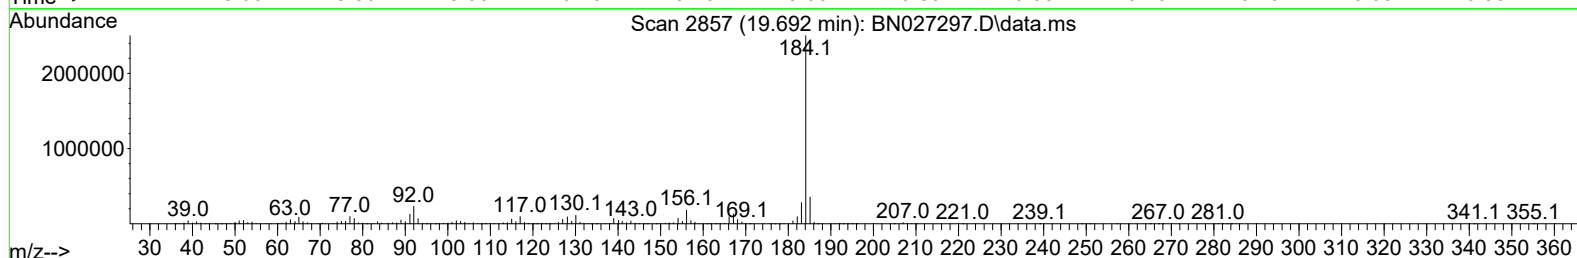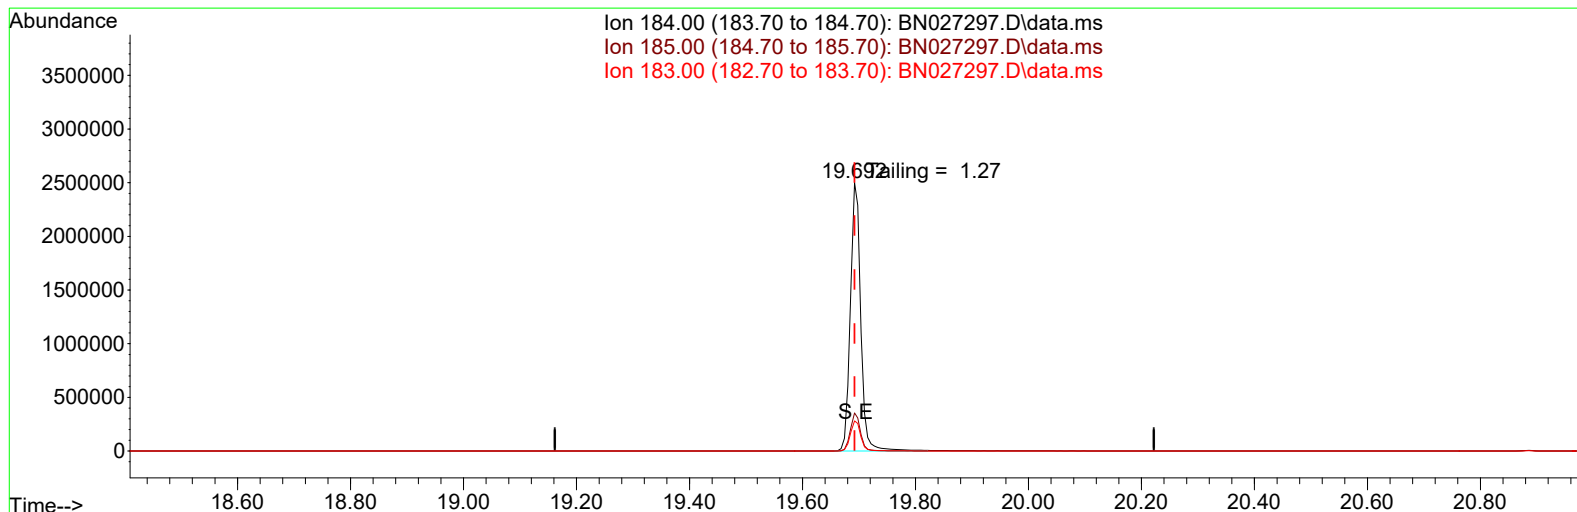

TIC: BN027297.D\data.ms

(77) Benzidine

19.692min (0.000) 0.00 ng

response 3226036

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.19
183.00	13.20	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/30/2023	BNA_N	<u>BN027297.D</u>
Compound Name	Response	Retention Time
DDT	3052686	20.886
DDD	120546	20.445
DDE	3214	19.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
123760	3176446	3.90

Instrument :
BNA_N
ClientSampleId :
DFTPP