


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
 Data File : BN027315.D
 Acq On : 31 Aug 2023 18:13
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 01 09:08:53 2023

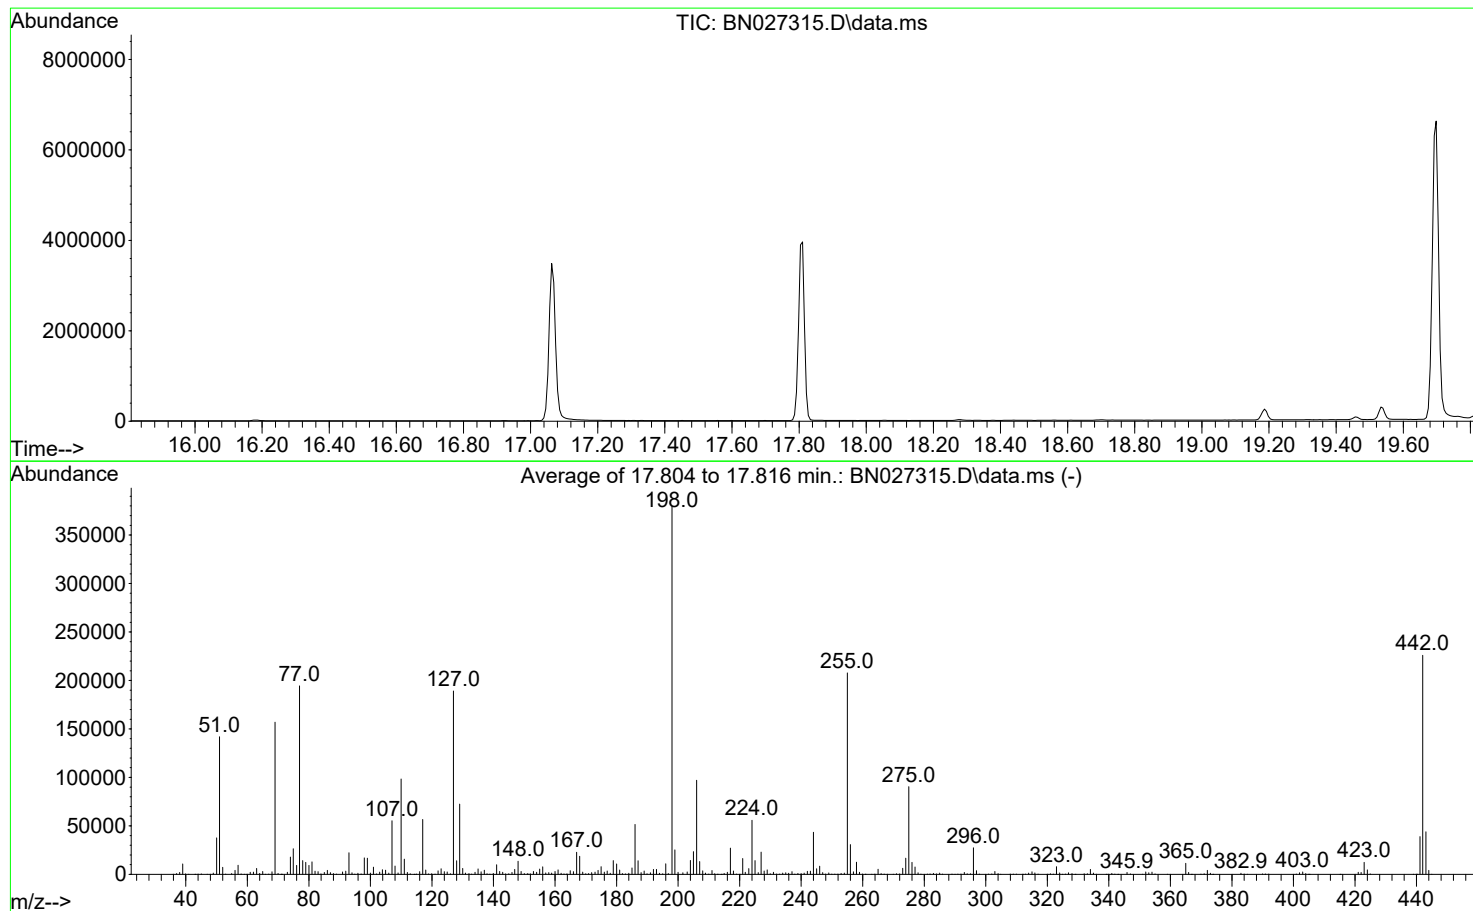




AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	142008	PASS
68	69	0.00	2	1.7	2612	PASS
69	198	0.00	100	41.4	156955	PASS
70	69	0.00	2	0.6	993	PASS
127	198	10	80	49.8	189099	PASS
197	198	0.00	2	0.2	796	PASS
198	198	100	100	100.0	379413	PASS
199	198	5	9	6.7	25304	PASS
275	198	10	60	23.8	90445	PASS
365	198	1	100	3.0	11416	PASS
441	198	0.01	100	10.3	38973	PASS
442	442	50	100	100.0	226005	PASS
443	442	15	24	19.4	43891	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
Data File : BN027315.D
Acq On : 31 Aug 2023 18:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 01 07:34:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 01 07:34:32 2023
Response via : Initial Calibration

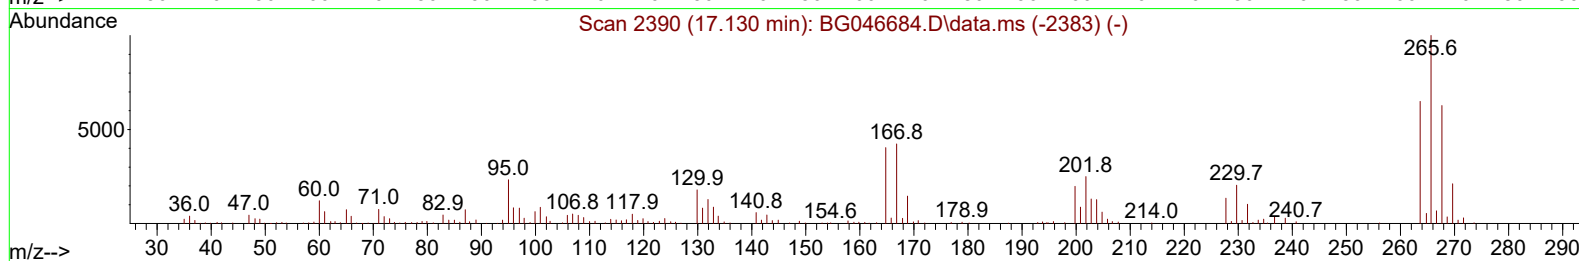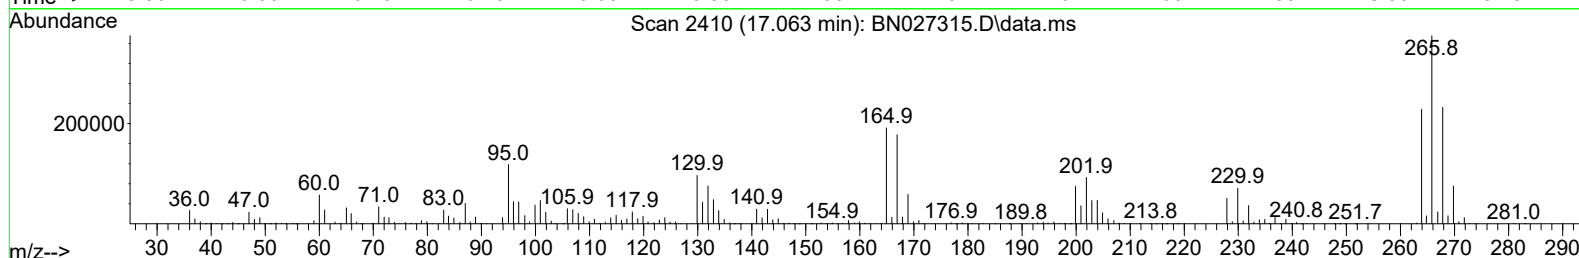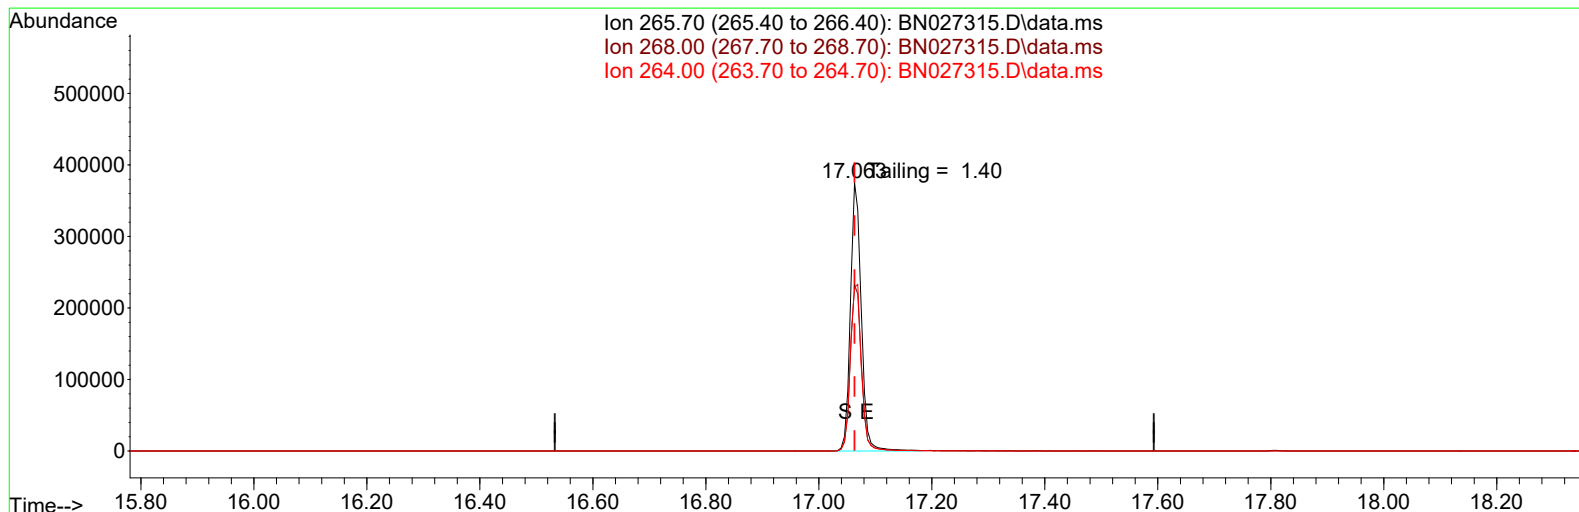

TIC: BN027315.D\data.ms

(70) Pentachlorophenol (C)

17.063min (0.000) 24062.34 ng




response 502868

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.97
264.00	61.60	60.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
 Data File : BN027315.D
 Acq On : 31 Aug 2023 18:13
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 01 07:34:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 01 07:34:32 2023
 Response via : Initial Calibration

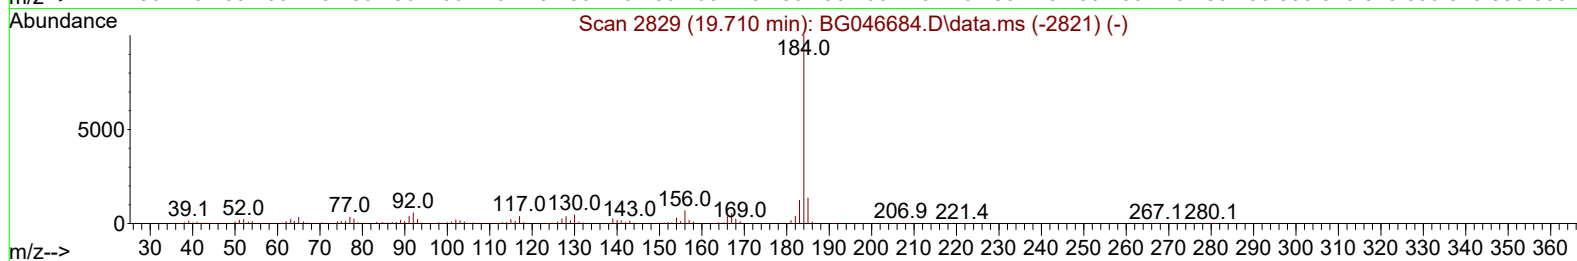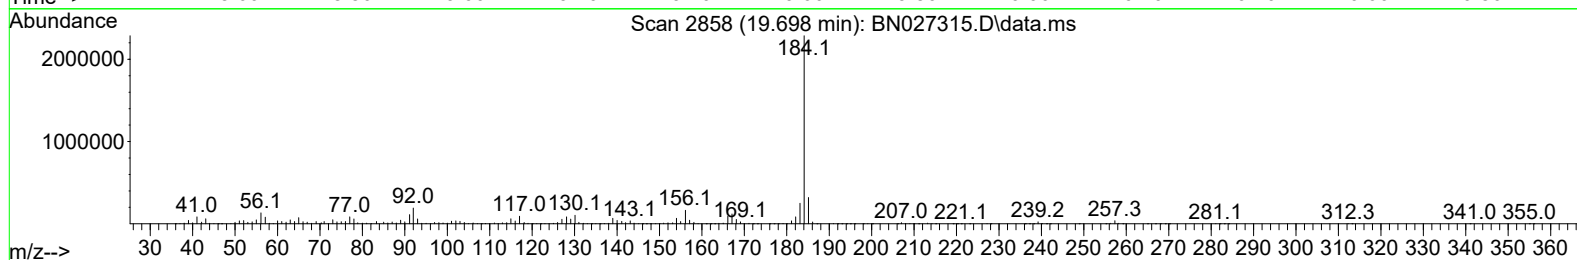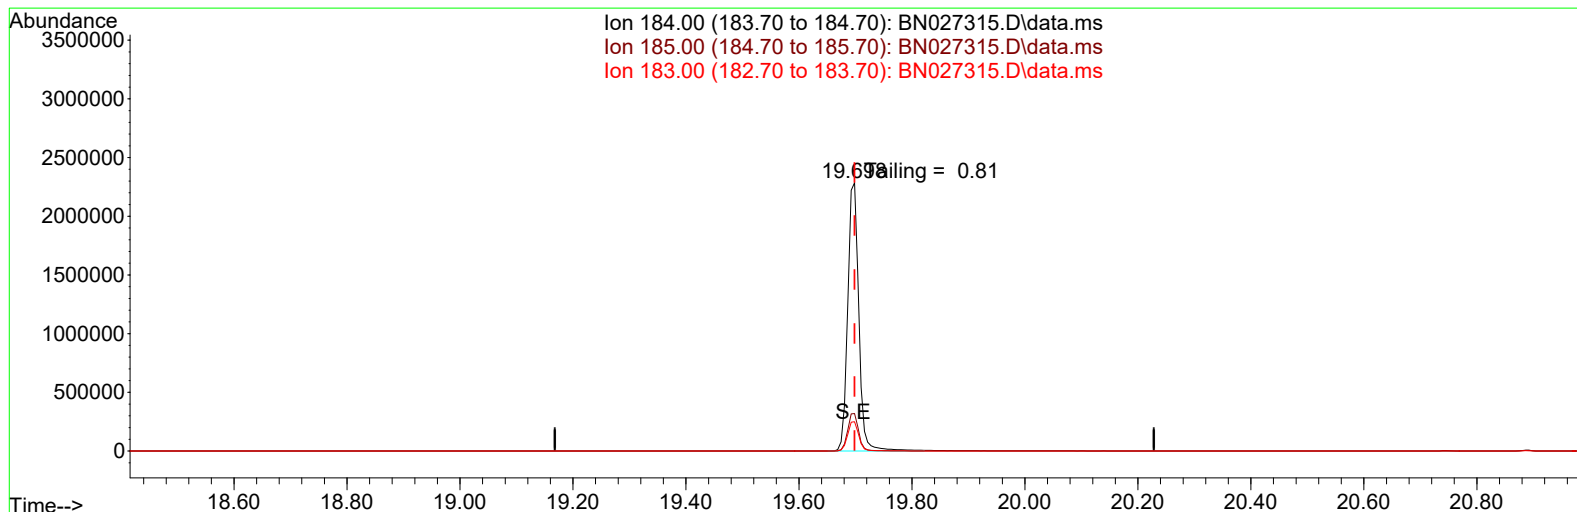

TIC: BN027315.D\data.ms

(77) Benzidine

19.698min (0.000) 1414918.68 ng

response 3096693

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	10.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/30/2023	BNA_N	<u>BN027315.D</u>
Compound Name	Response	Retention Time
DDT	1749186	20.886
DDD	21999	20.451
DDE	1184	19.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23183	1772369	1.31

Instrument :
BNA_N
ClientSampleId :
DFTPP