
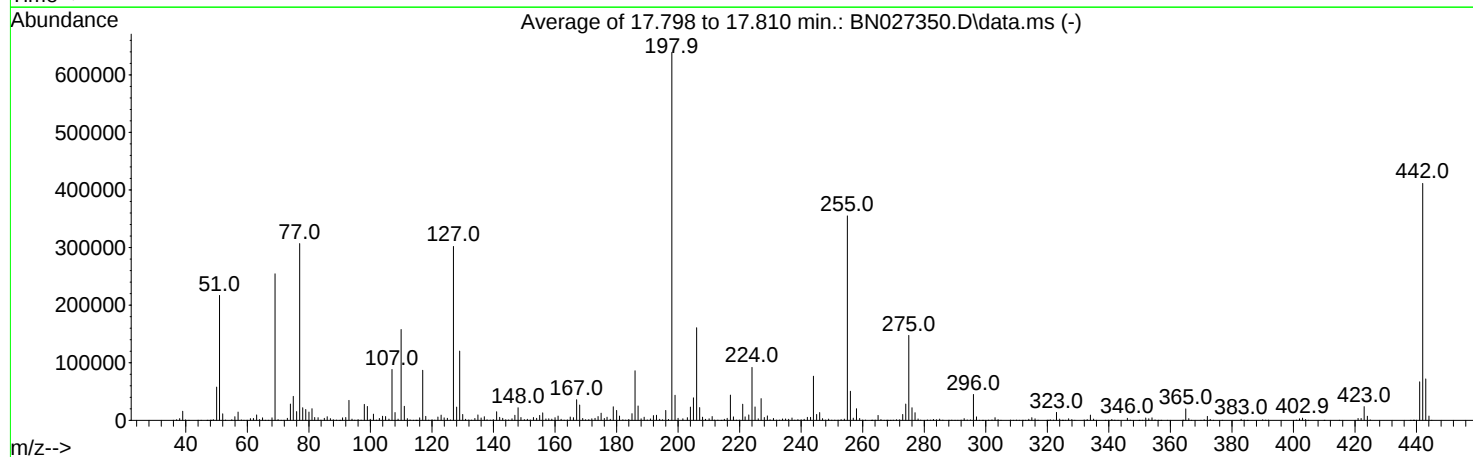


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
 Data File : BN027350.D
 Acq On : 01 Sep 2023 17:57
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 131 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 01 09:08:53 2023

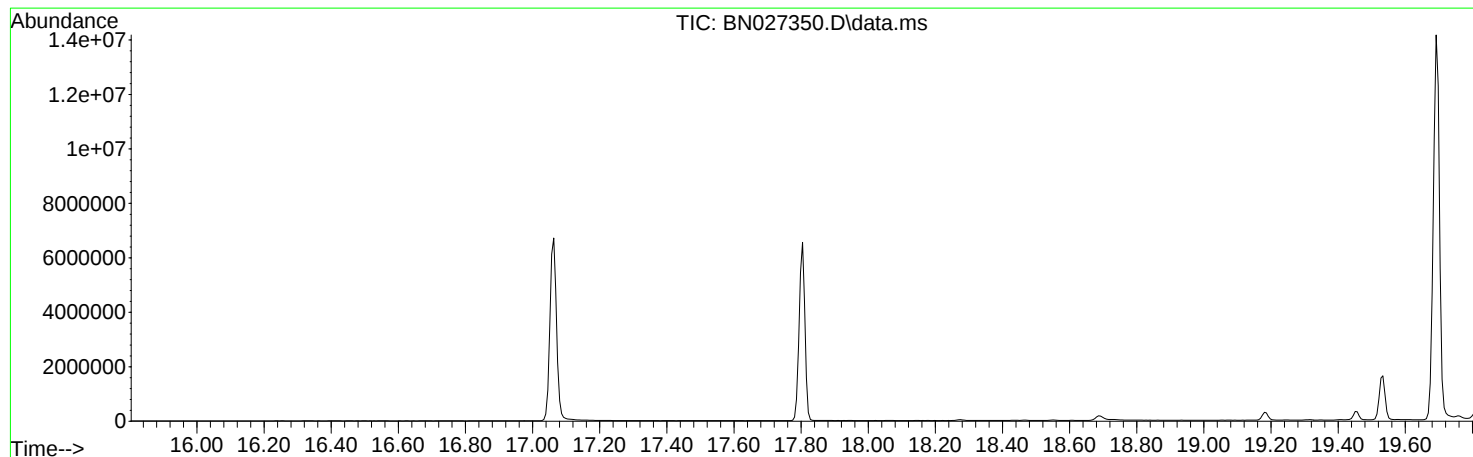




AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	216976	PASS
68	69	0.00	2	1.7	4320	PASS
69	198	0.00	100	39.9	254623	PASS
70	69	0.00	2	0.5	1301	PASS
127	198	10	80	47.3	302080	PASS
197	198	0.00	2	0.3	1739	PASS
198	198	100	100	100.0	638805	PASS
199	198	5	9	6.8	43571	PASS
275	198	10	60	23.1	147547	PASS
365	198	1	100	3.1	19949	PASS
441	198	0.01	100	10.5	67120	PASS
442	442	50	100	100.0	411627	PASS
443	442	15	24	17.5	72061	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
 Data File : BN027350.D
 Acq On : 01 Sep 2023 17:57
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 131 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 02 04:36:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 04:36:41 2023
 Response via : Initial Calibration

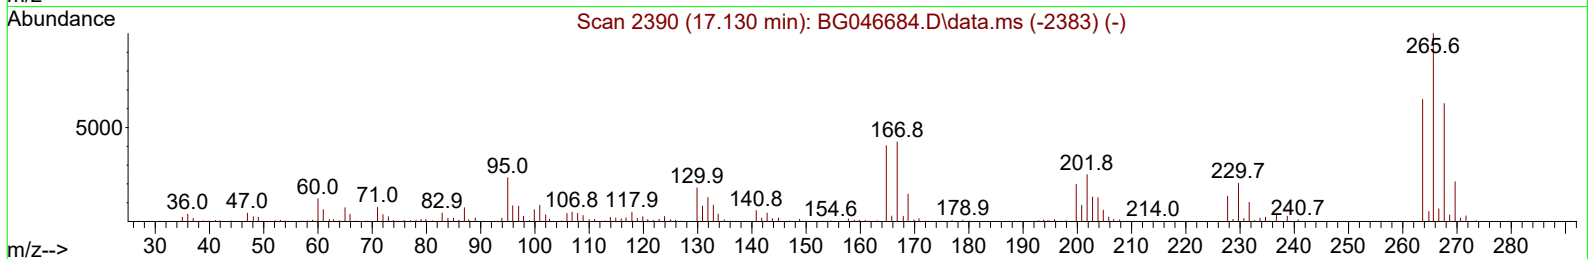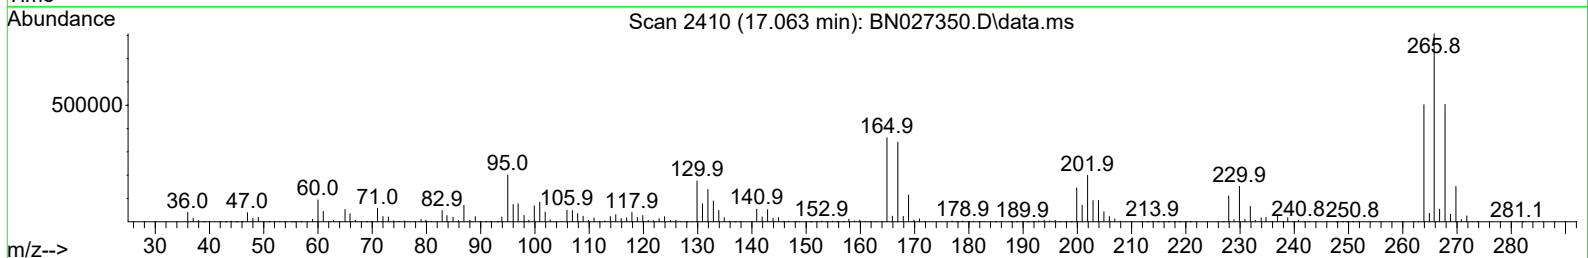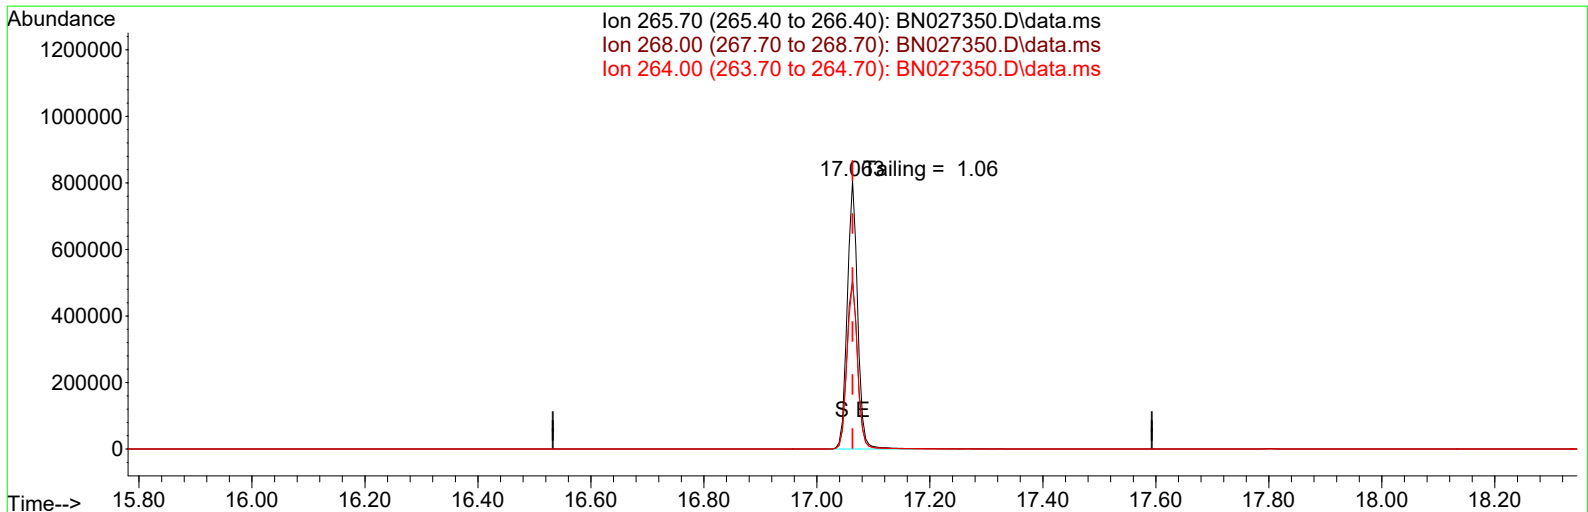

TIC: BN027350.D\data.ms

(70) Pentachlorophenol (C)

17.063min (0.000) 32606.02 ng




response 1033003

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.47
264.00	61.60	62.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083023\
 Data File : BN027350.D
 Acq On : 01 Sep 2023 17:57
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 131 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 02 04:36:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 04:36:41 2023
 Response via : Initial Calibration

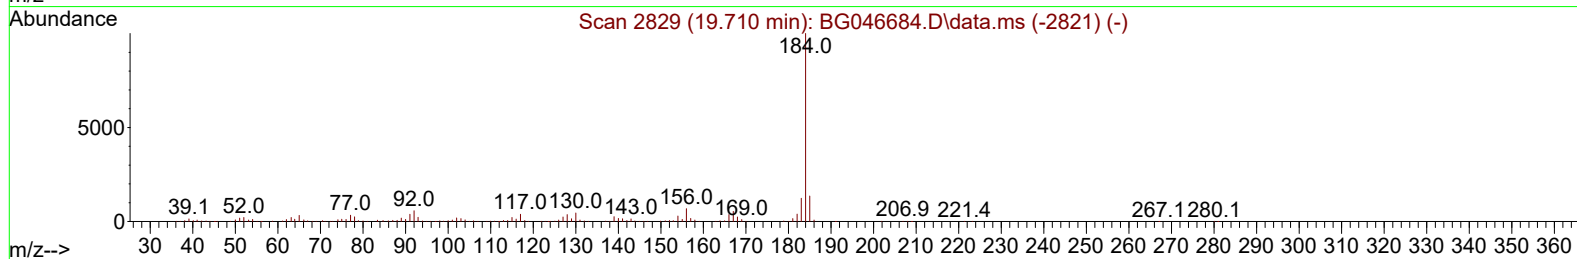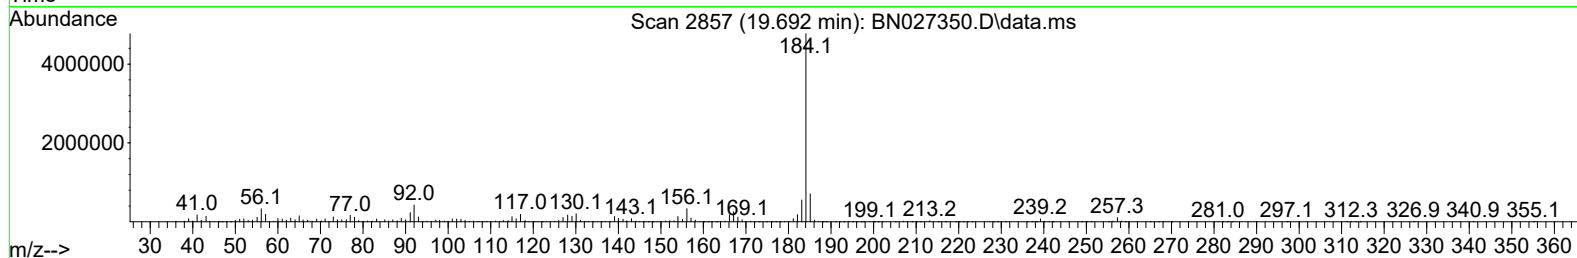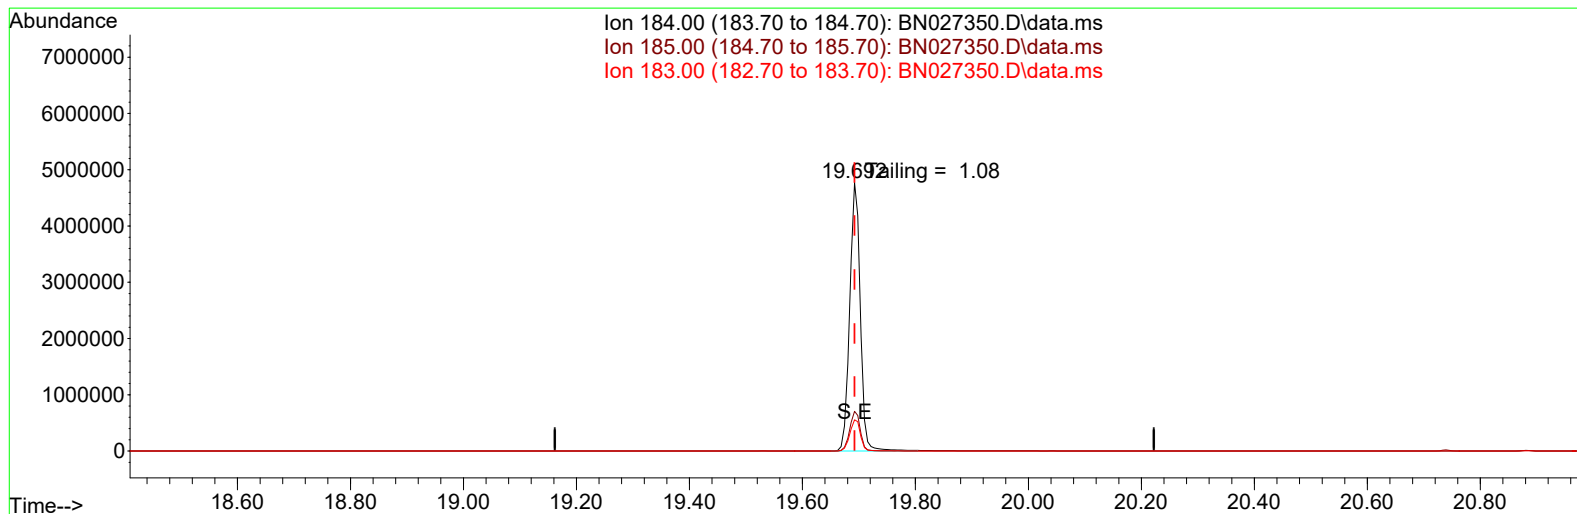

TIC: BN027350.D\data.ms

(77) Benzidine

19.692min (0.000) 296839.97 ng

response 6194687

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.81
183.00	13.20	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/30/2023	BNA_N	<u>BN027350.D</u>
Compound Name	Response	Retention Time
DDT	2935165	20.886
DDD	104120	20.445
DDE	2611	19.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
106731	3041896	3.51

Instrument :
BNA_N
ClientSampleId :
DFTPP