


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN090119\
 Data File : BN007526.D
 Acq On : 01 Sep 2019 14:57
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 29 12:18:45 2019

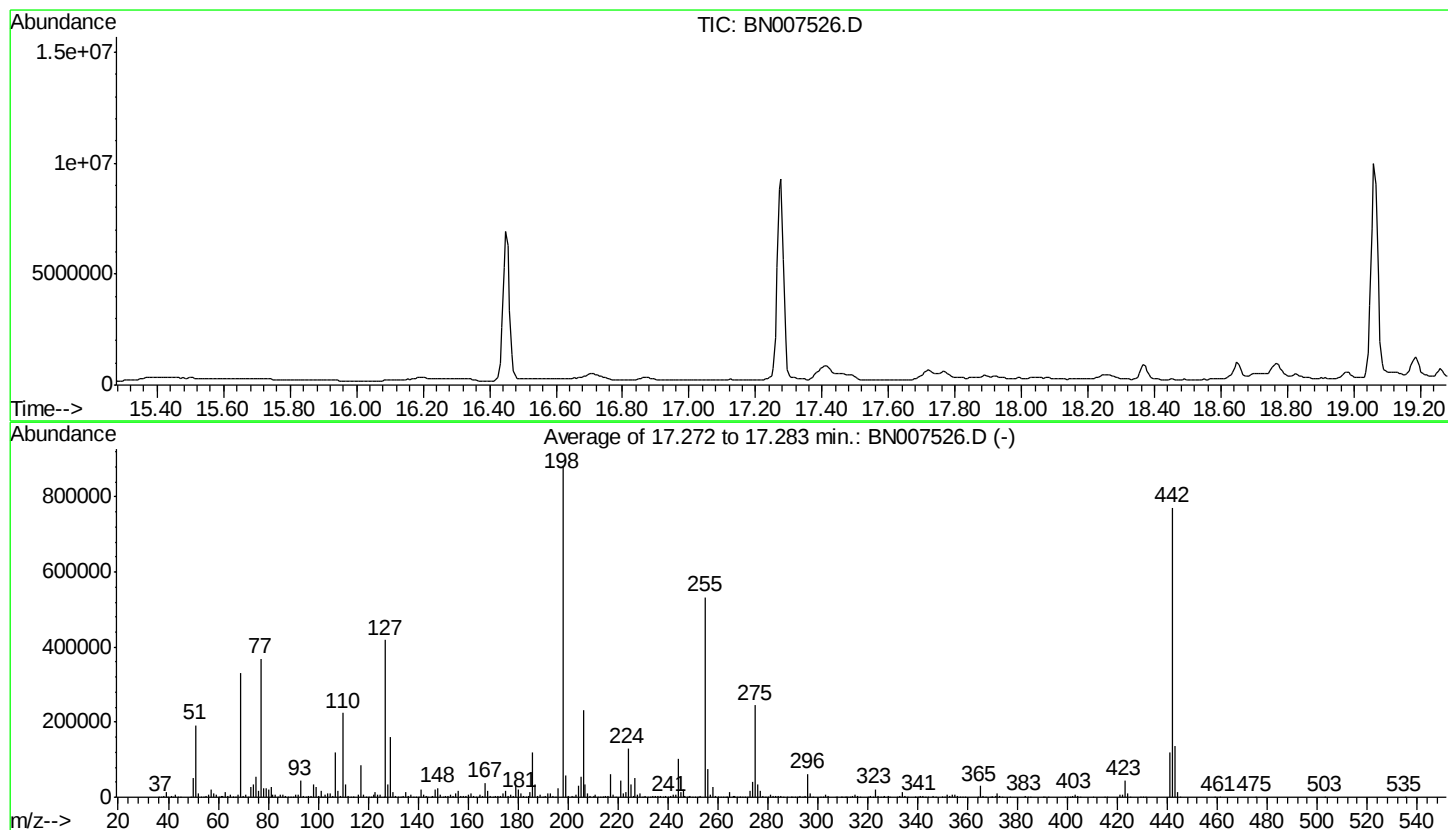

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.8	192827	PASS
68	69	0.00	2	2.0	6612	PASS
69	198	0.00	100	37.5	331606	PASS
70	69	0.00	2	0.6	1953	PASS
127	198	10	80	47.4	418664	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	883568	PASS
199	198	5	9	6.8	59741	PASS
275	198	10	60	27.7	244650	PASS
365	198	1	100	3.3	29162	PASS
441	198	0.01	100	13.6	120560	PASS
442	198	50	100	87.4	772522	PASS
443	442	15	24	17.8	137501	PASS