

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090221\
 Data File : BN016146.D
 Acq On : 02 Sep 2021 20:33
 Operator : CG/JU
 Sample : M3518-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B85

Quant Time: Sep 03 02:19:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 02 13:32:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.871	152	2876	0.400	ng/ul	0.00
4) Naphthalene-d8	10.666	136	12190	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.506	164	7376	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.255	188	14737	0.400	ng/ul	0.00
17) Chrysene-d12	21.445	240	14393	0.400	ng/ul	0.00
23) Perylene-d12	23.842	264	14527	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	12911	3.857	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.261	152	5545	0.323	ng/ul	0.00
18) Fluoranthene-d10	19.285	212	15501	0.401	ng/ul	0.00
Target Compounds						
10) Acenaphthylene	14.224	152	1006	0.036	ng/ul#	Qvalue 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090221\
Data File : BN016146.D
Acq On : 02 Sep 2021 20:33
Operator : CG/JU
Sample : M3518-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B85


Quant Time: Sep 03 02:19:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 02 13:32:21 2021
Response via : Initial Calibration

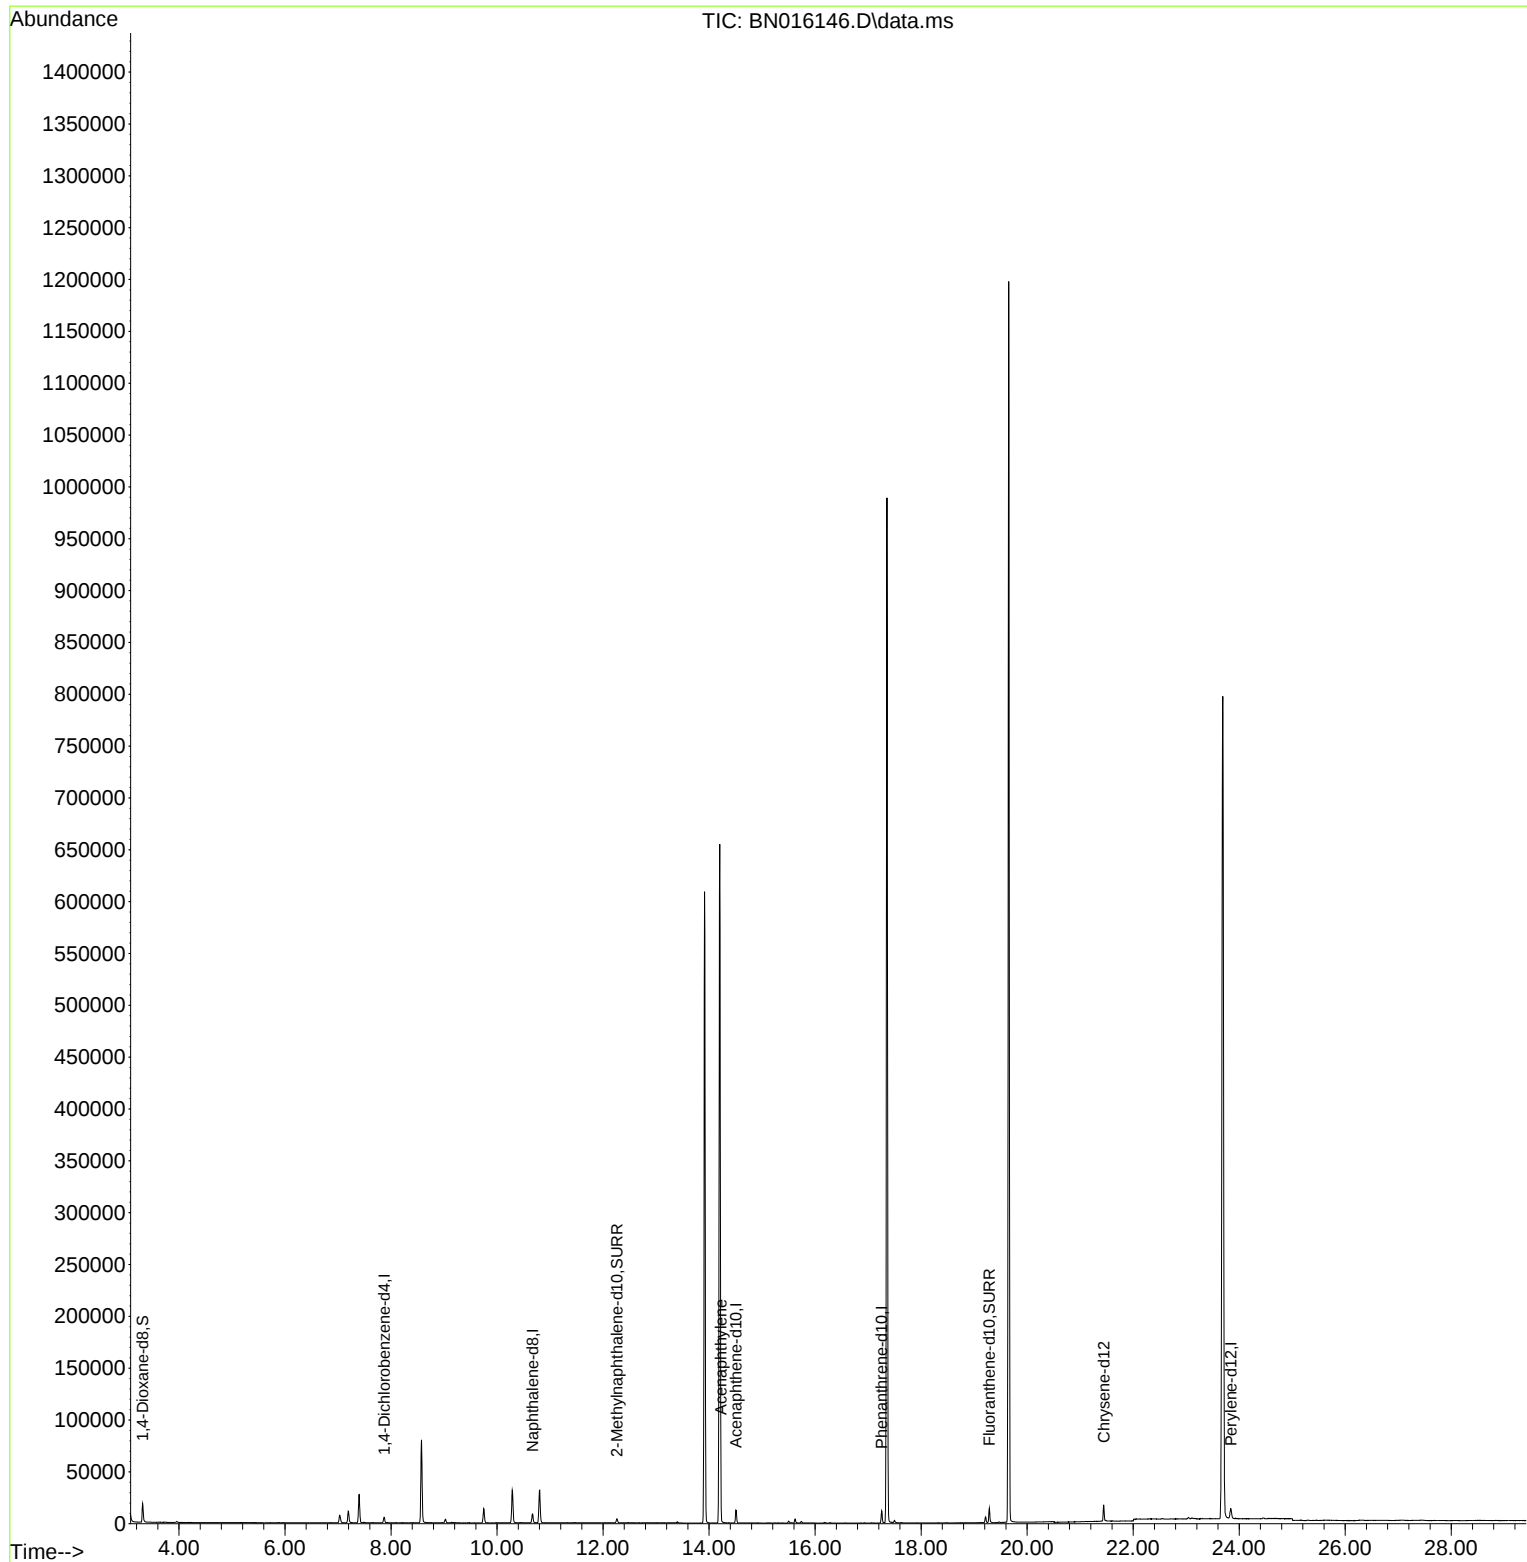

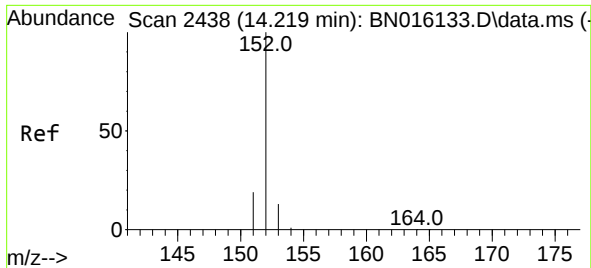

#10
Acenaphthylene
Concen: 0.036 ng/ul
RT: 14.224 min Scan# 2439
Delta R.T. 0.005 min
Lab File: BN016146.D
Acq: 02 Sep 2021 20:33

Instrument :
BNA_N
ClientSampleId :
C0B85

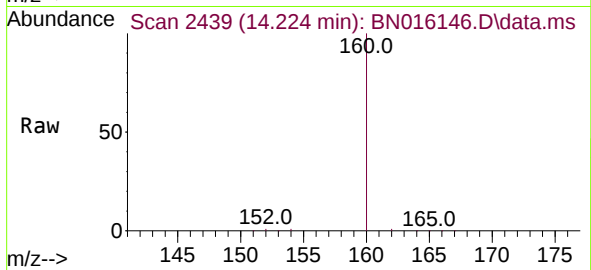

Tgt Ion	Ratio	Lower	Upper
152	100		
151	32.7	15.8	23.6#
153	29.9	11.2	16.8#

