
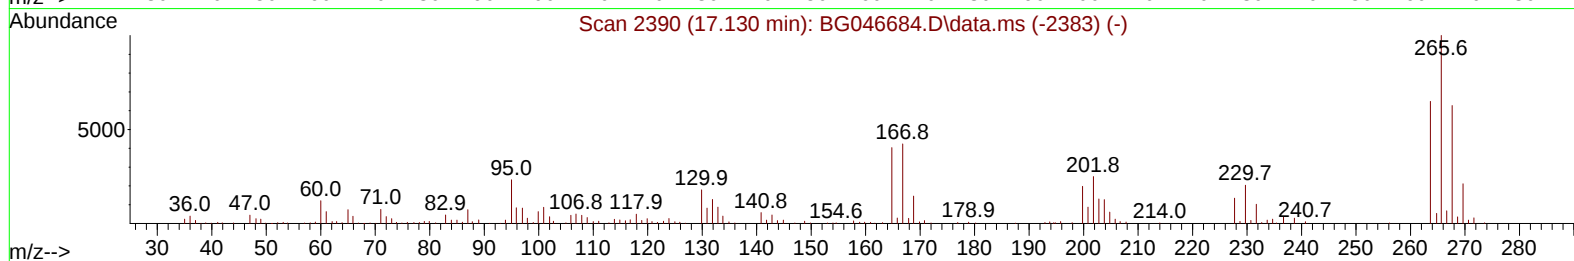
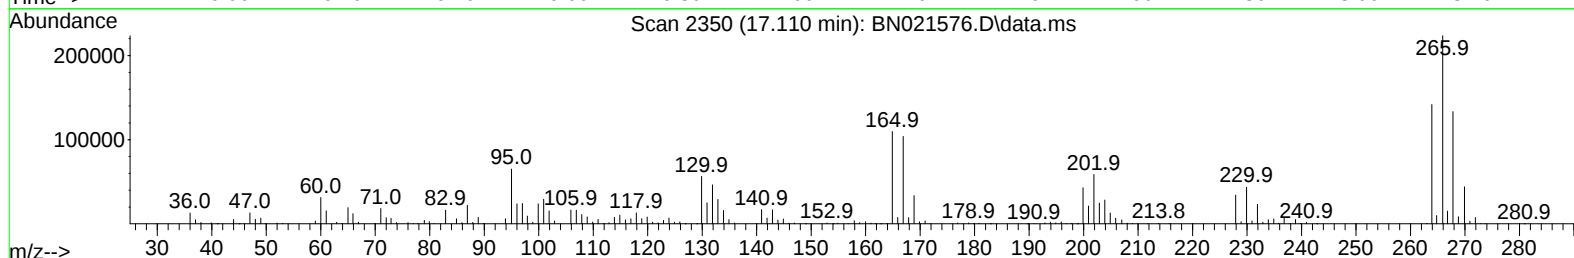


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090222\
Data File : BN021576.D
Acq On : 03 Sep 2022 01:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 05:13:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 05:12:16 2022
Response via : Initial Calibration

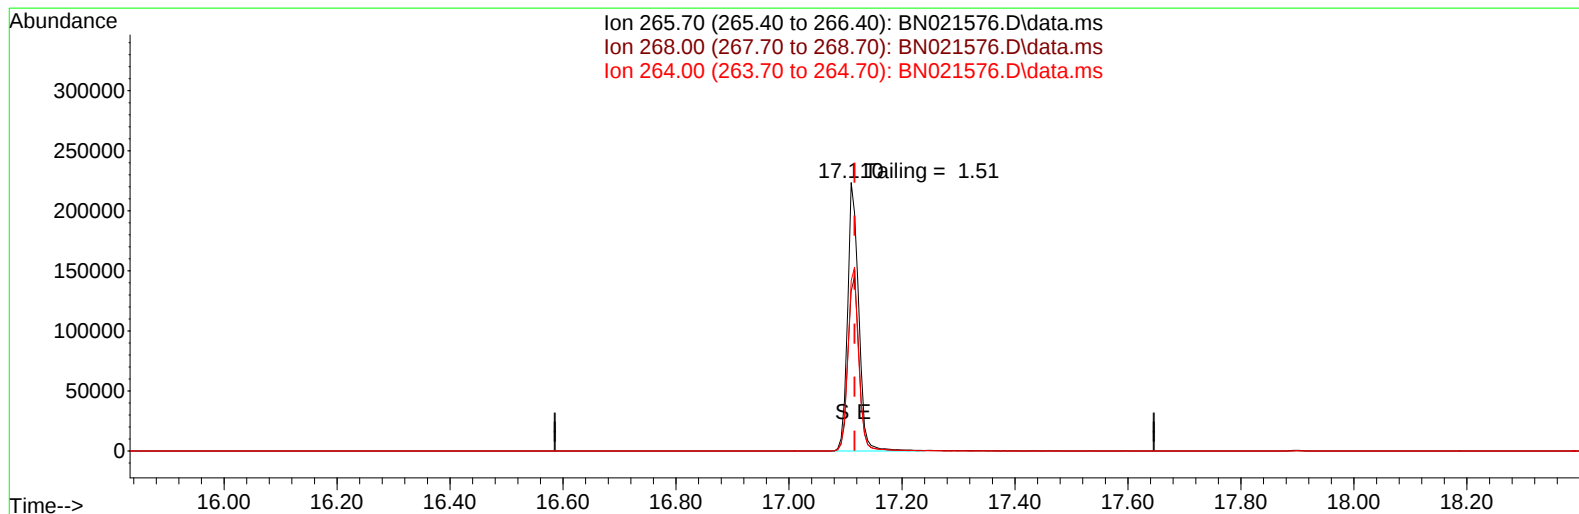

TIC: BN021576.D\data.ms

(70) Pentachlorophenol (C)




17.110min (-0.006) 19365.51 ng

response 305775

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.65
264.00	61.60	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090222\
Data File : BN021576.D
Acq On : 03 Sep 2022 01:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 05:13:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 05:12:16 2022
Response via : Initial Calibration

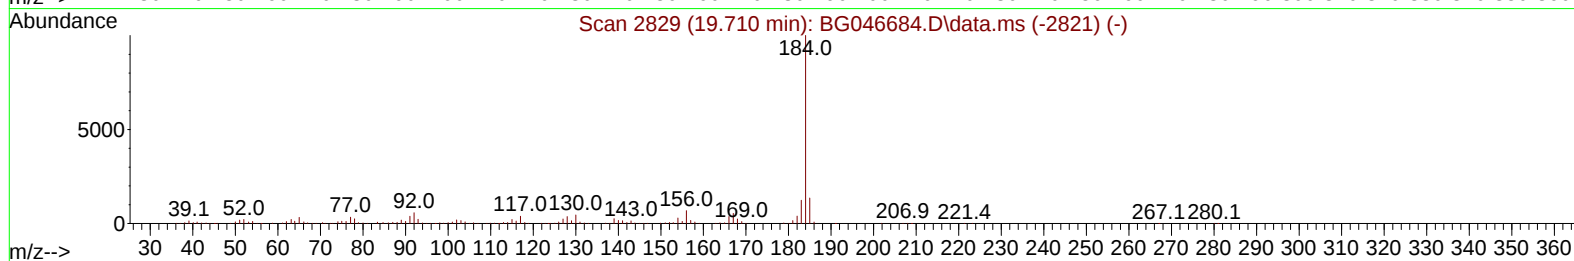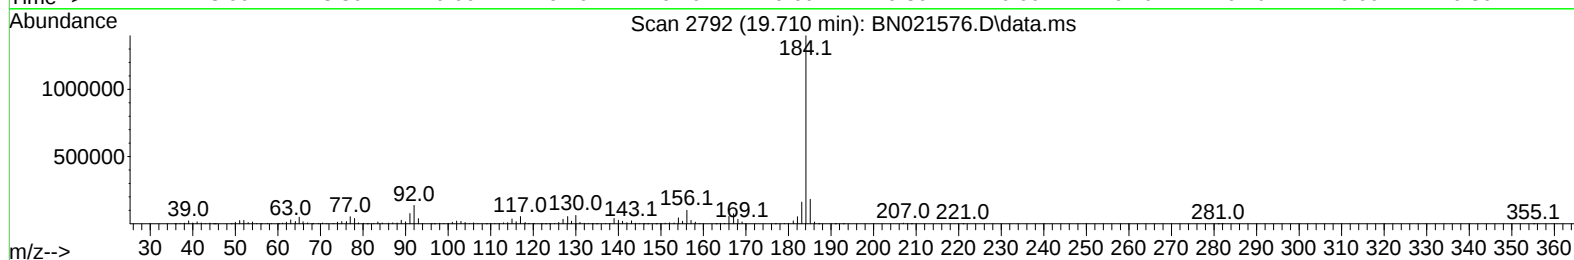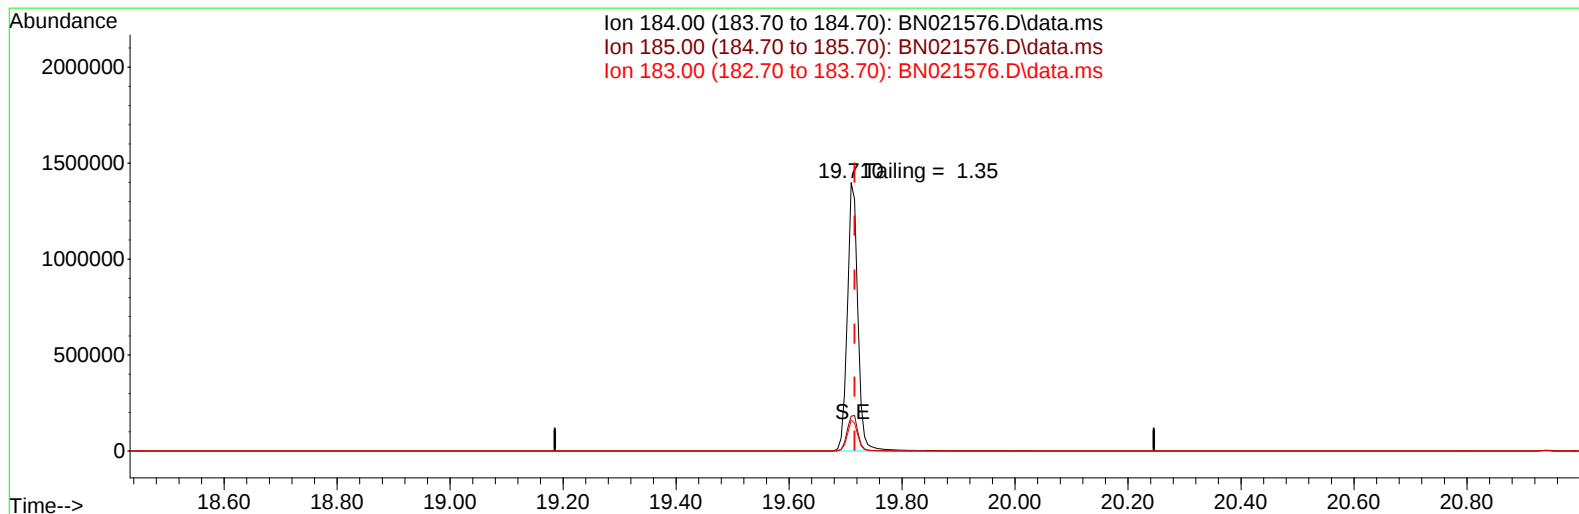

TIC: BN021576.D\data.ms

(77) Benzdine

19.710min (-0.006) 0.00 ng

response 1808790

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	11.54
0.00	0.00	0.00