


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090222\
 Data File : BN021558.D
 Acq On : 02 Sep 2022 12:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 00:53:31 2022

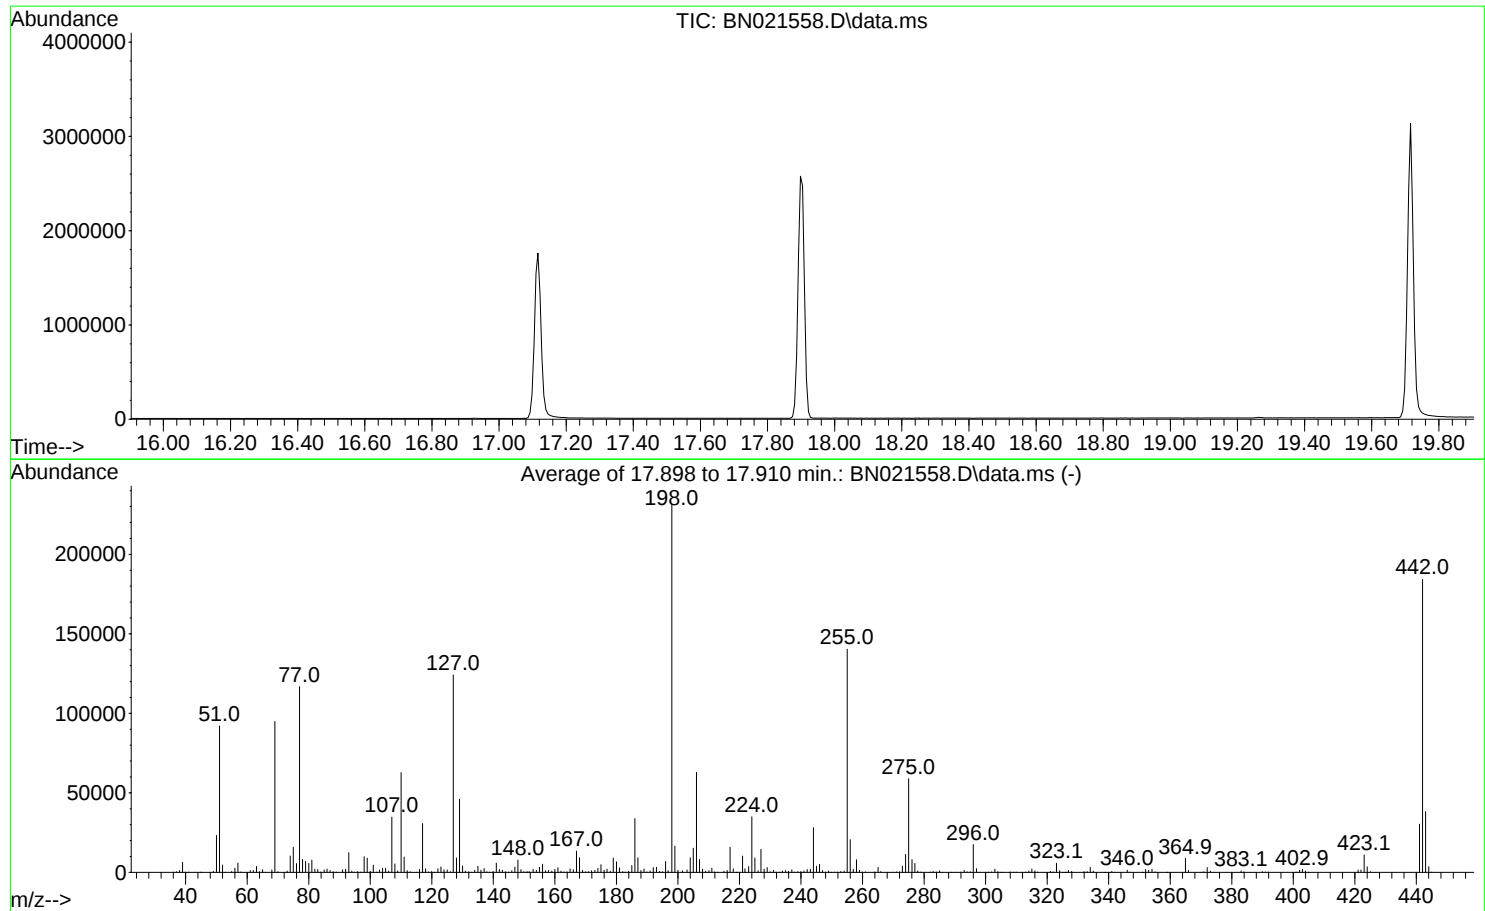

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	92085	PASS
68	69	0.00	2	1.6	1514	PASS
69	198	0.00	100	41.0	94880	PASS
70	69	0.00	2	0.5	441	PASS
127	198	10	80	53.7	124211	PASS
197	198	0.00	2	0.5	1156	PASS
198	198	100	100	100.0	231360	PASS
199	198	5	9	7.1	16535	PASS
275	198	10	60	25.4	58869	PASS
365	198	1	100	3.8	8729	PASS
441	198	0.01	100	13.1	30309	PASS
442	442	50	100	100.0	184277	PASS
443	442	15	24	20.7	38229	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/2/2022	BNA_N	<u>BN021558.D</u>
Compound Name	Response	Retention Time
DDT	846918	20.945
DDD	10124	20.504
DDE	776	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10900	857818	1.27

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090222\
 Data File : BN021558.D
 Acq On : 02 Sep 2022 12:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 03 05:12:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 03 05:12:16 2022
 Response via : Initial Calibration

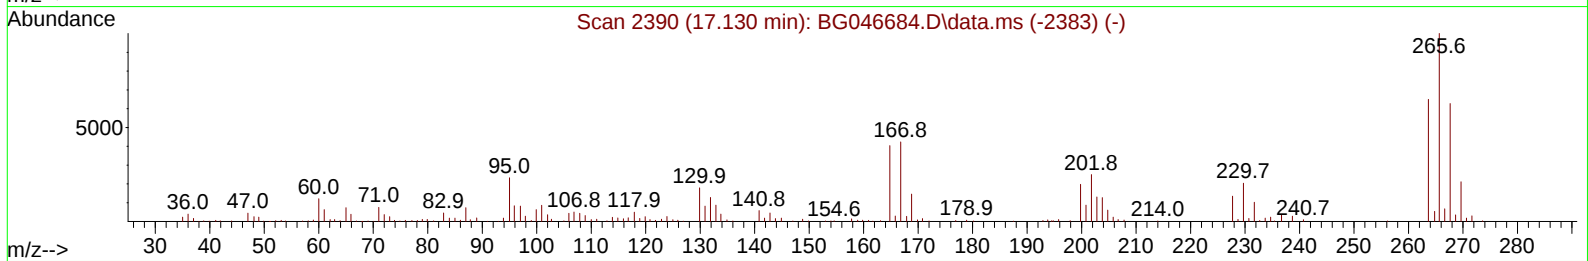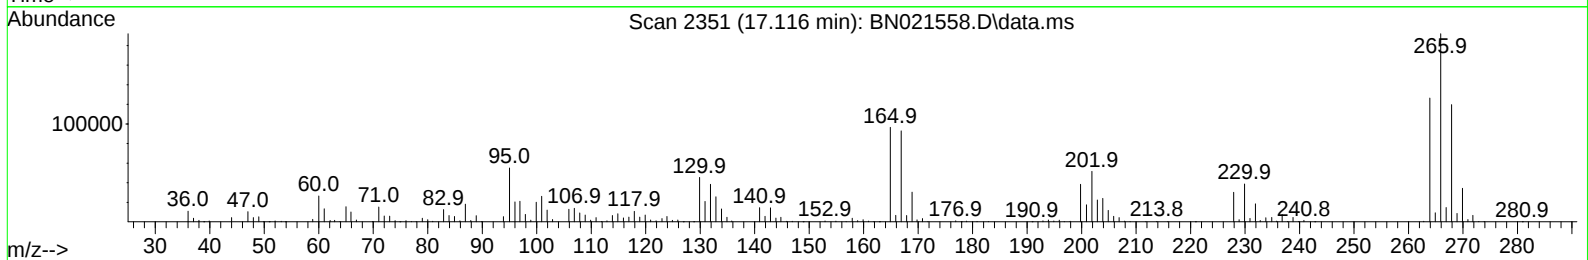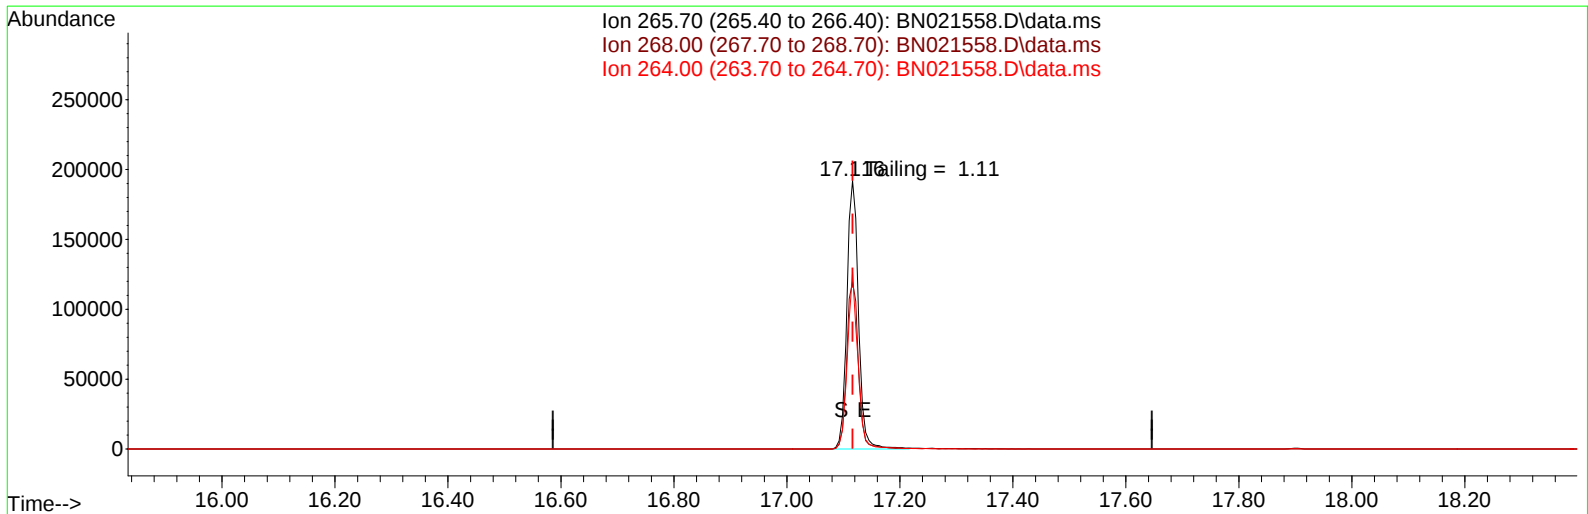

TIC: BN021558.D\data.ms

(70) Pentachlorophenol (C)

17.116min (0.000) 17743.15 ng




response 274728

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.32
264.00	61.60	65.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090222\
 Data File : BN021558.D
 Acq On : 02 Sep 2022 12:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 03 05:12:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 03 05:12:16 2022
 Response via : Initial Calibration

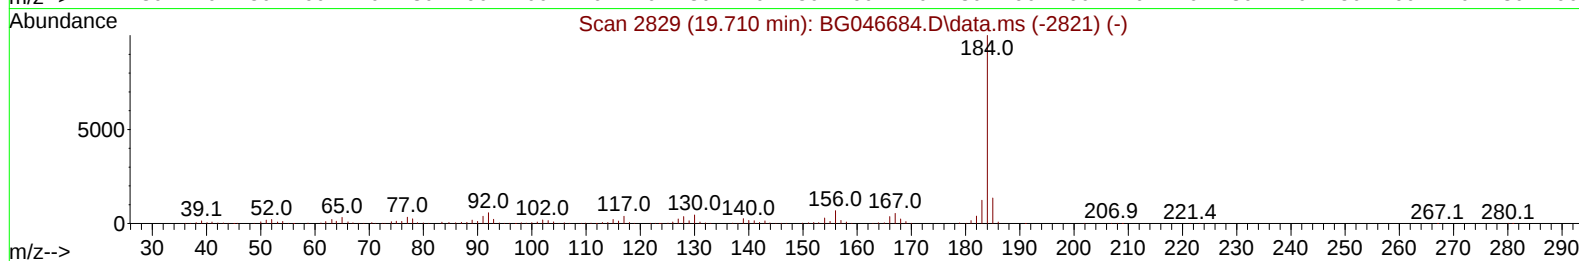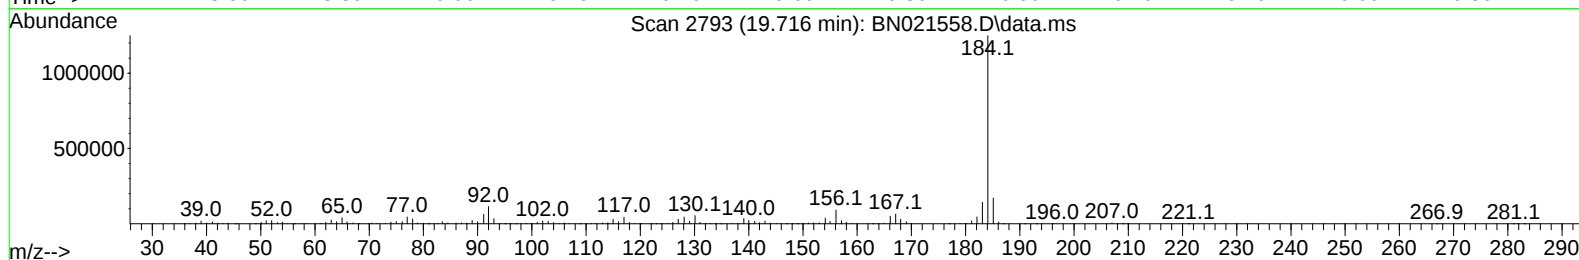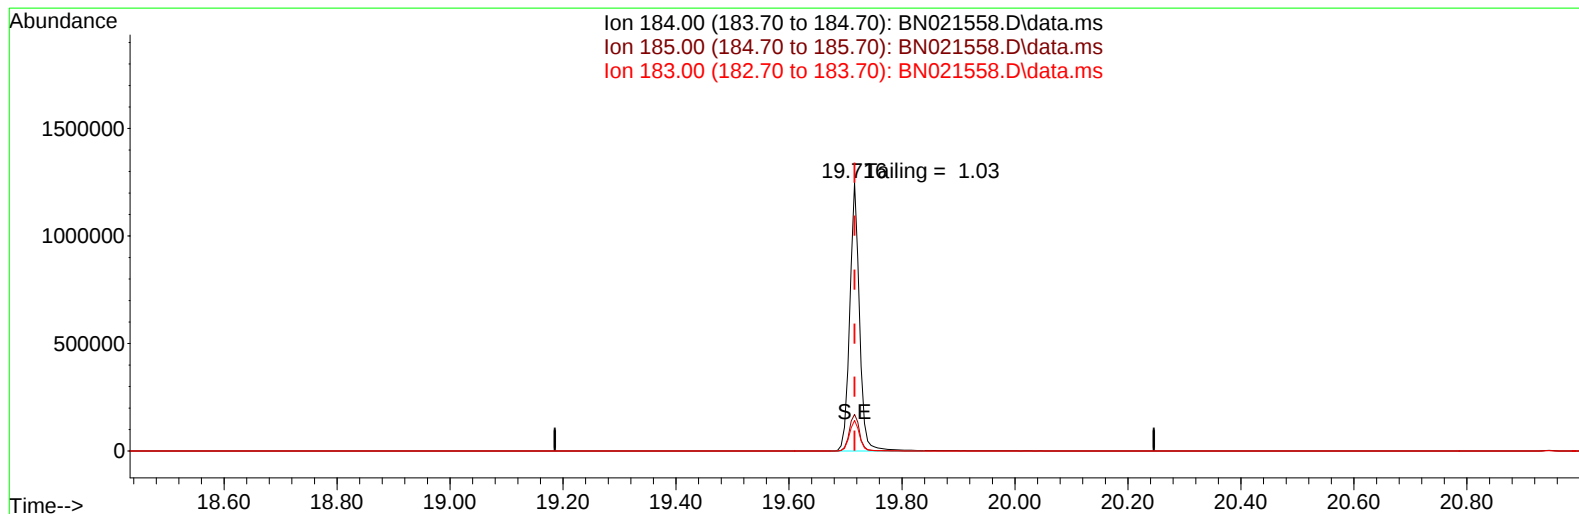

TIC: BN021558.D\data.ms

(77) Benzidine

19.716min (0.000) 0.00 ng

response 1501296

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.69
183.00	13.20	11.39
0.00	0.00	0.00