
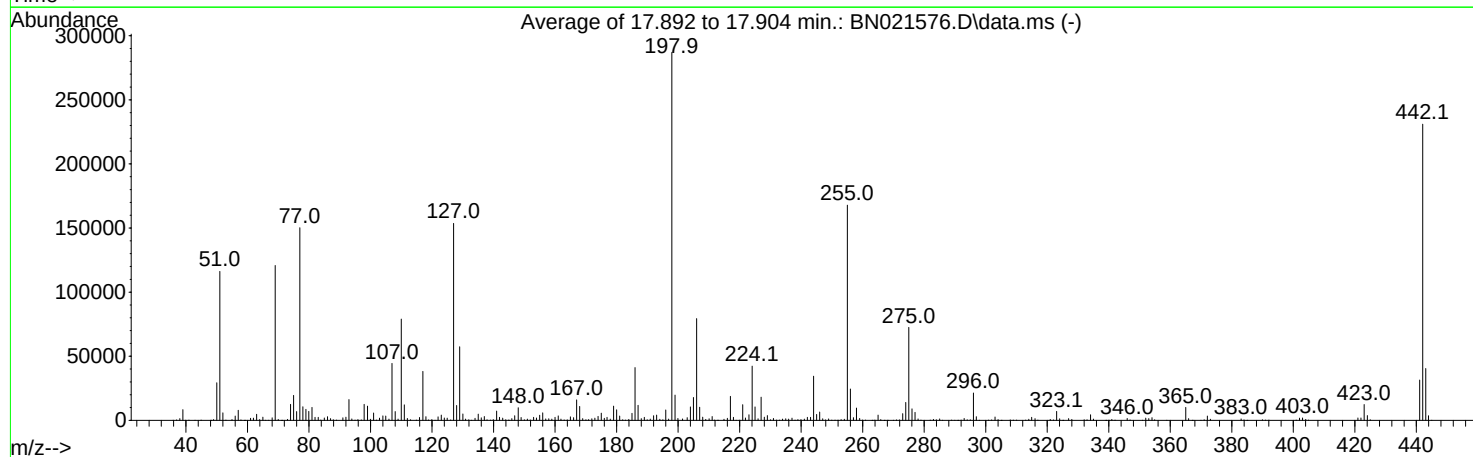


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090222\
 Data File : BN021576.D
 Acq On : 03 Sep 2022 01:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 00:53:31 2022

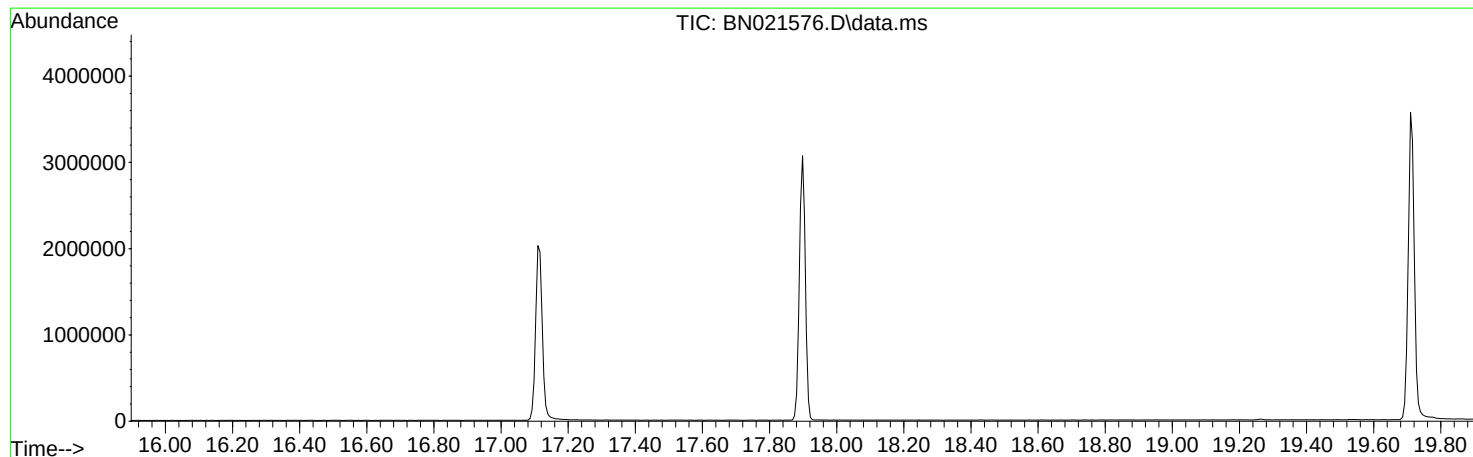

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	116197	PASS
68	69	0.00	2	1.6	1956	PASS
69	198	0.00	100	42.1	120859	PASS
70	69	0.00	2	0.6	707	PASS
127	198	10	80	53.6	153667	PASS
197	198	0.00	2	0.3	982	PASS
198	198	100	100	100.0	286912	PASS
199	198	5	9	6.9	19717	PASS
275	198	10	60	25.3	72461	PASS
365	198	1	100	3.5	10092	PASS
441	198	0.01	100	11.0	31488	PASS
442	442	50	100	100.0	231019	PASS
443	442	15	24	17.5	40419	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/2/2022	BNA_N	<u>BN021576.D</u>
Compound Name	Response	Retention Time
DDT	938156	20.939
DDD	13103	20.498
DDE	900	19.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14003	952159	1.47

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090222\
Data File : BN021576.D
Acq On : 03 Sep 2022 01:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 03 05:13:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 05:12:16 2022
Response via : Initial Calibration

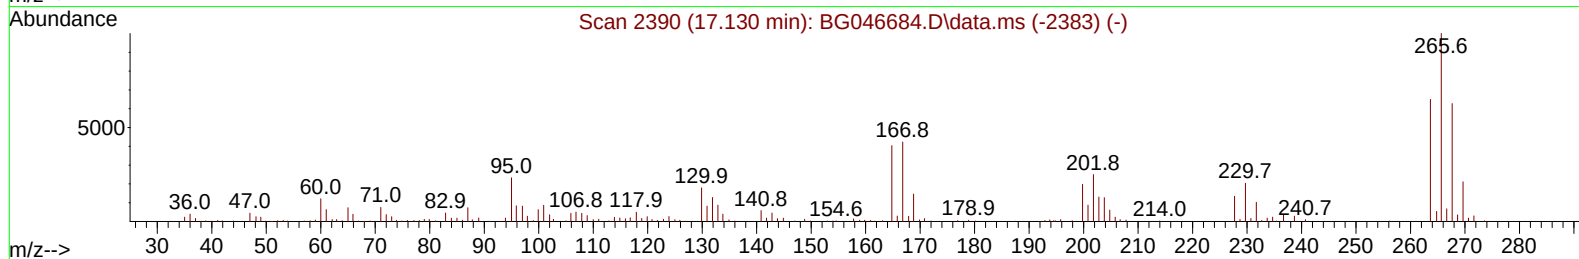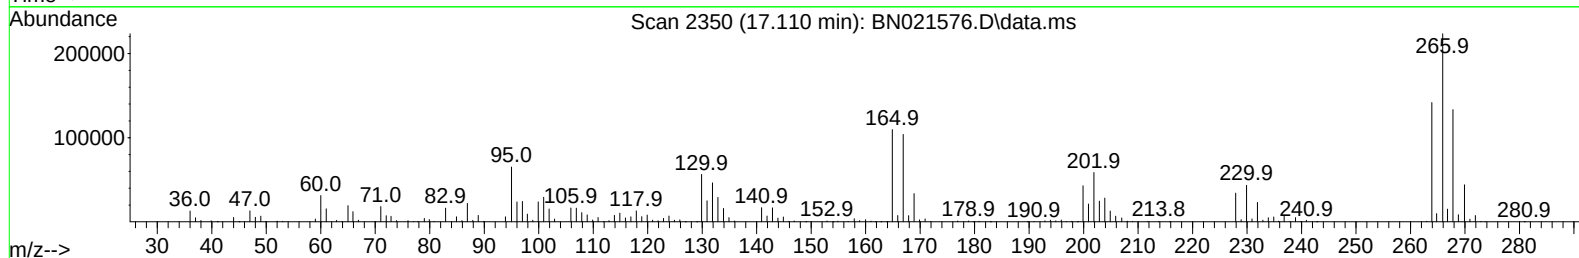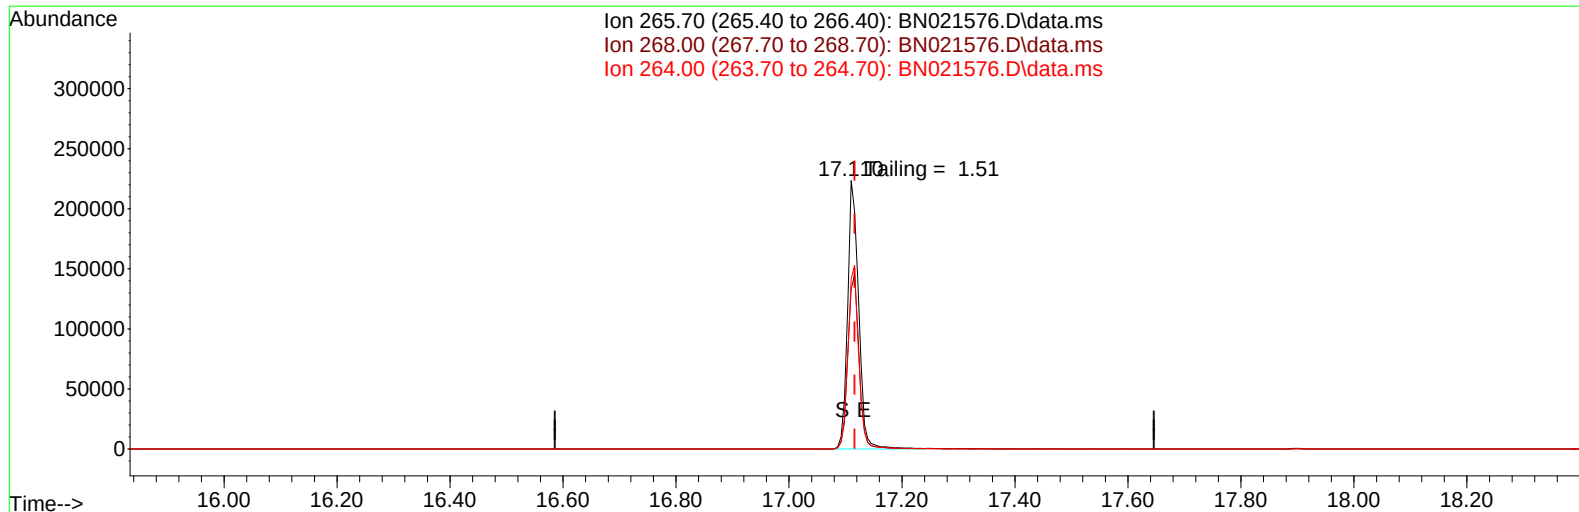

TIC: BN021576.D\data.ms

(70) Pentachlorophenol (C)

17.110min (-0.006) 19365.51 ng




response 305775

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.65
264.00	61.60	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090222\
Data File : BN021576.D
Acq On : 03 Sep 2022 01:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 03 05:13:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 05:12:16 2022
Response via : Initial Calibration

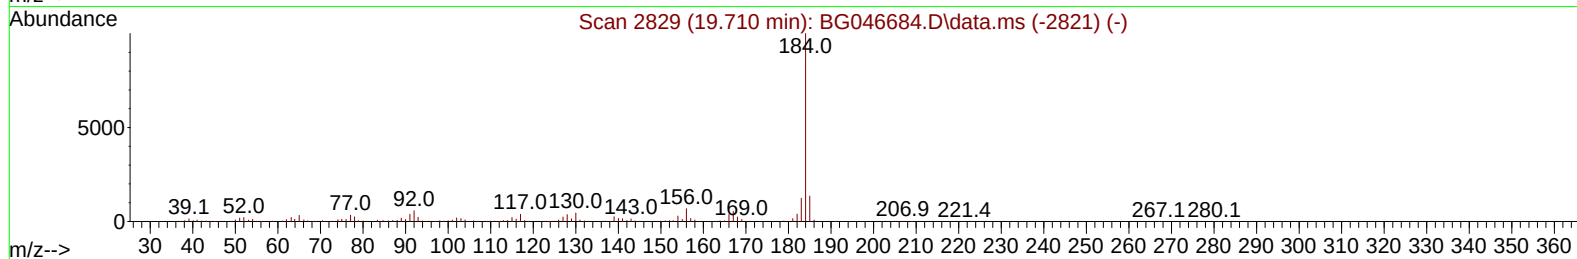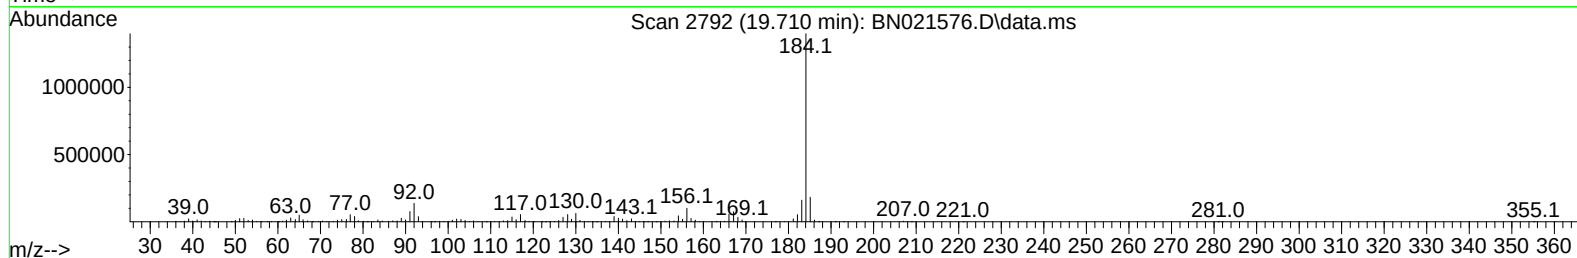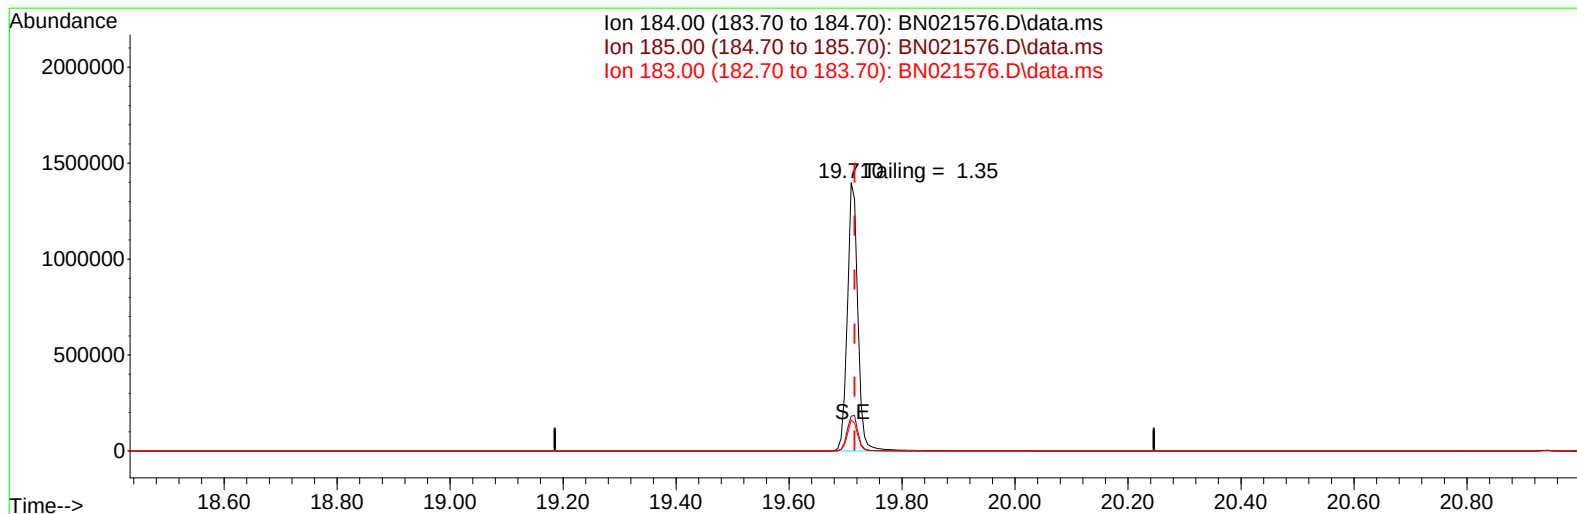

TIC: BN021576.D\data.ms

(77) Benzidine

19.710min (-0.006) 0.00 ng

response 1808790

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	11.54
0.00	0.00	0.00