


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090319\
 Data File : BN007530.D
 Acq On : 03 Sep 2019 09:53
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 29 12:18:45 2019

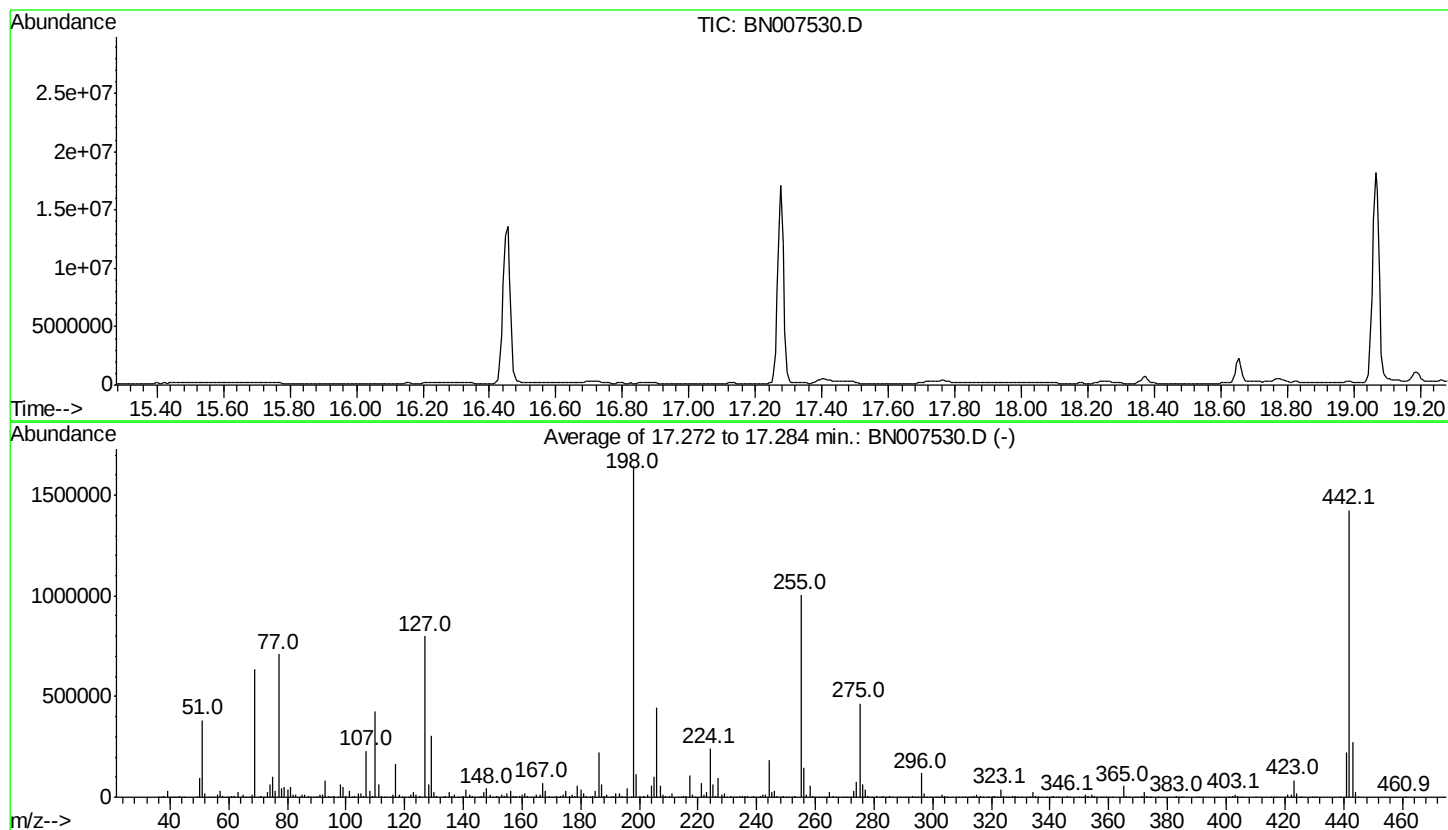

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.2	382618	PASS
68	69	0.00	2	1.8	11694	PASS
69	198	0.00	100	38.6	634967	PASS
70	69	0.00	2	0.5	3241	PASS
127	198	10	80	48.6	799677	PASS
197	198	0.00	2	0.2	3119	PASS
198	198	100	100	100.0	1646782	PASS
199	198	5	9	6.8	111597	PASS
275	198	10	60	28.3	465493	PASS
365	198	1	100	3.4	56232	PASS
441	198	0.01	100	13.4	220352	PASS
442	198	50	100	86.6	1426773	PASS
443	442	15	24	19.3	276053	PASS