
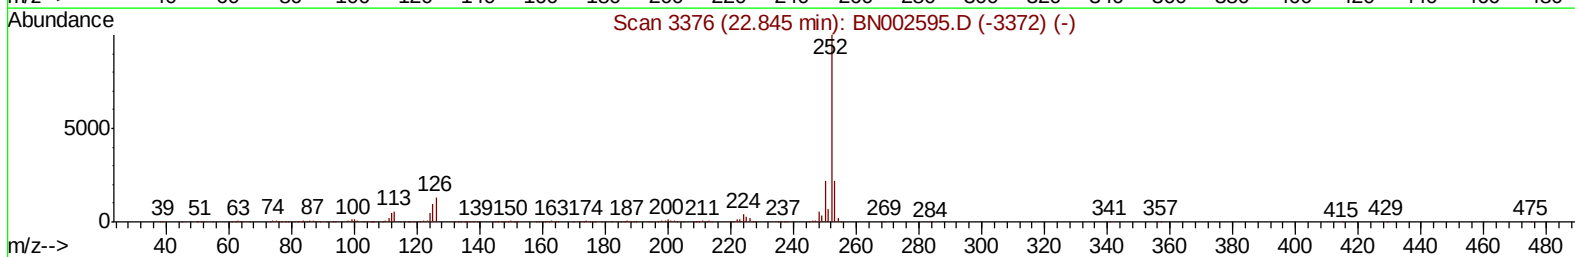
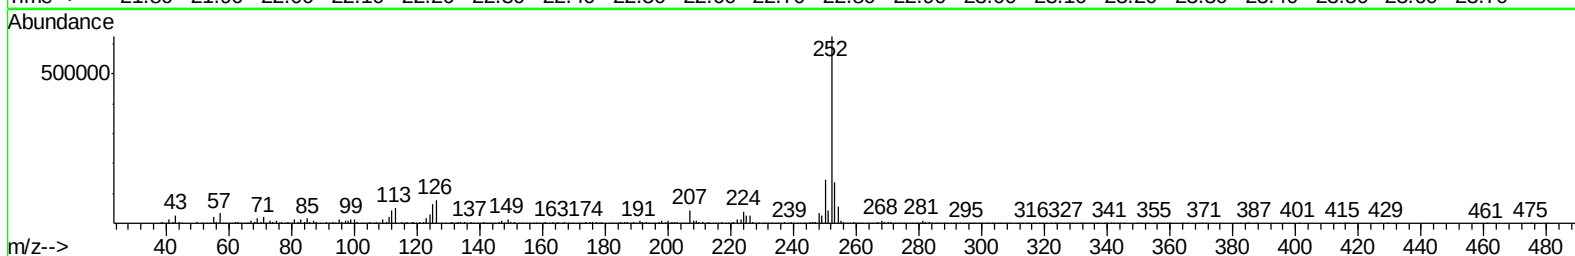


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090518\
Data File : BN002603.D
Acq On : 06 Sep 2018 04:48
Operator : JU/SJ
Sample : J4688-20MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Sep 06 06:58:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 06 06:54:57 2018
Response via : Initial Calibration

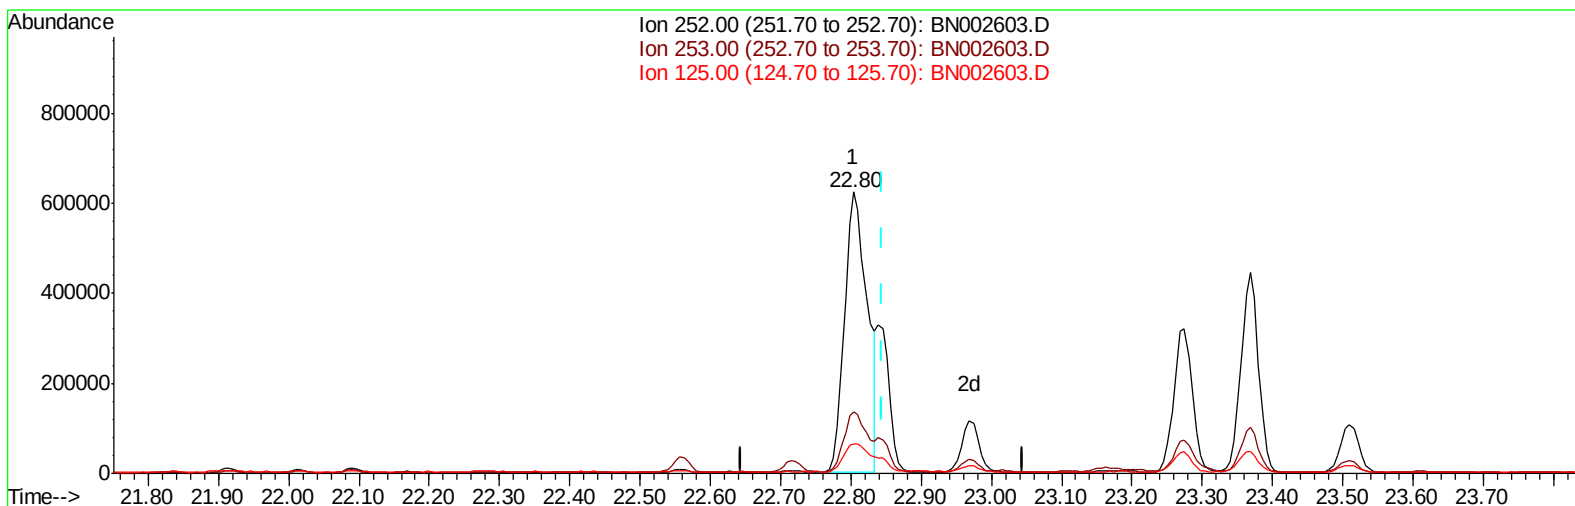

TIC: BN002603.D

(88) Benzo(k)fluoranthene

22.804min (-0.041) 29.39ng/ul

response 1419955

Ion	Exp%	Act%
252.00	100	100
253.00	21.60	22.06
125.00	10.20	10.58
0.00	0.00	0.00