

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN090518\
 Data File : BN002588.D
 Acq On : 05 Sep 2018 20:00
 Operator : JU/SJ
 Sample : J4688-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 06 05:15:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 06 05:13:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	133091	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	619908	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	399157	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	973266	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	1050186	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	931189	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	7061	2.50	ng/uL	0.00
5) Phenol-d5	6.85	99	162838	13.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	109991	14.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	137317	14.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	134639	13.80	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	65201	13.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	77391	14.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	137006	14.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	186413	18.08	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	519858	15.71	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	616120	15.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	53489	8.55	ng/ul	0.00
57) Fluorene-d10	15.29	176	457334	15.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	62081	10.02	ng/ul	0.00
70) Anthracene-d10	17.15	188	732020	15.74	ng/ul	0.00
78) Pyrene-d10	19.45	212	850023	16.92	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	786372	16.15	ng/ul	-0.01

Target Compounds


					Ovalue
44) Dimethylphthalate	13.76	163	387726	11.948	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN090518\
Data File : BN002588.D
Acq On : 05 Sep 2018 20:00
Operator : JU/SJ
Sample : J4688-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 06 05:15:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 06 05:13:50 2018
Response via : Initial Calibration

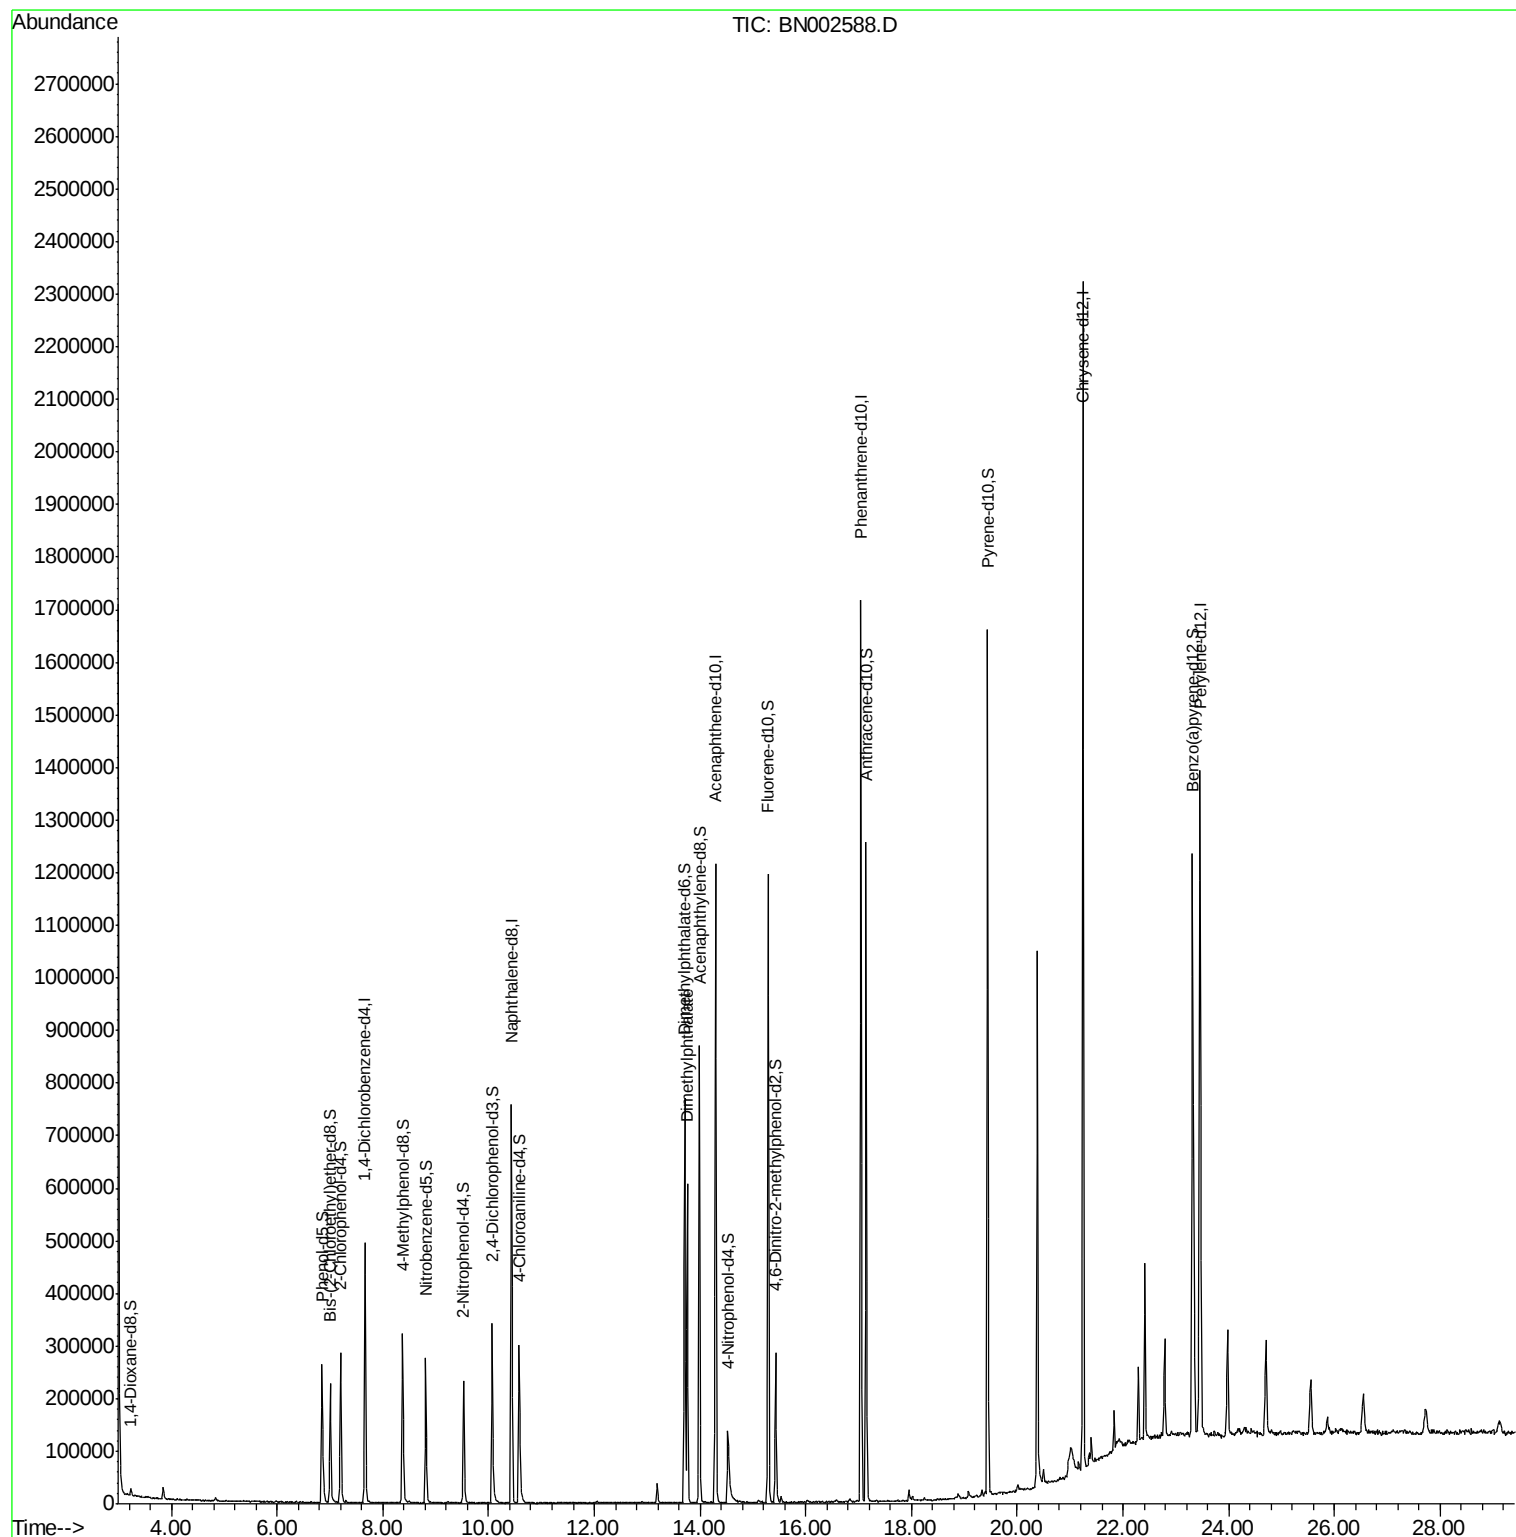

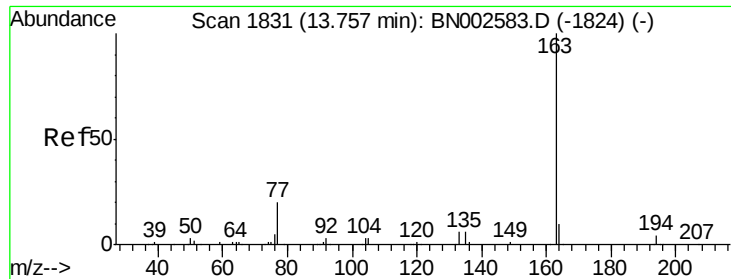

#44
 Dimethylphthalate
 Concen: 11.948 ng/ul
 RT: 13.76 min Scan# 1831
 Delta R.T. 0.00 min
 Lab File: BN002588.D
 Acq: 05 Sep 2018 20:00

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:	163	Resp:	387726
Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.2	4.8
164	9.9	7.8	11.8

