

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090518\
 Data File : BN002592.D
 Acq On : 05 Sep 2018 22:21
 Operator : JU/SJ
 Sample : PB112628BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 06 05:16:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 06 05:13:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	118355	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	562852	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	366583	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	883376	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1016995	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	936168	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	16891	6.74	ng/uL	0.00
5) Phenol-d5	6.85	99	377561	34.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	245503	36.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	307506	37.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	316117	36.44	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	160853	35.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	185694	39.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	312151	36.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	475136	50.77	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1171542	38.55	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1398503	37.51	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	172429	30.02	ng/ul	0.00
57) Fluorene-d10	15.29	176	1008562	38.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	172715	30.71	ng/ul	0.00
70) Anthracene-d10	17.15	188	1639262	38.84	ng/ul	0.00
78) Pyrene-d10	19.45	212	1873021	38.49	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	1928352	39.39	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.37	70	8266	1.129	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN090518\
Data File : BN002592.D
Acq On : 05 Sep 2018 22:21
Operator : JU/SJ
Sample : PB112628BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 06 05:16:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 06 05:13:50 2018
Response via : Initial Calibration

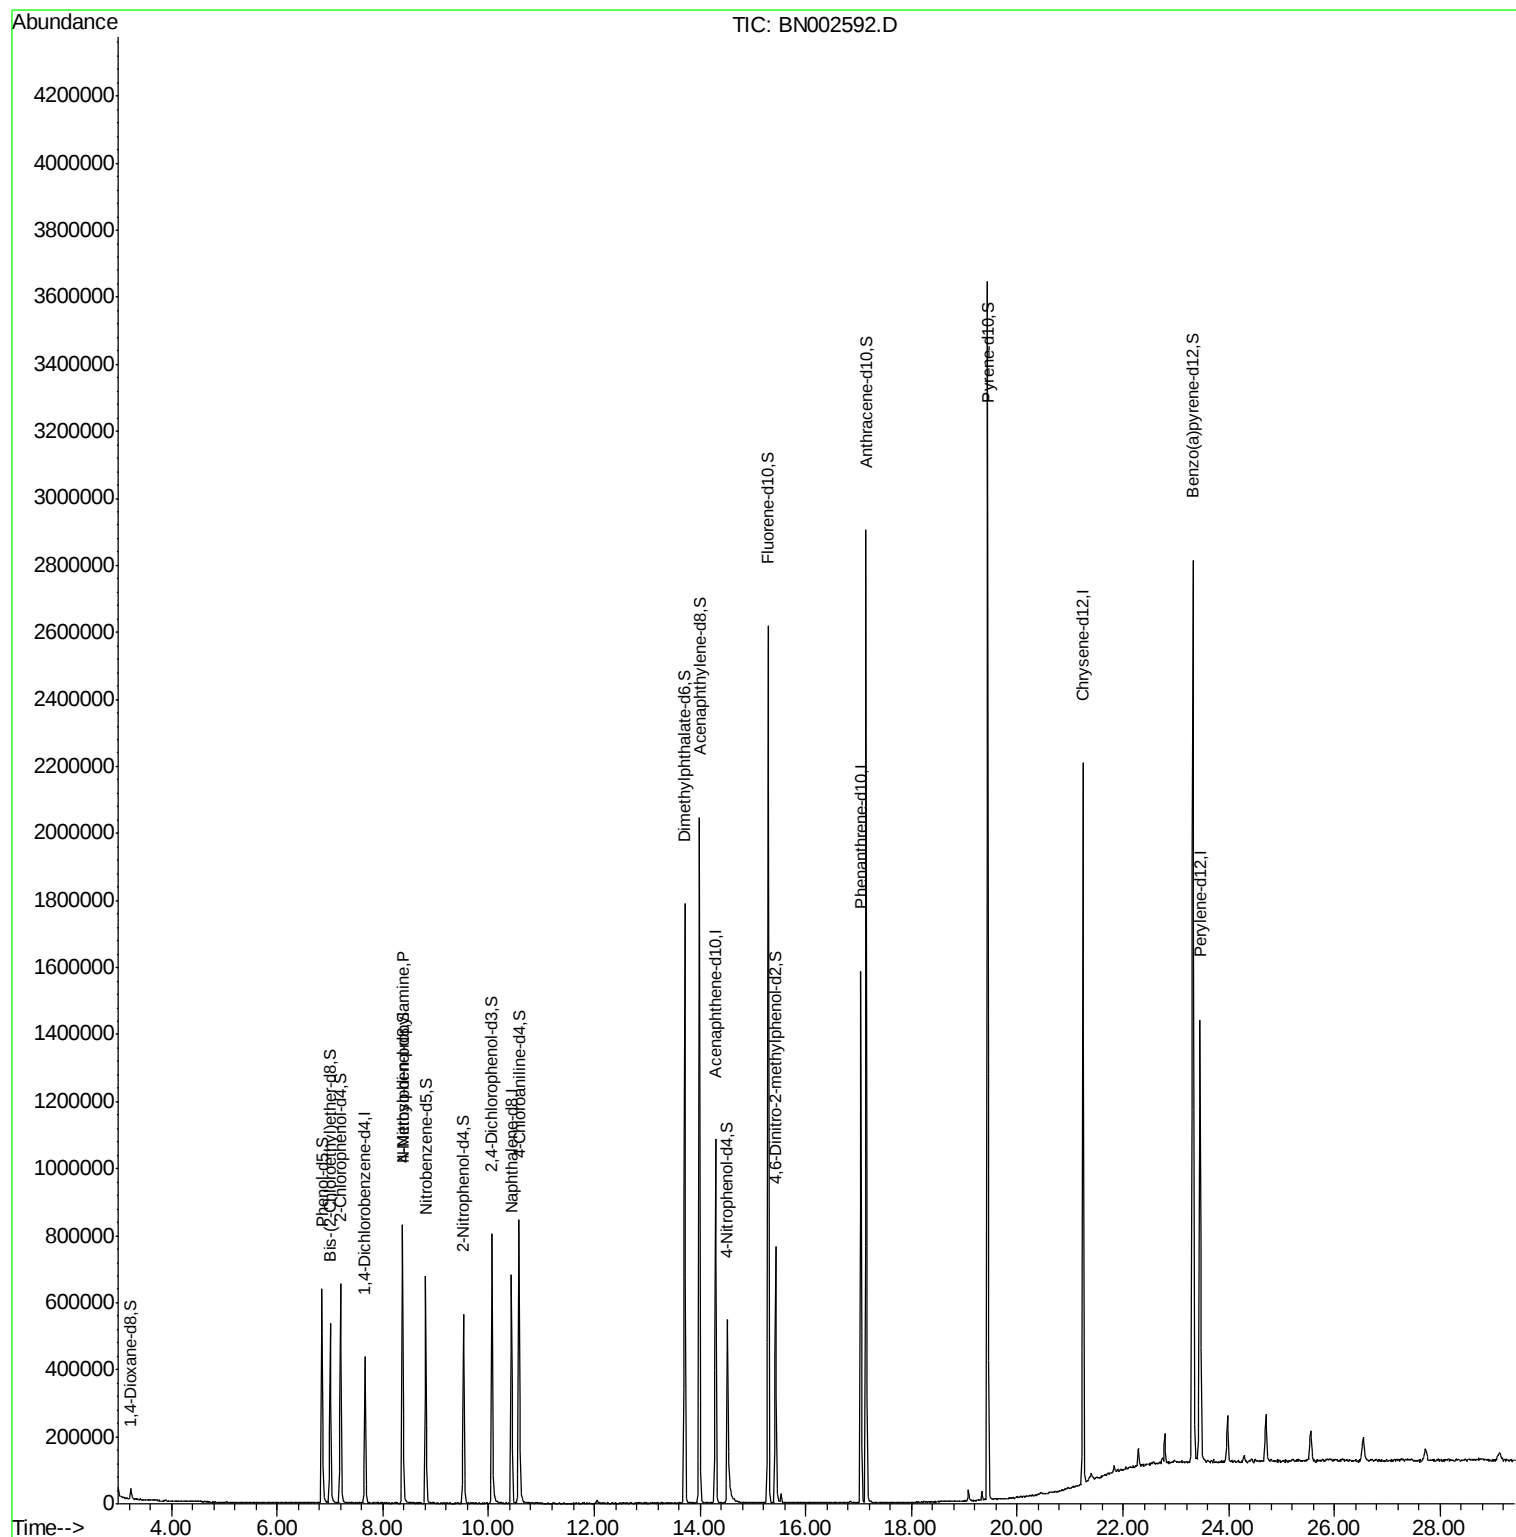

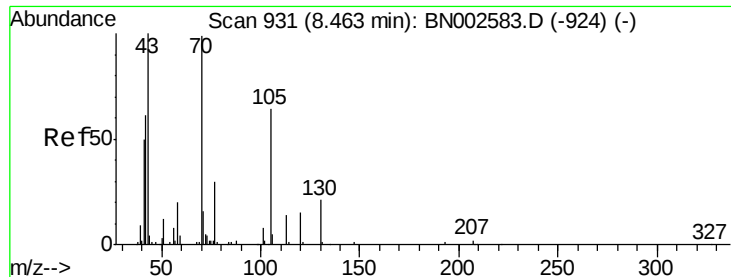

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.129 ng/ul
 RT: 8.37 min Scan# 915
 Delta R.T. -0.09 min
 Lab File: BN002592.D
 Acq: 05 Sep 2018 22:21

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 8266
 Ion Ratio Lower Upper
 70 100
 42 358.1 35.4 53.0#
 101 0.0 8.4 12.6#
 130 0.0 18.2 27.4#

