

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
 Data File : BN027378.D
 Acq On : 05 Sep 2023 16:45
 Operator : MA/JU
 Sample : PB155063BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK063

Quant Time: Sep 06 00:42:29 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	4359	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	15199	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	8550	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	19328	0.400	ng/ul	0.00
17) Chrysene-d12	21.618	240	14003	0.400	ng/ul	0.00
23) Perylene-d12	24.135	264	16534	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	44287	7.638	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	7063	0.306	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	16269	0.339	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.679	166	2755	0.073	ng/ul#	14
20) Pyrene	19.822	202	2838	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.971	252	6390	0.105	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027378.D
Acq On : 05 Sep 2023 16:45
Operator : MA/JU
Sample : PB155063BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK063

Quant Time: Sep 06 00:42:29 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




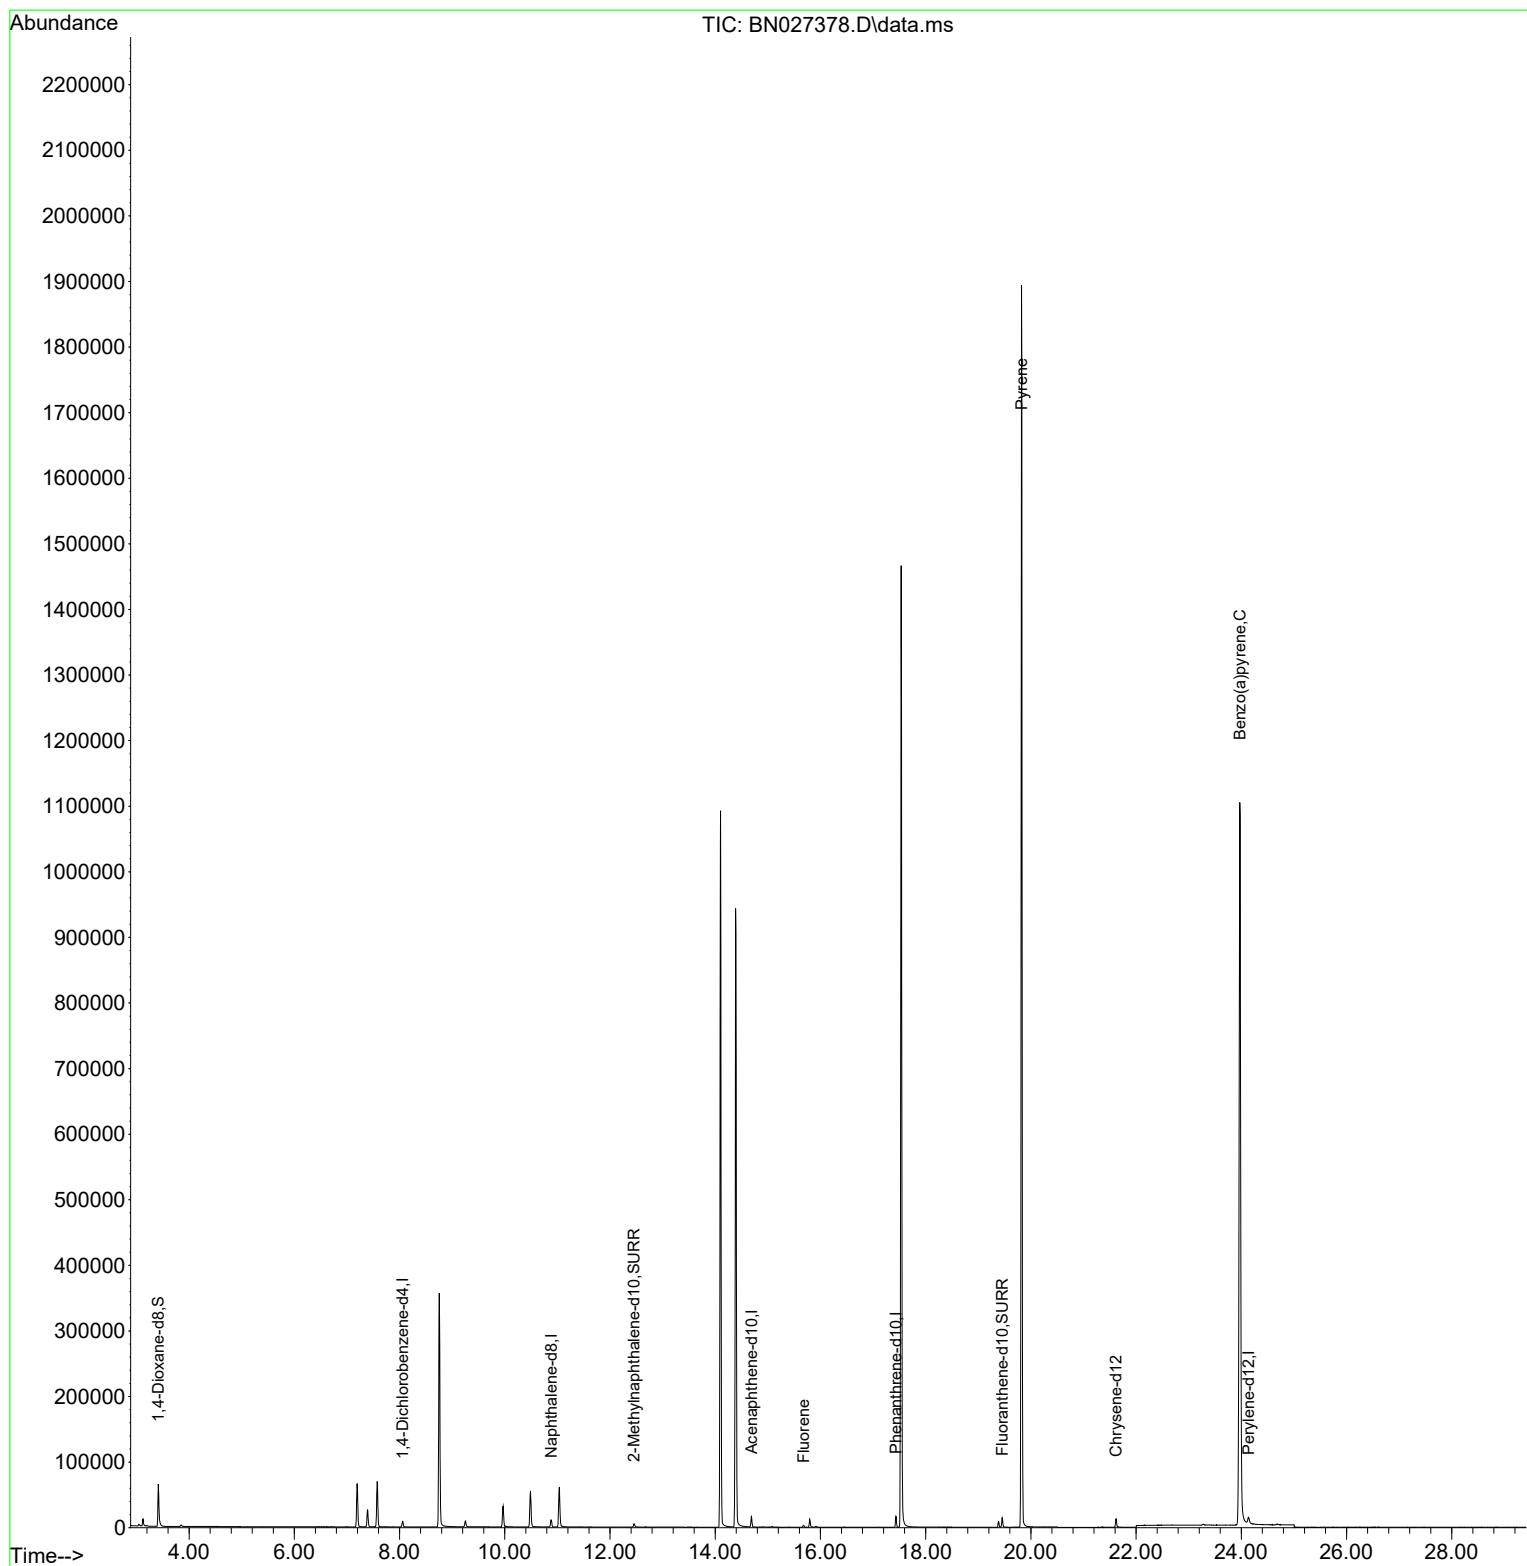


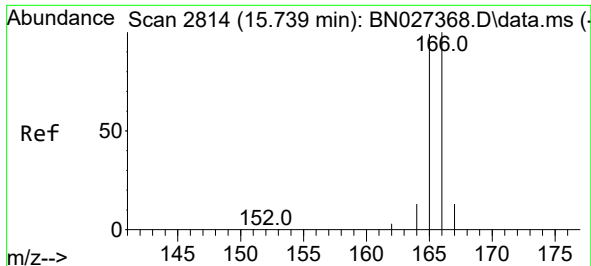

#12
Fluorene
Concen: 0.073 ng/ul
RT: 15.679 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN027378.D
Acq: 05 Sep 2023 16:45




Instrument :
BNA_N
ClientSampleId :
SBLK063


Tgt Ion:166 Resp: 2755
Ion Ratio Lower Upper
166 100
165 9.2 79.6 119.4#
167 36.2 11.4 17.0#

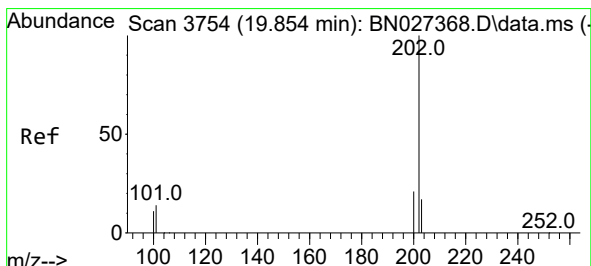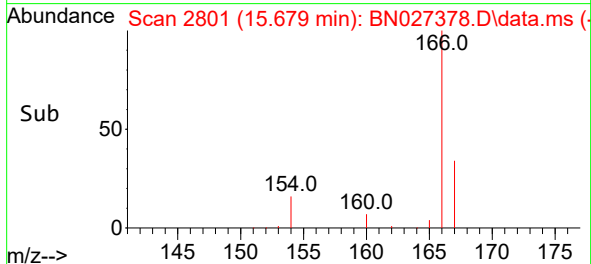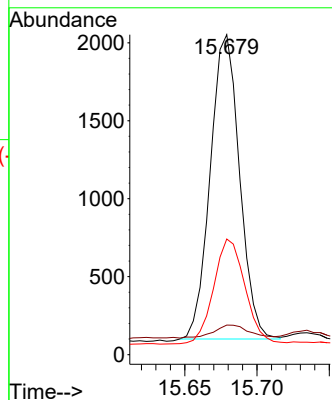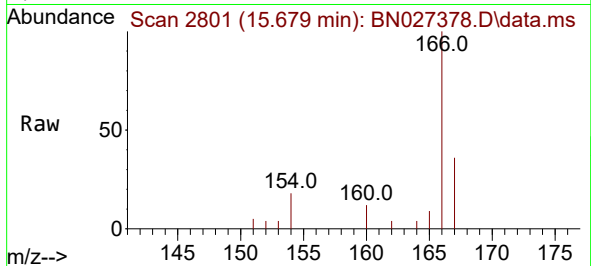

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.822 min Scan# 3747
Delta R.T. -0.028 min
Lab File: BN027378.D
Acq: 05 Sep 2023 16:45


Tgt Ion:202 Resp: 2838
Ion Ratio Lower Upper
202 100
101 174.7 11.4 17.2#
100 1326.9 9.4 14.2#

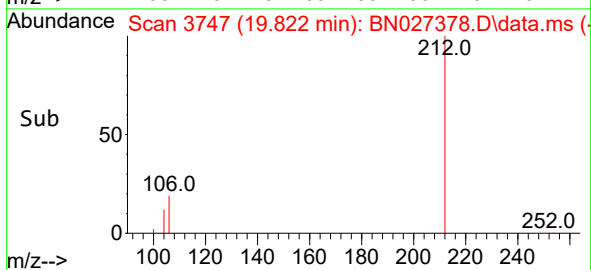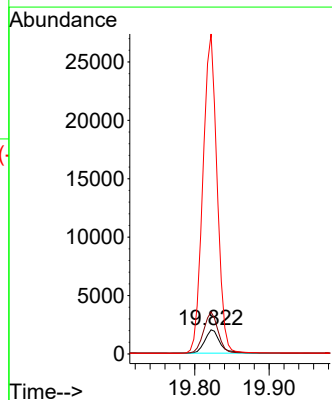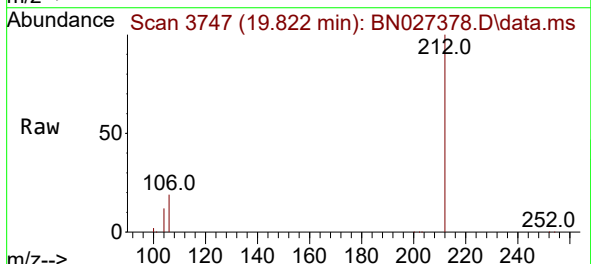

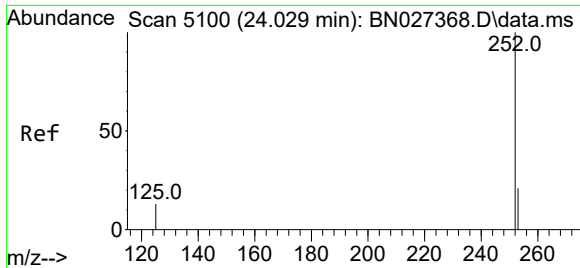

#26
Benzo(a)pyrene
Concen: 0.105 ng/ul
RT: 23.971 min Scan# 50
Delta R.T. -0.047 min
Lab File: BN027378.D
Acq: 05 Sep 2023 16:45

Instrument :
BNA_N
ClientSampleId :
SBLK063

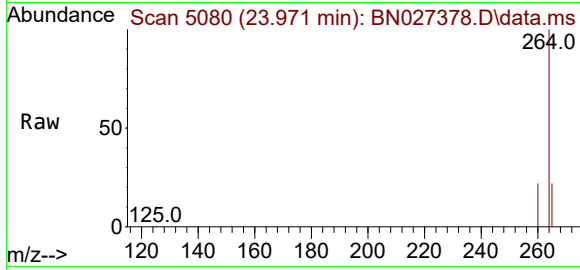

Tgt Ion:252 Resp: 6390
Ion Ratio Lower Upper
252 100
253 43.2 22.4 33.6#
125 41.4 17.4 26.2#

