

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
 Data File : BN027379.D
 Acq On : 05 Sep 2023 17:22
 Operator : MA/JU
 Sample : PB155073BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK073

Quant Time: Sep 06 00:42:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	3793	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	13189	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	7439	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	16906	0.400	ng/ul	0.00
17) Chrysene-d12	21.621	240	12445	0.400	ng/ul	0.01
23) Perylene-d12	24.141	264	14613	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	41733	8.271	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	6636	0.332	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	15563	0.365	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.679	166	2609	0.079	ng/ul#	14
20) Pyrene	19.822	202	2792	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.977	252	6247	0.116	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027379.D
Acq On : 05 Sep 2023 17:22
Operator : MA/JU
Sample : PB155073BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK073

Quant Time: Sep 06 00:42:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




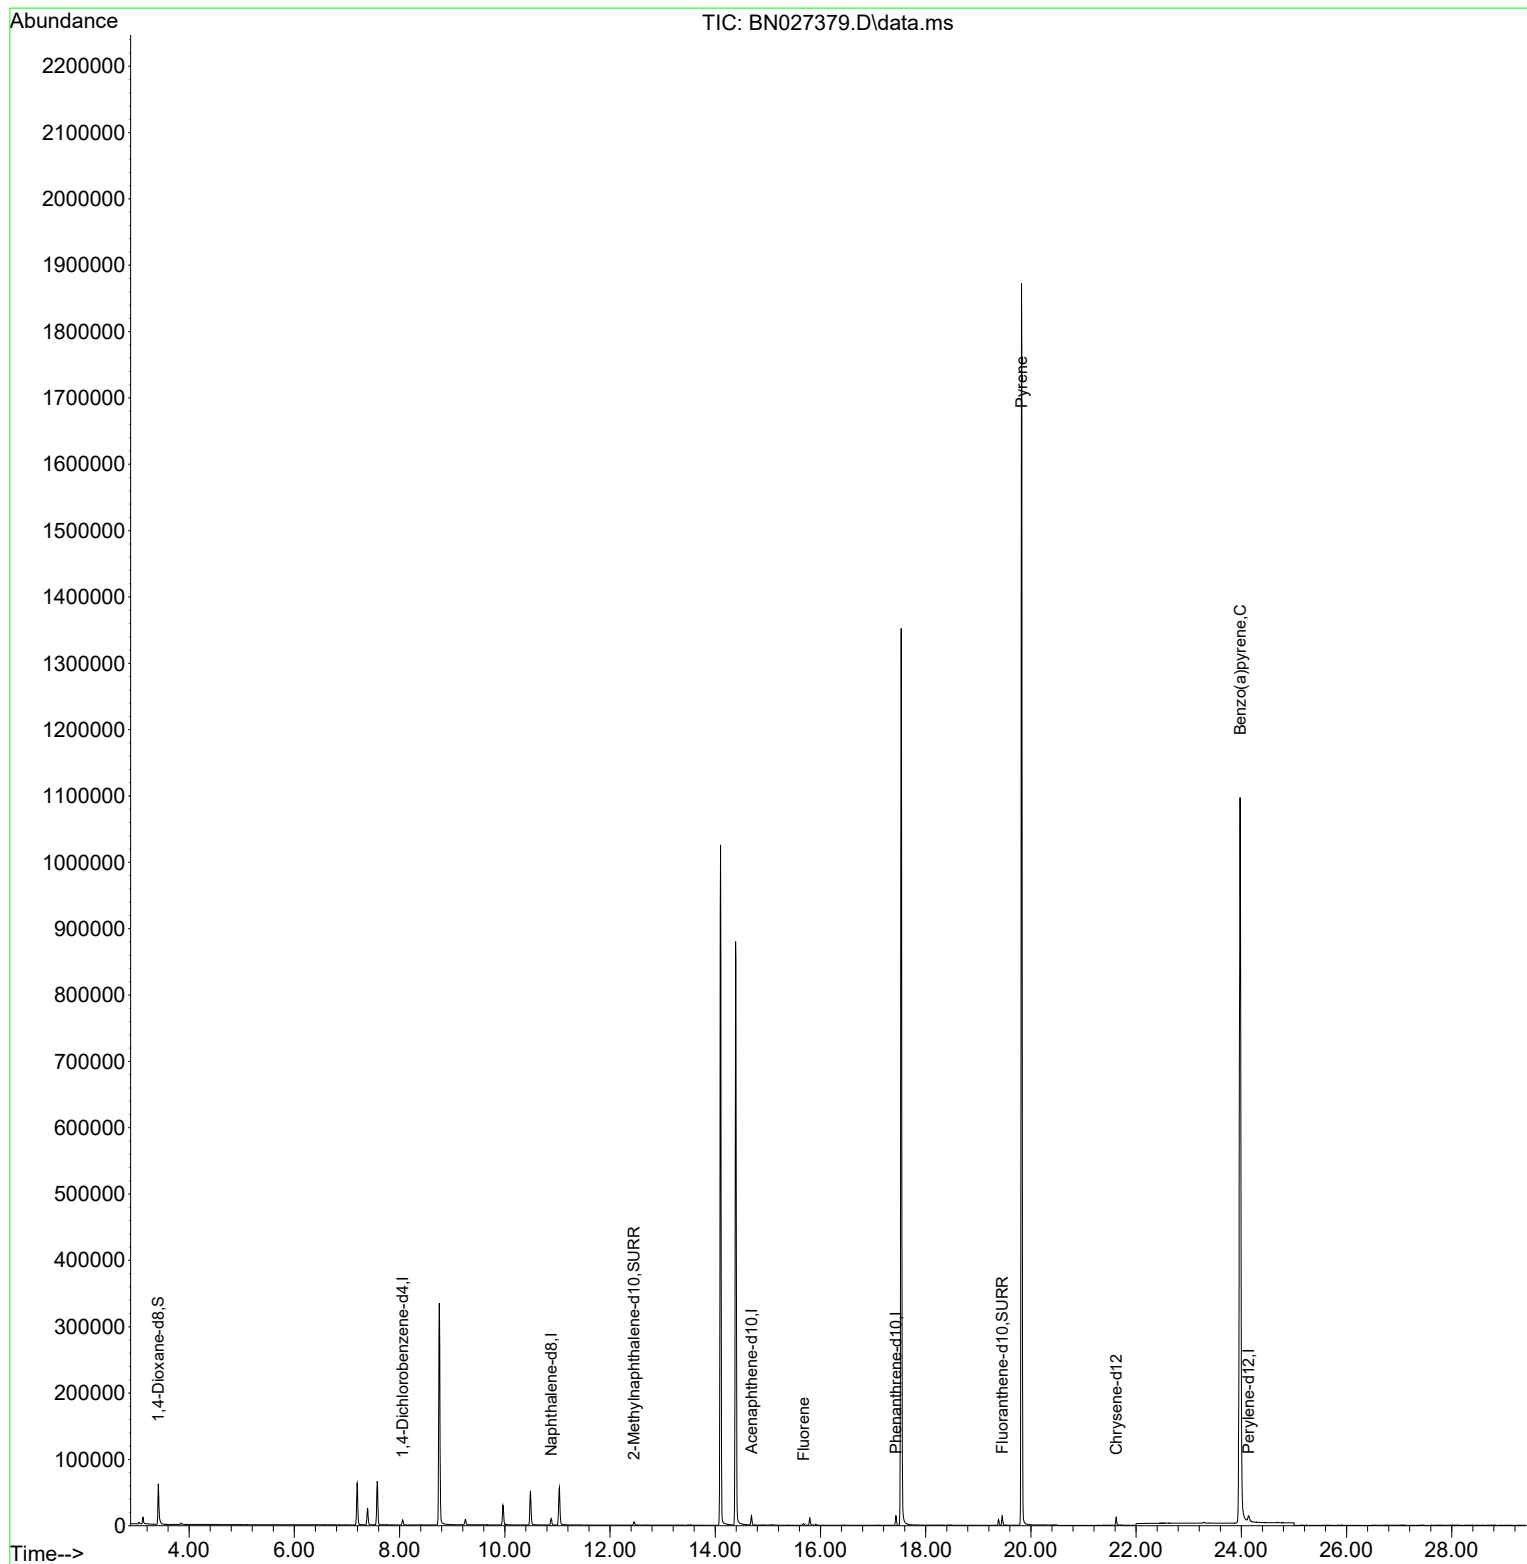


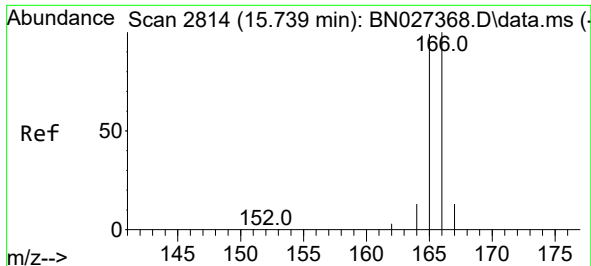

#12
 Fluorene
 Concen: 0.079 ng/ul
 RT: 15.679 min Scan# 21
 Delta R.T. -0.060 min
 Lab File: BN027379.D
 Acq: 05 Sep 2023 17:22




Instrument :
 BNA_N
 ClientSampleId :
 SBLK073


Tgt Ion:166 Resp: 2609
 Ion Ratio Lower Upper
 166 100
 165 9.3 79.6 119.4#
 167 35.5 11.4 17.0#

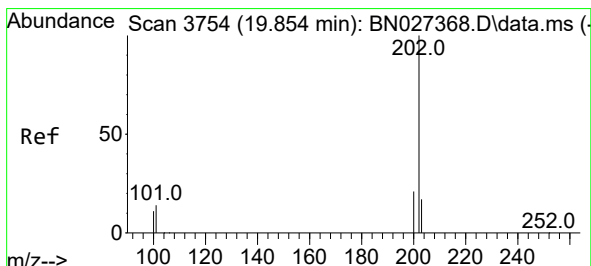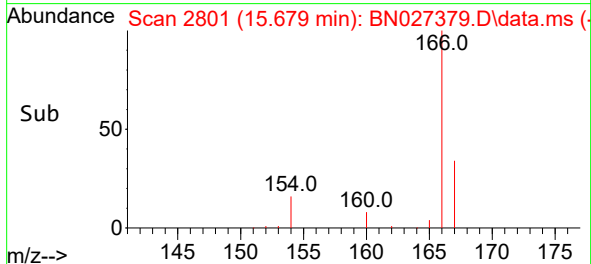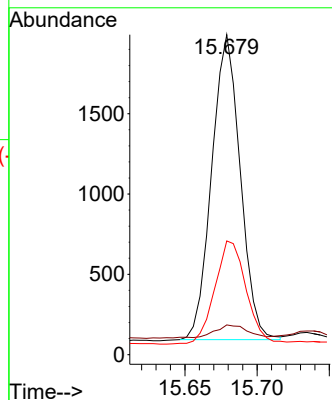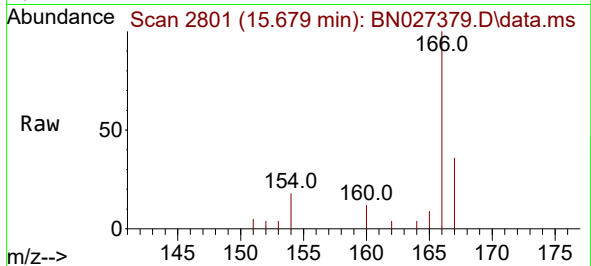

#20
 Pyrene
 Concen: 0.048 ng/ul
 RT: 19.822 min Scan# 3747
 Delta R.T. -0.028 min
 Lab File: BN027379.D
 Acq: 05 Sep 2023 17:22

Tgt Ion:202 Resp: 2792
 Ion Ratio Lower Upper
 202 100
 101 175.8 11.4 17.2#
 100 1347.4 9.4 14.2#

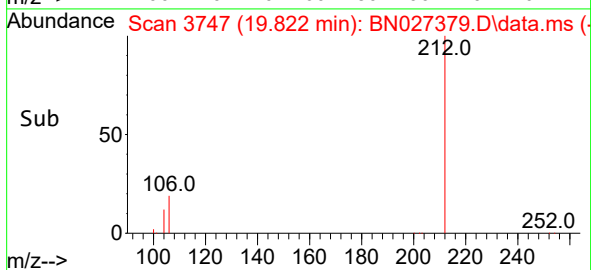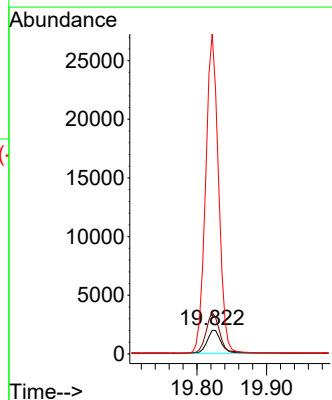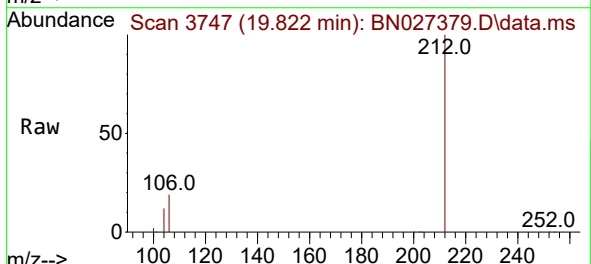

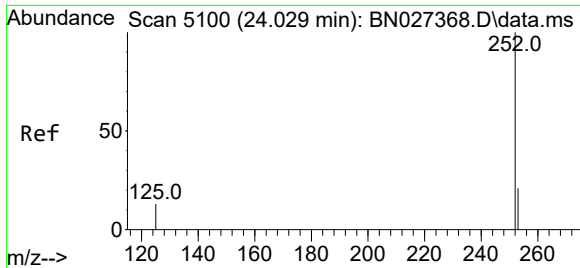

#26
 Benzo(a)pyrene
 Concen: 0.116 ng/ul
 RT: 23.977 min Scan# 50
 Delta R.T. -0.041 min
 Lab File: BN027379.D
 Acq: 05 Sep 2023 17:22

Instrument :
 BNA_N
 ClientSampleId :
 SBLK073

Tgt Ion:	252	Resp:	6247
Ion	Ratio	Lower	Upper
252	100		
253	44.3	22.4	33.6#
125	43.2	17.4	26.2#

