

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
 Data File : BN027385.D
 Acq On : 05 Sep 2023 21:09
 Operator : MA/JU
 Sample : 04148-01RE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH8S3

Quant Time: Sep 06 00:43:16 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	4192	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	14208	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	8398	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	19610	0.400	ng/ul	0.00
17) Chrysene-d12	21.612	240	16574	0.400	ng/ul	0.00
23) Perylene-d12	24.129	264	18375	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	27259	4.888	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	6537	0.303	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	18766	0.330	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.452	88	2966	0.526	ng/ul	93
20) Pyrene	19.822	202	3692	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.965	252	7151	0.106	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027385.D
Acq On : 05 Sep 2023 21:09
Operator : MA/JU
Sample : 04148-01RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH8S3

Quant Time: Sep 06 00:43:16 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




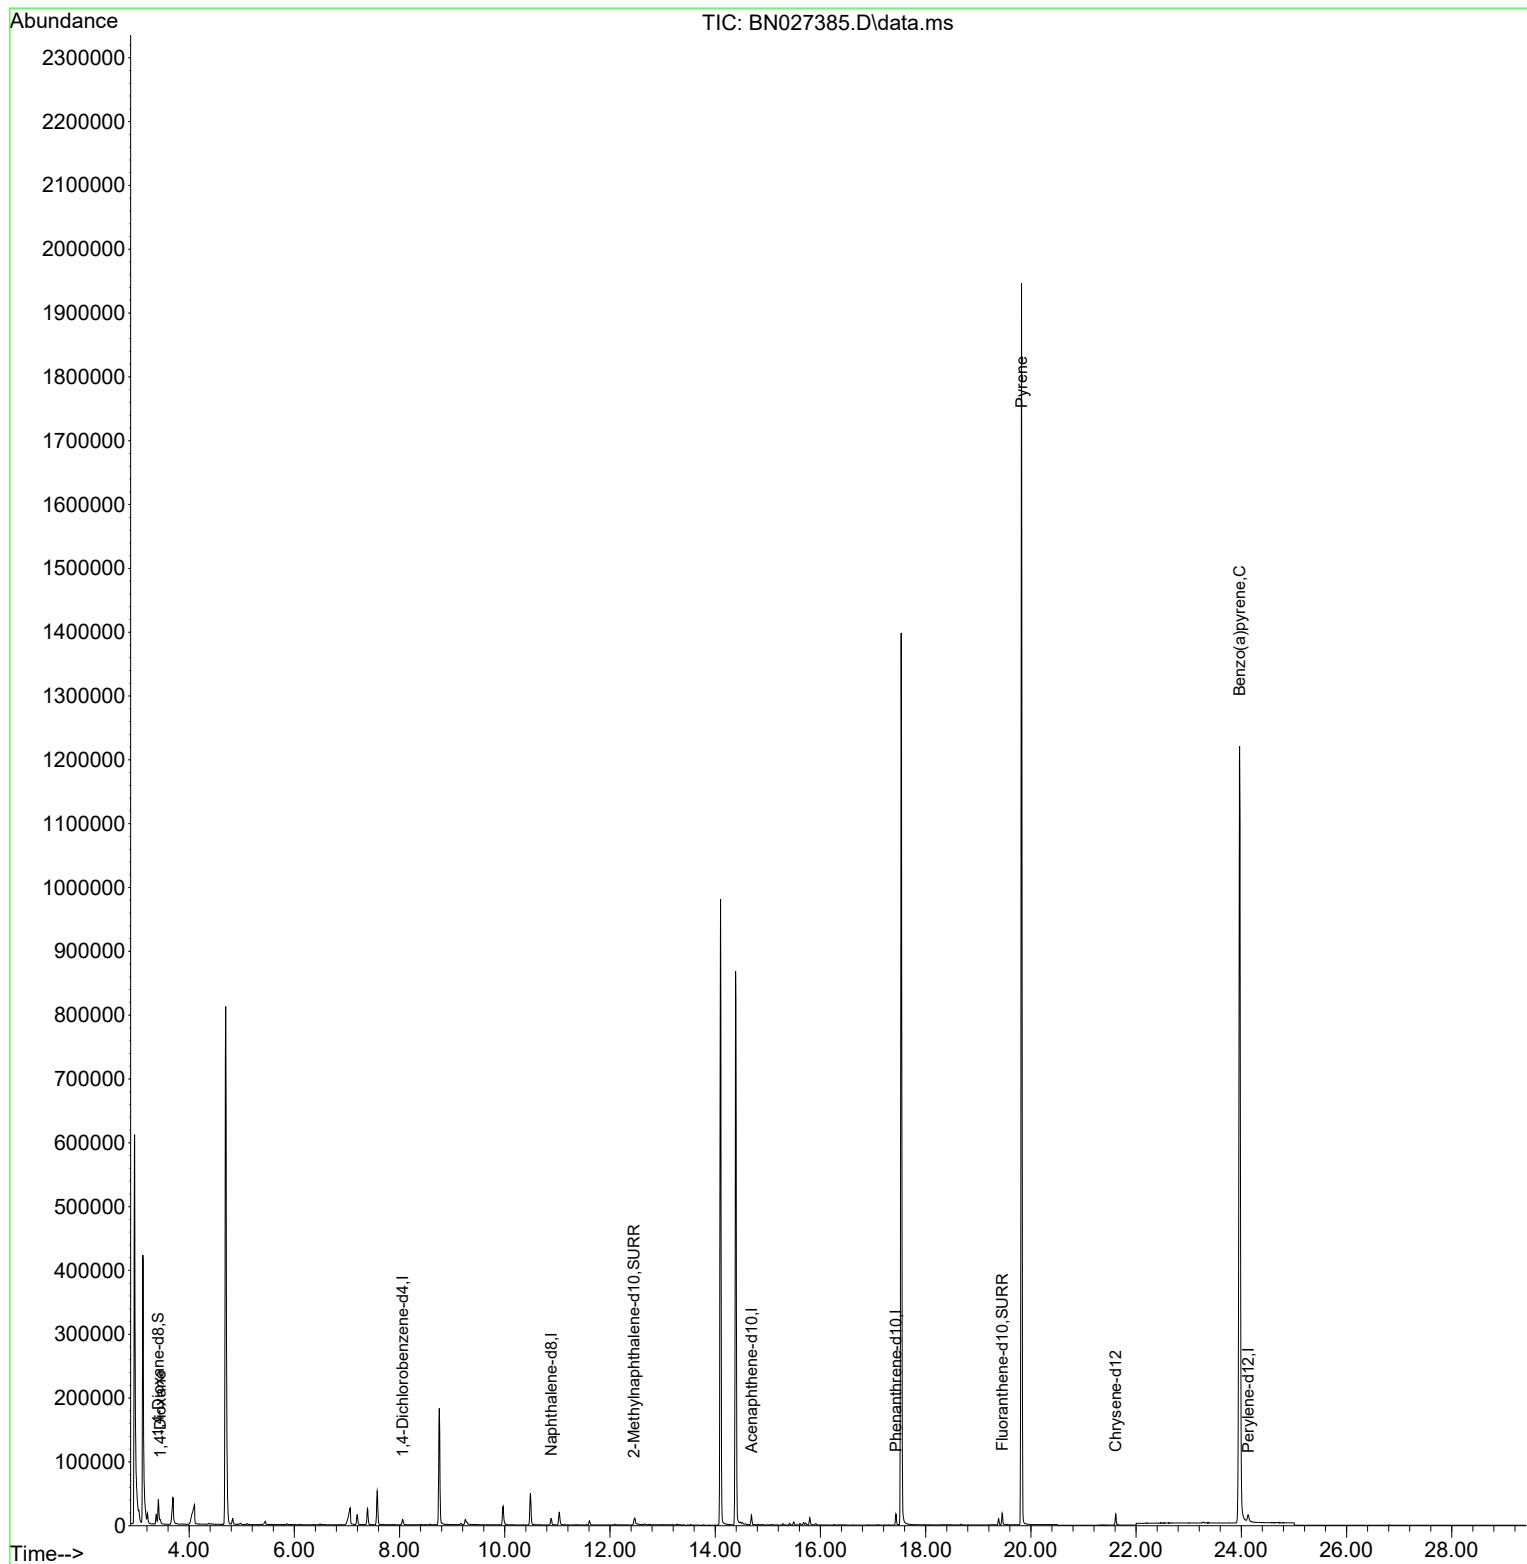


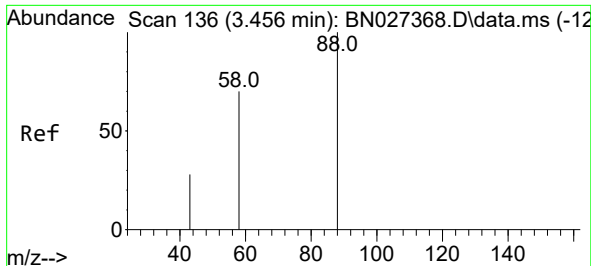

#2
1,4-Dioxane
Concen: 0.526 ng/ul
RT: 3.452 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN027385.D
Acq: 05 Sep 2023 21:09




Instrument :
BNA_N
ClientSampleId :
BH8S3


Tgt Ion: 88 Resp: 2966
Ion Ratio Lower Upper
88 100
43 37.1 26.8 40.2
58 55.2 39.9 59.9

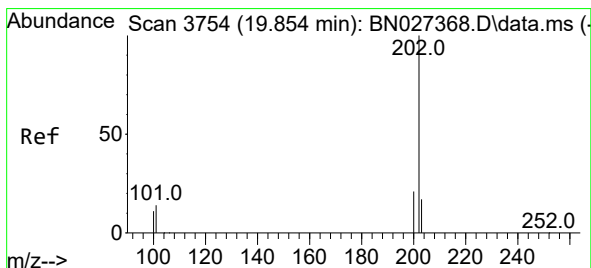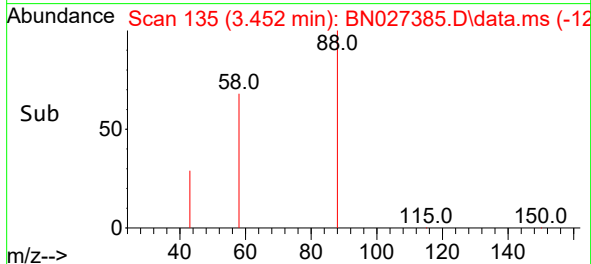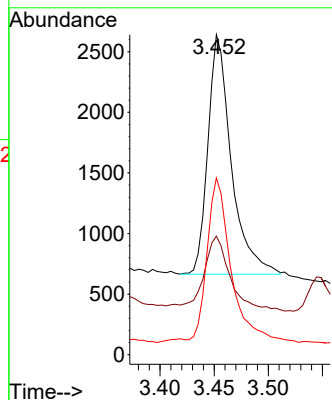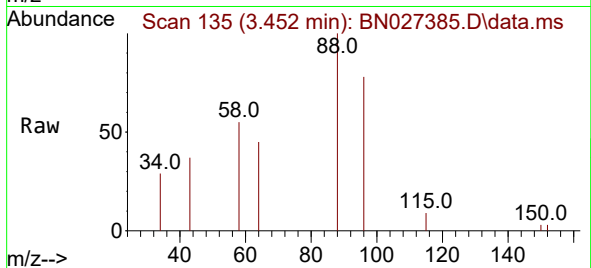

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.822 min Scan# 3747
Delta R.T. -0.028 min
Lab File: BN027385.D
Acq: 05 Sep 2023 21:09

Tgt Ion: 202 Resp: 3692
Ion Ratio Lower Upper
202 100
101 167.5 11.4 17.2#
100 1251.5 9.4 14.2#

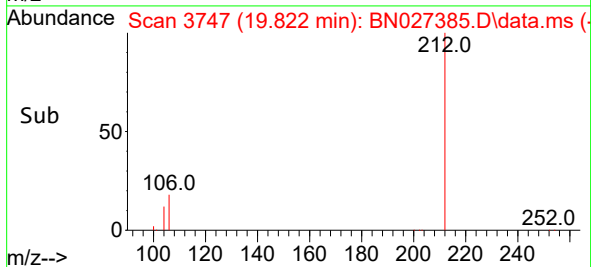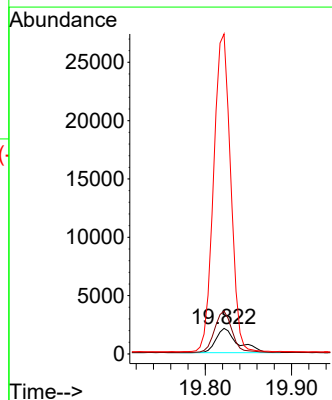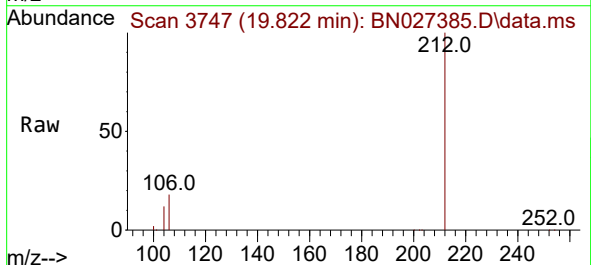

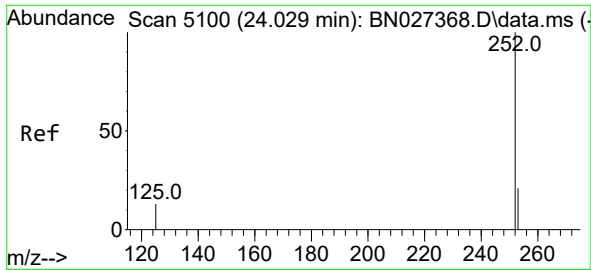

#26

Benzo(a)pyrene

Concen: 0.106 ng/ul

RT: 23.965 min Scan# 50

Delta R.T. -0.053 min

Lab File: BN027385.D


Acq: 05 Sep 2023 21:09

Instrument :

BNA_N

ClientSampleId :

BH8S3

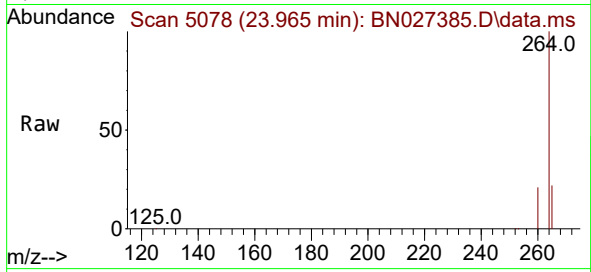

Tgt Ion:252 Resp: 7151

Ion Ratio Lower Upper

252 100

253 43.5 22.4 33.6#

125 42.5 17.4 26.2#

