

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
 Data File : BN027387.D
 Acq On : 05 Sep 2023 22:24
 Operator : MA/JU
 Sample : 04123-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH923

Quant Time: Sep 06 00:43:28 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	4224	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	14822	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	8606	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	19603	0.400	ng/ul	0.00
17) Chrysene-d12	21.609	240	16367	0.400	ng/ul	0.00
23) Perylene-d12	24.126	264	19160	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	27754	4.939	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	7288	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	19004	0.339	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.452	88	1142	0.201	ng/ul#	87
20) Pyrene	19.822	202	3210	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.962	252	7403	0.105	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027387.D
Acq On : 05 Sep 2023 22:24
Operator : MA/JU
Sample : 04123-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH923

Quant Time: Sep 06 00:43:28 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




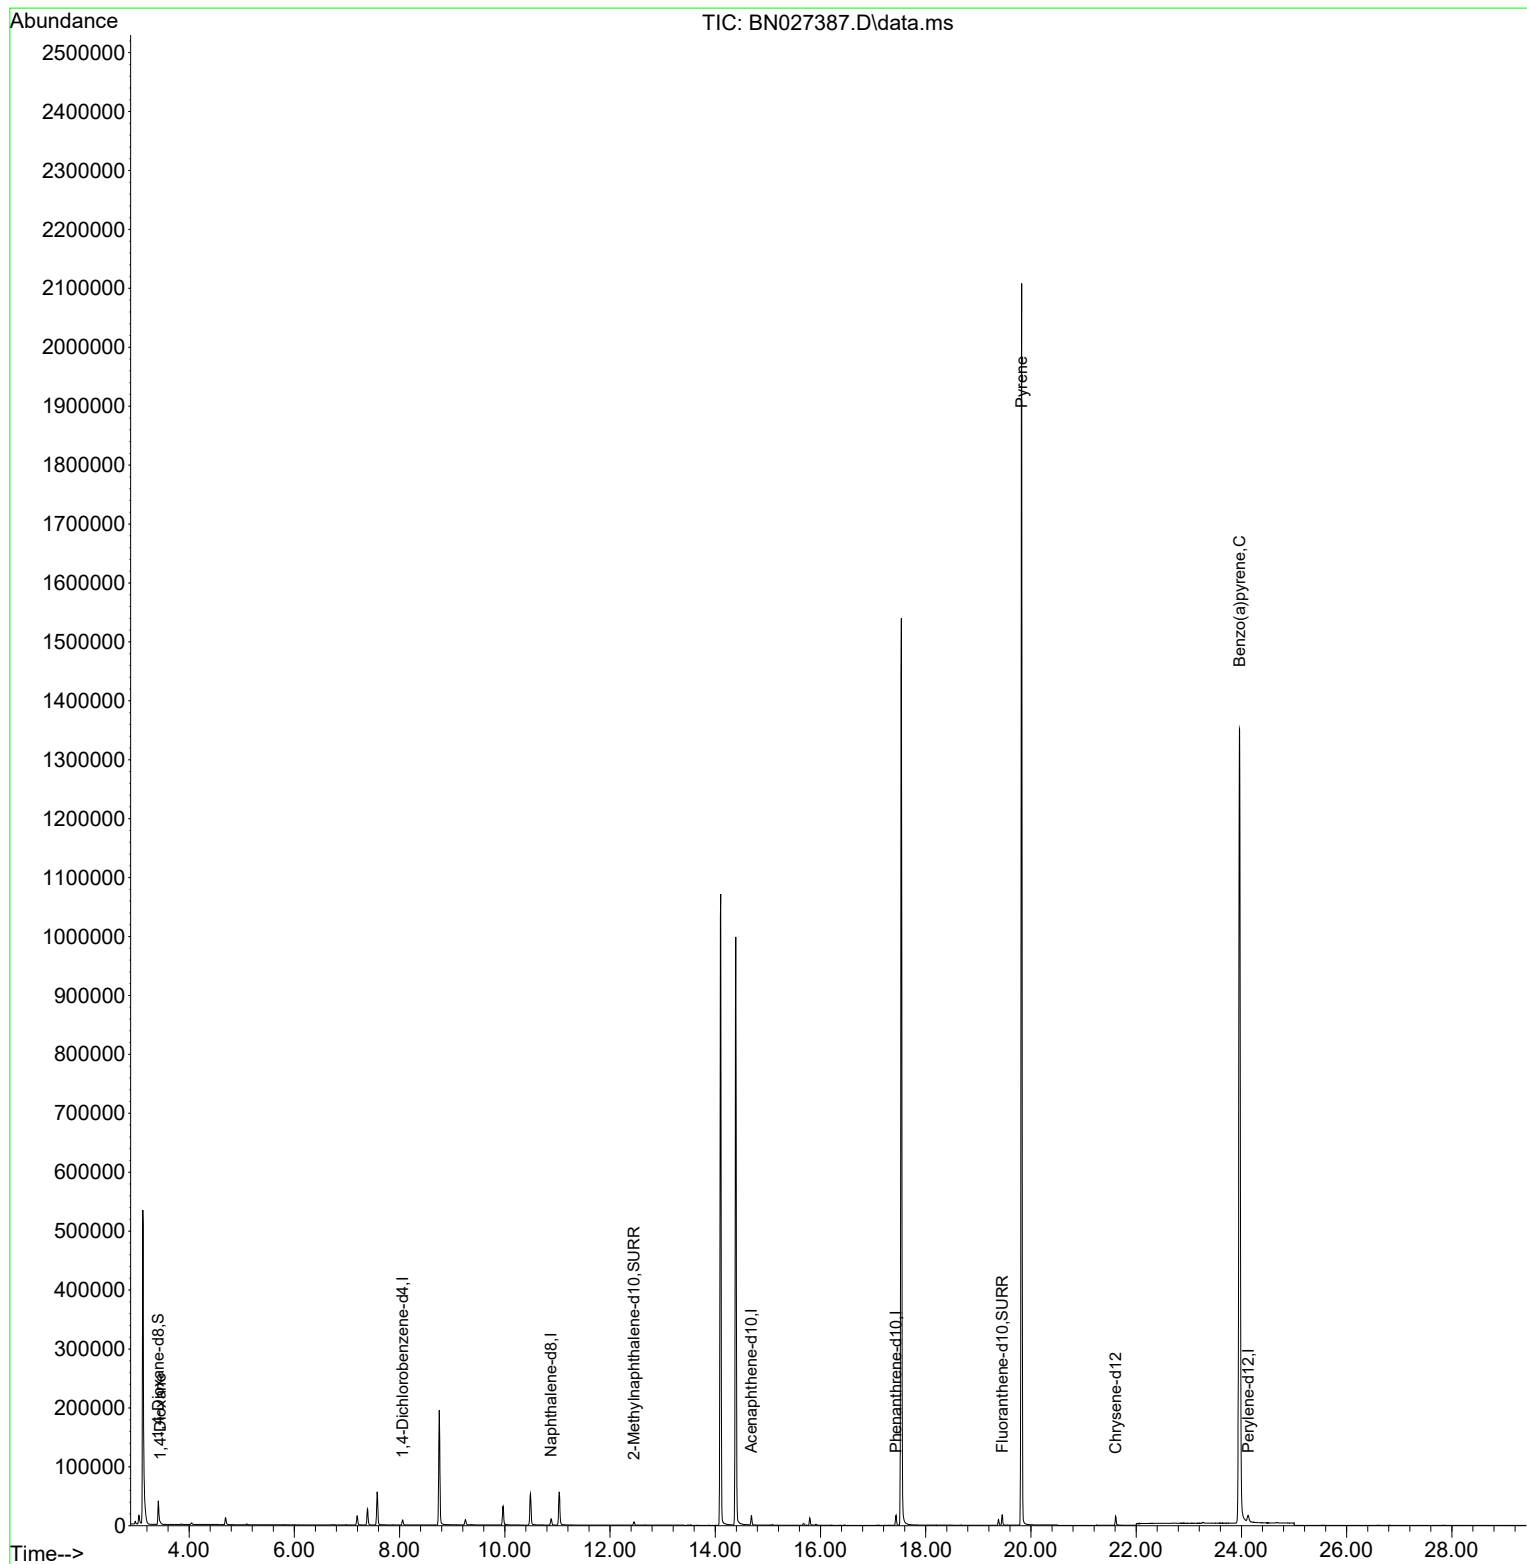


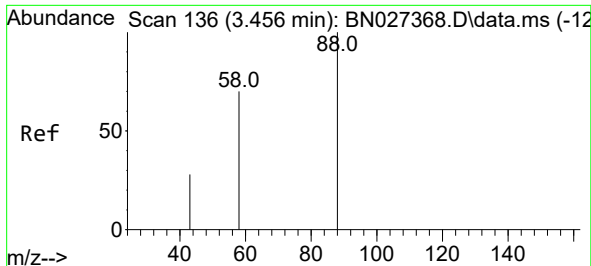

#2
1,4-Dioxane
Concen: 0.201 ng/ul
RT: 3.452 min Scan# 1142
Delta R.T. -0.004 min
Lab File: BN027387.D
Acq: 05 Sep 2023 22:24




Instrument :
BNA_N
ClientSampleId :
BH923


Tgt Ion: 88 Resp: 1142
Ion Ratio Lower Upper
88 100
43 43.6 26.8 40.2#
58 43.4 39.9 59.9

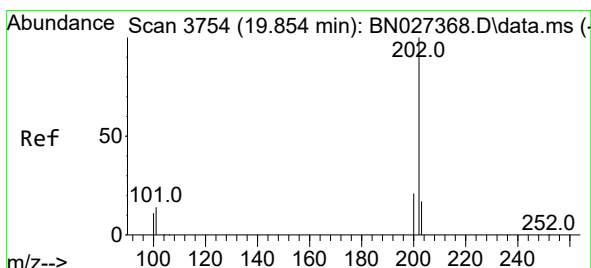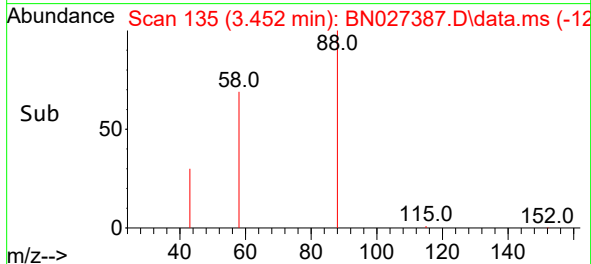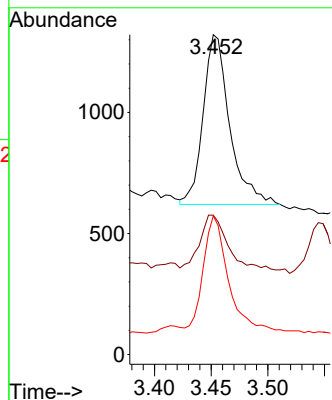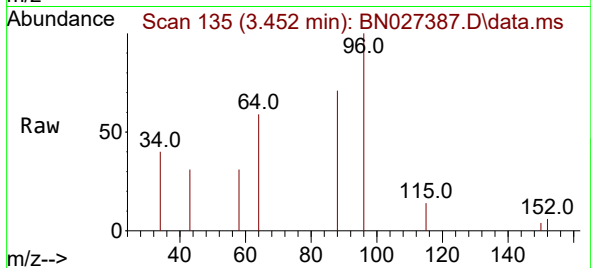

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.822 min Scan# 3747
Delta R.T. -0.028 min
Lab File: BN027387.D
Acq: 05 Sep 2023 22:24


Tgt Ion: 202 Resp: 3210
Ion Ratio Lower Upper
202 100
101 163.2 11.4 17.2#
100 1196.6 9.4 14.2#

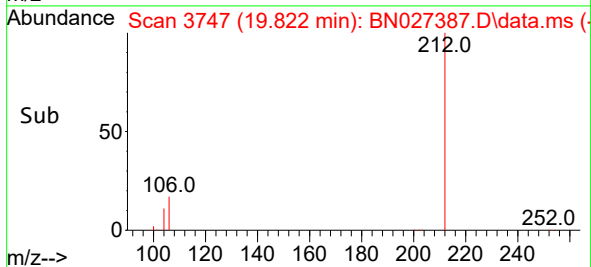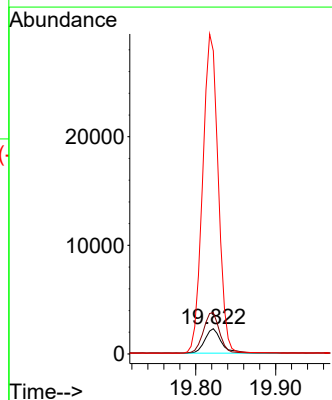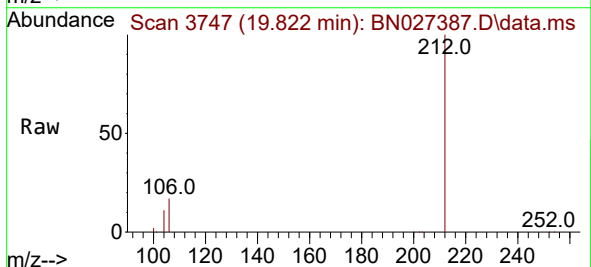

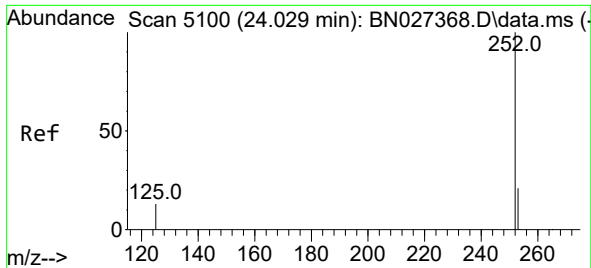

#26
Benzo(a)pyrene
Concen: 0.105 ng/ul
RT: 23.962 min Scan# 50
Delta R.T. -0.055 min
Lab File: BN027387.D
Acq: 05 Sep 2023 22:24

Instrument :
BNA_N
ClientSampleId :
BH923

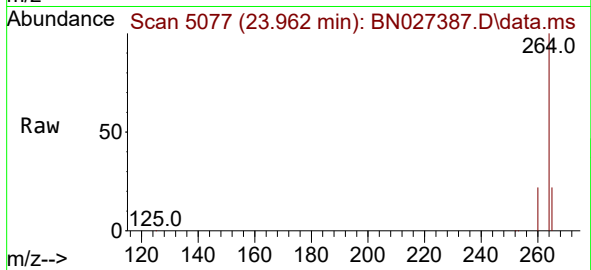

Tgt Ion:252 Resp: 7403
Ion Ratio Lower Upper
252 100
253 42.1 22.4 33.6#
125 40.1 17.4 26.2#

