

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
 Data File : BN027372.D
 Acq On : 05 Sep 2023 13:00
 Operator : MA/JU
 Sample : 04134-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCHJ7

Quant Time: Sep 06 00:49:05 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	4287	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	15182	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	9576	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.435	188	21814	0.400	ng/ul	0.00
17) Chrysene-d12	21.612	240	16427	0.400	ng/ul	0.00
23) Perylene-d12	24.135	264	15897	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	25609	4.491	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	7556	0.328	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	20618	0.366	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.059	266	22151	5.208	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027372.D
Acq On : 05 Sep 2023 13:00
Operator : MA/JU
Sample : 04134-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCHJ7

Quant Time: Sep 06 00:49:05 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

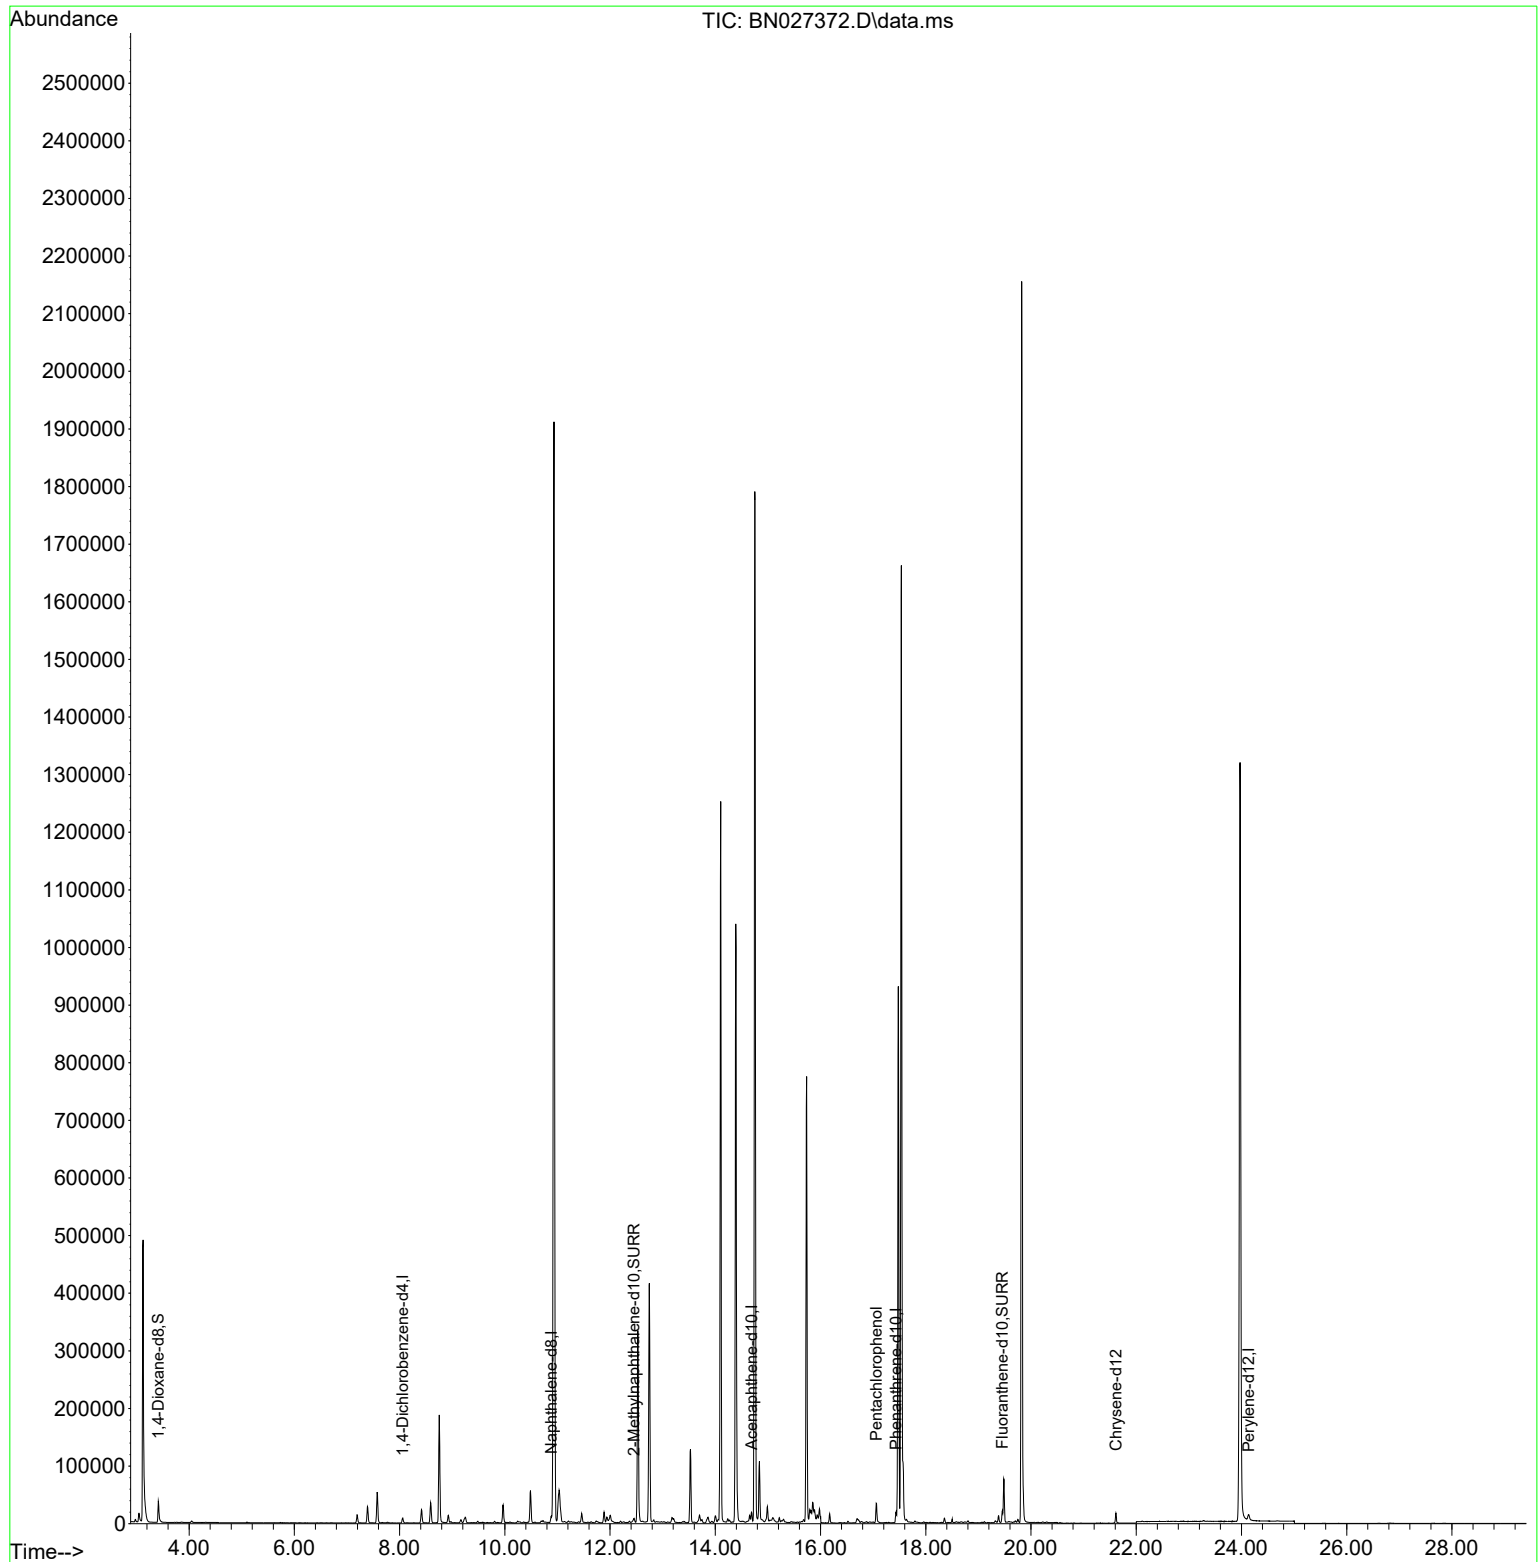

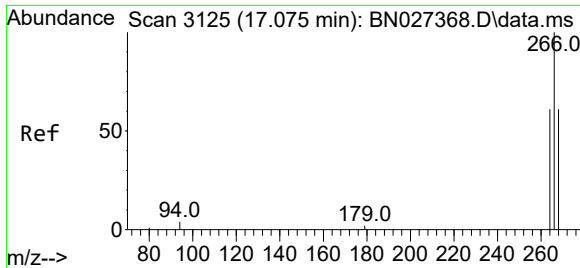

#14
 Pentachlorophenol
 Concen: 5.208 ng/ul
 RT: 17.059 min Scan# 31
 Delta R.T. -0.008 min
 Lab File: BN027372.D
 Acq: 05 Sep 2023 13:00

Instrument :
 BNA_N
 ClientSampleId :
 DCHJ7

Tgt Ion:	266	Resp:	22151
Ion	Ratio	Lower	Upper
266	100		
264	62.9	50.4	75.6
268	63.8	51.9	77.9

