

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
 Data File : BN027373.D
 Acq On : 05 Sep 2023 13:37
 Operator : MA/JU
 Sample : 04134-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCHJ9

Quant Time: Sep 06 00:41:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	3823	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	13536	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	9007	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.434	188	19874	0.400	ng/ul	0.00
17) Chrysene-d12	21.615	240	16321	0.400	ng/ul	0.00
23) Perylene-d12	24.137	264	17493	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	23169	4.556	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	7947	0.387	ng/ul	0.00
18) Fluoranthene-d10	19.454	212	21875	0.391	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.063	266	17958	4.635	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027373.D
Acq On : 05 Sep 2023 13:37
Operator : MA/JU
Sample : 04134-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCHJ9


Quant Time: Sep 06 00:41:50 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

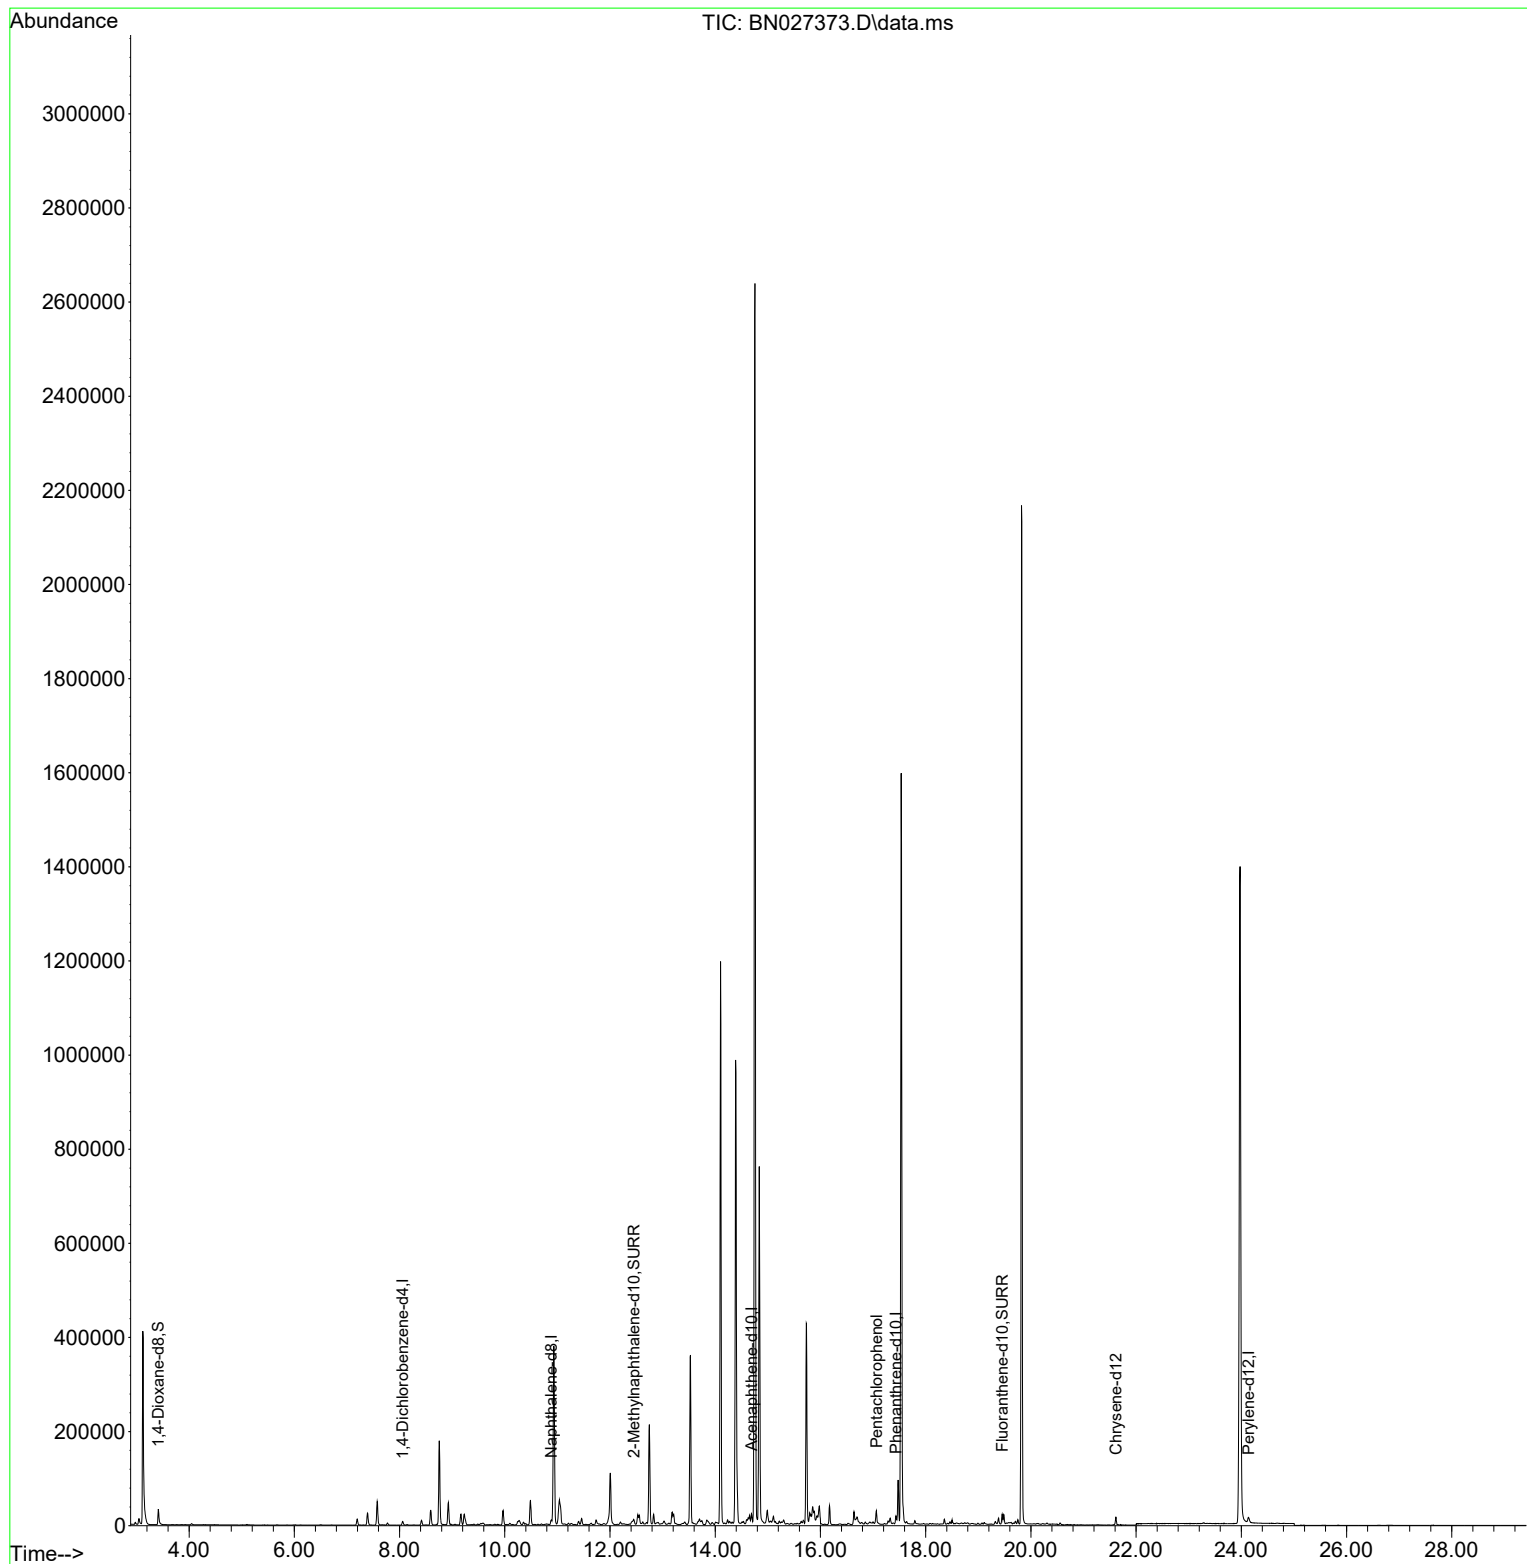

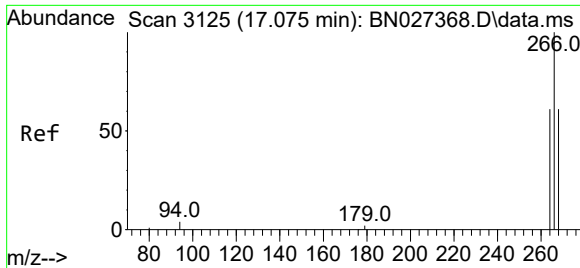

#14
Pentachlorophenol
Concen: 4.635 ng/ul
RT: 17.063 min Scan# 31
Delta R.T. -0.004 min
Lab File: BN027373.D
Acq: 05 Sep 2023 13:37

Instrument :
BNA_N
ClientSampleId :
DCHJ9

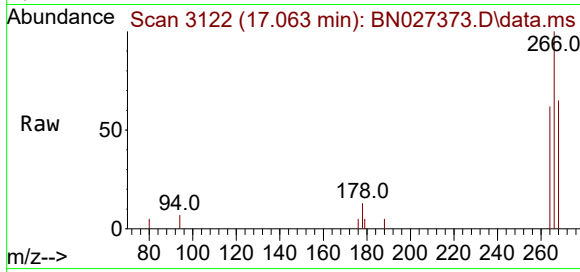

Tgt Ion:266 Resp: 17958
Ion Ratio Lower Upper
266 100
264 63.0 50.4 75.6
268 63.9 51.9 77.9

