

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
 Data File : BN027381.D
 Acq On : 05 Sep 2023 18:38
 Operator : MA/JU
 Sample : 04134-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCHJ8

Quant Time: Sep 06 00:42:47 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	4077	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	14088	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	7753	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.435	188	17976	0.400	ng/ul	0.00
17) Chrysene-d12	21.612	240	14803	0.400	ng/ul	0.00
23) Perylene-d12	24.132	264	16382	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.418	96	26315	4.852	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	5978	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	16823	0.332	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.063	266	955	0.272	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027381.D
Acq On : 05 Sep 2023 18:38
Operator : MA/JU
Sample : 04134-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCHJ8


Quant Time: Sep 06 00:42:47 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

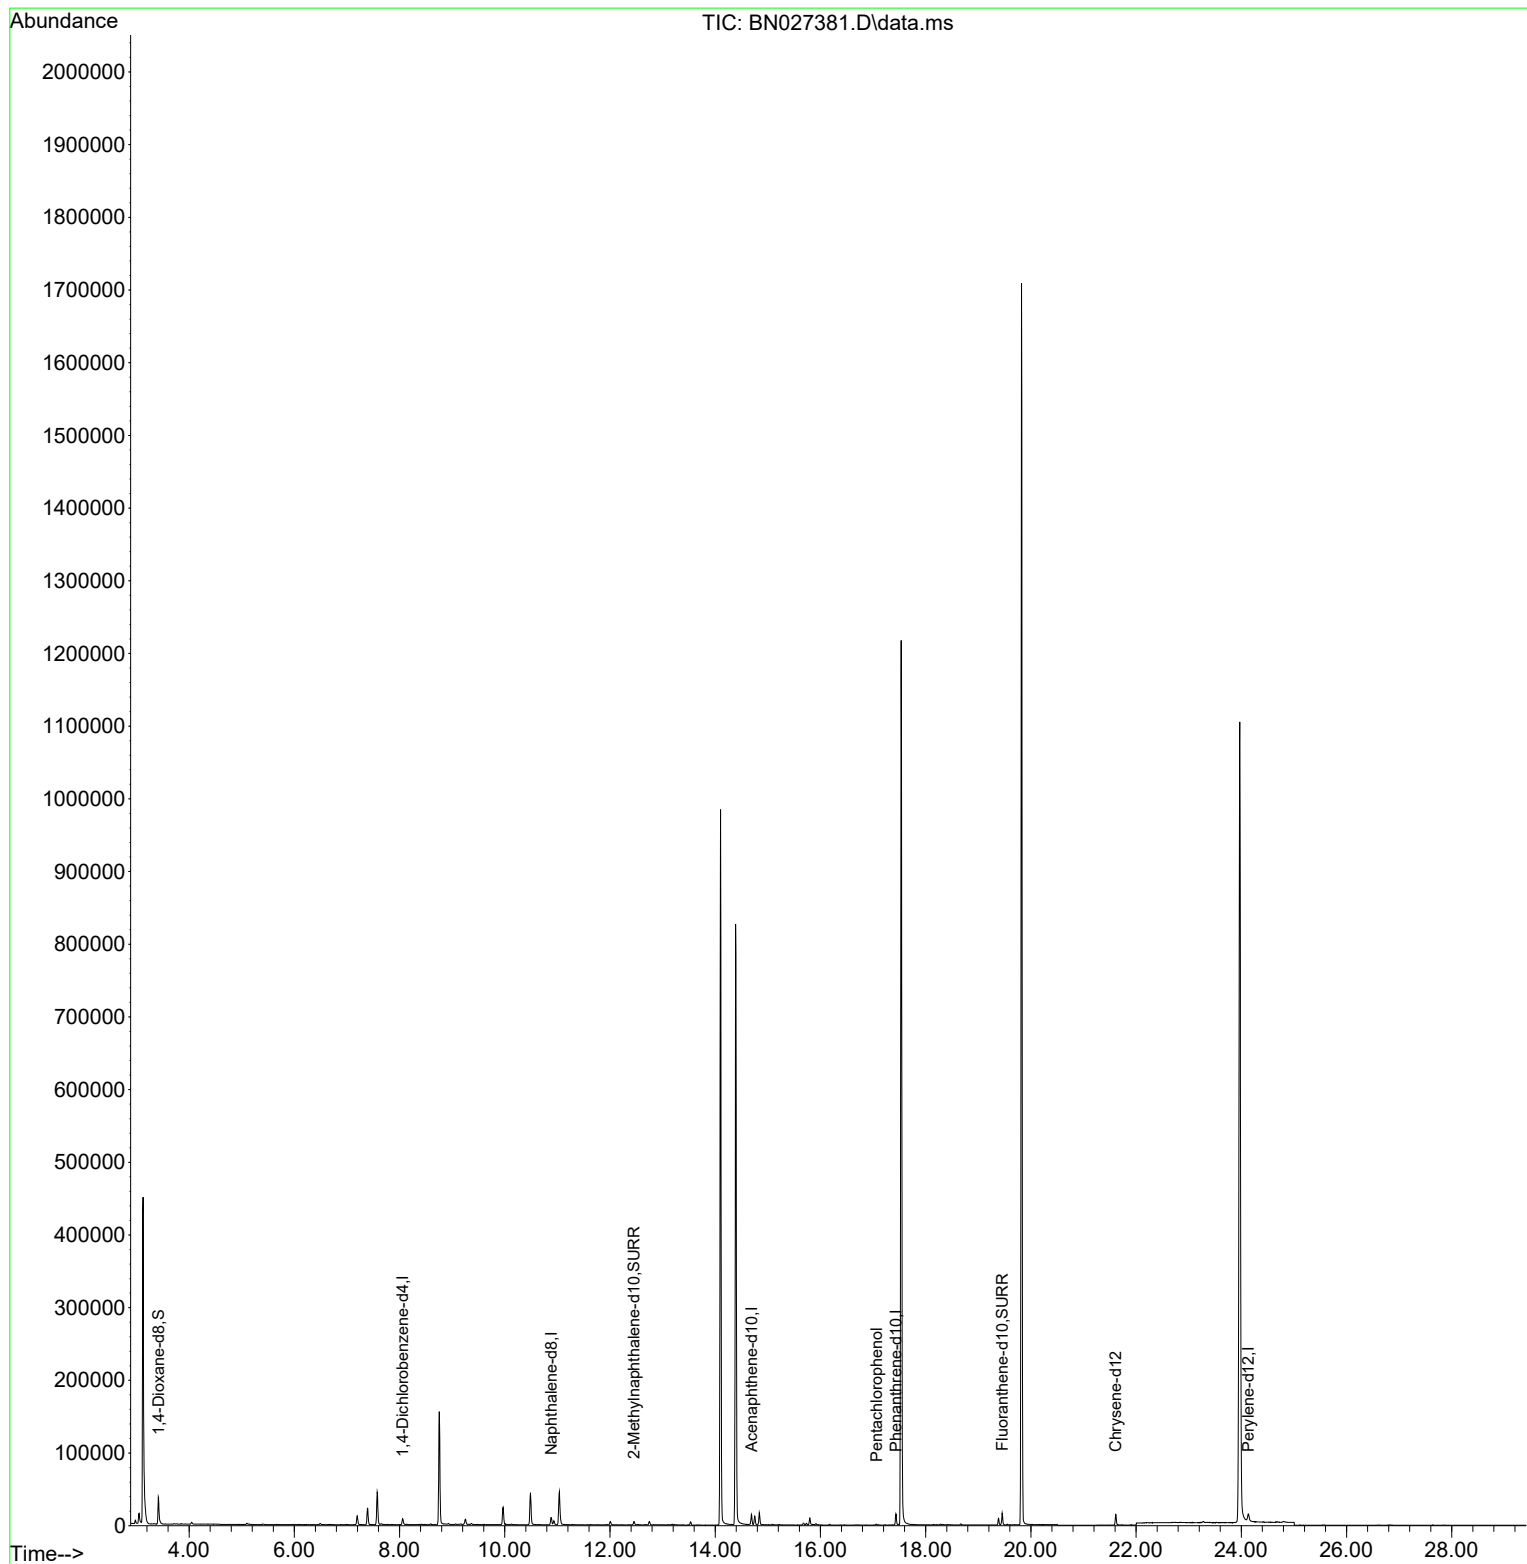

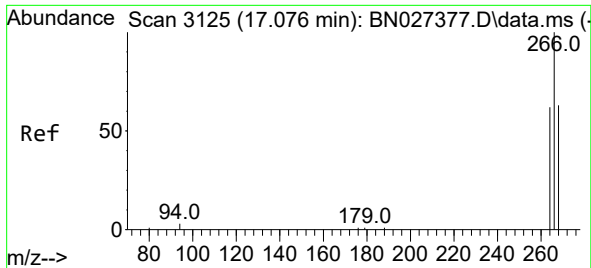

#14
Pentachlorophenol
Concen: 0.272 ng/ul
RT: 17.063 min Scan# 3122
Delta R.T. -0.004 min
Lab File: BN027381.D
Acq: 05 Sep 2023 18:38

Instrument :
BNA_N
ClientSampleId :
DCHJ8

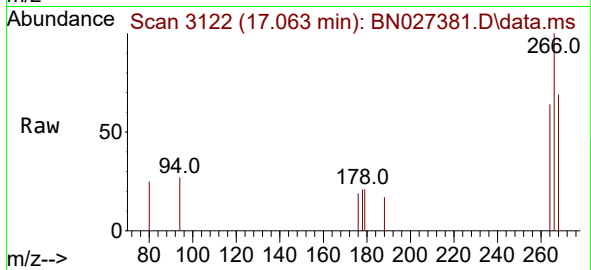

Tgt Ion:	266	Resp:	955
Ion	Ratio	Lower	Upper
266	100		
264	62.8	50.4	75.6
268	63.8	51.9	77.9

