

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
 Data File : BN027383.D
 Acq On : 05 Sep 2023 19:54
 Operator : MA/JU
 Sample : 04134-06DL 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCHJ9DL

Quant Time: Sep 06 00:43:02 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	4208	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	13761	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	8213	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.435	188	19745	0.400	ng/ul	0.00
17) Chrysene-d12	21.612	240	15424	0.400	ng/ul	0.00
23) Perylene-d12	24.138	264	12702	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.418	96	1450	0.259	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	599	0.029	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	1666	0.032	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.063	266	1248	0.324	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027383.D
Acq On : 05 Sep 2023 19:54
Operator : MA/JU
Sample : 04134-06DL 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCHJ9DL


Quant Time: Sep 06 00:43:02 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

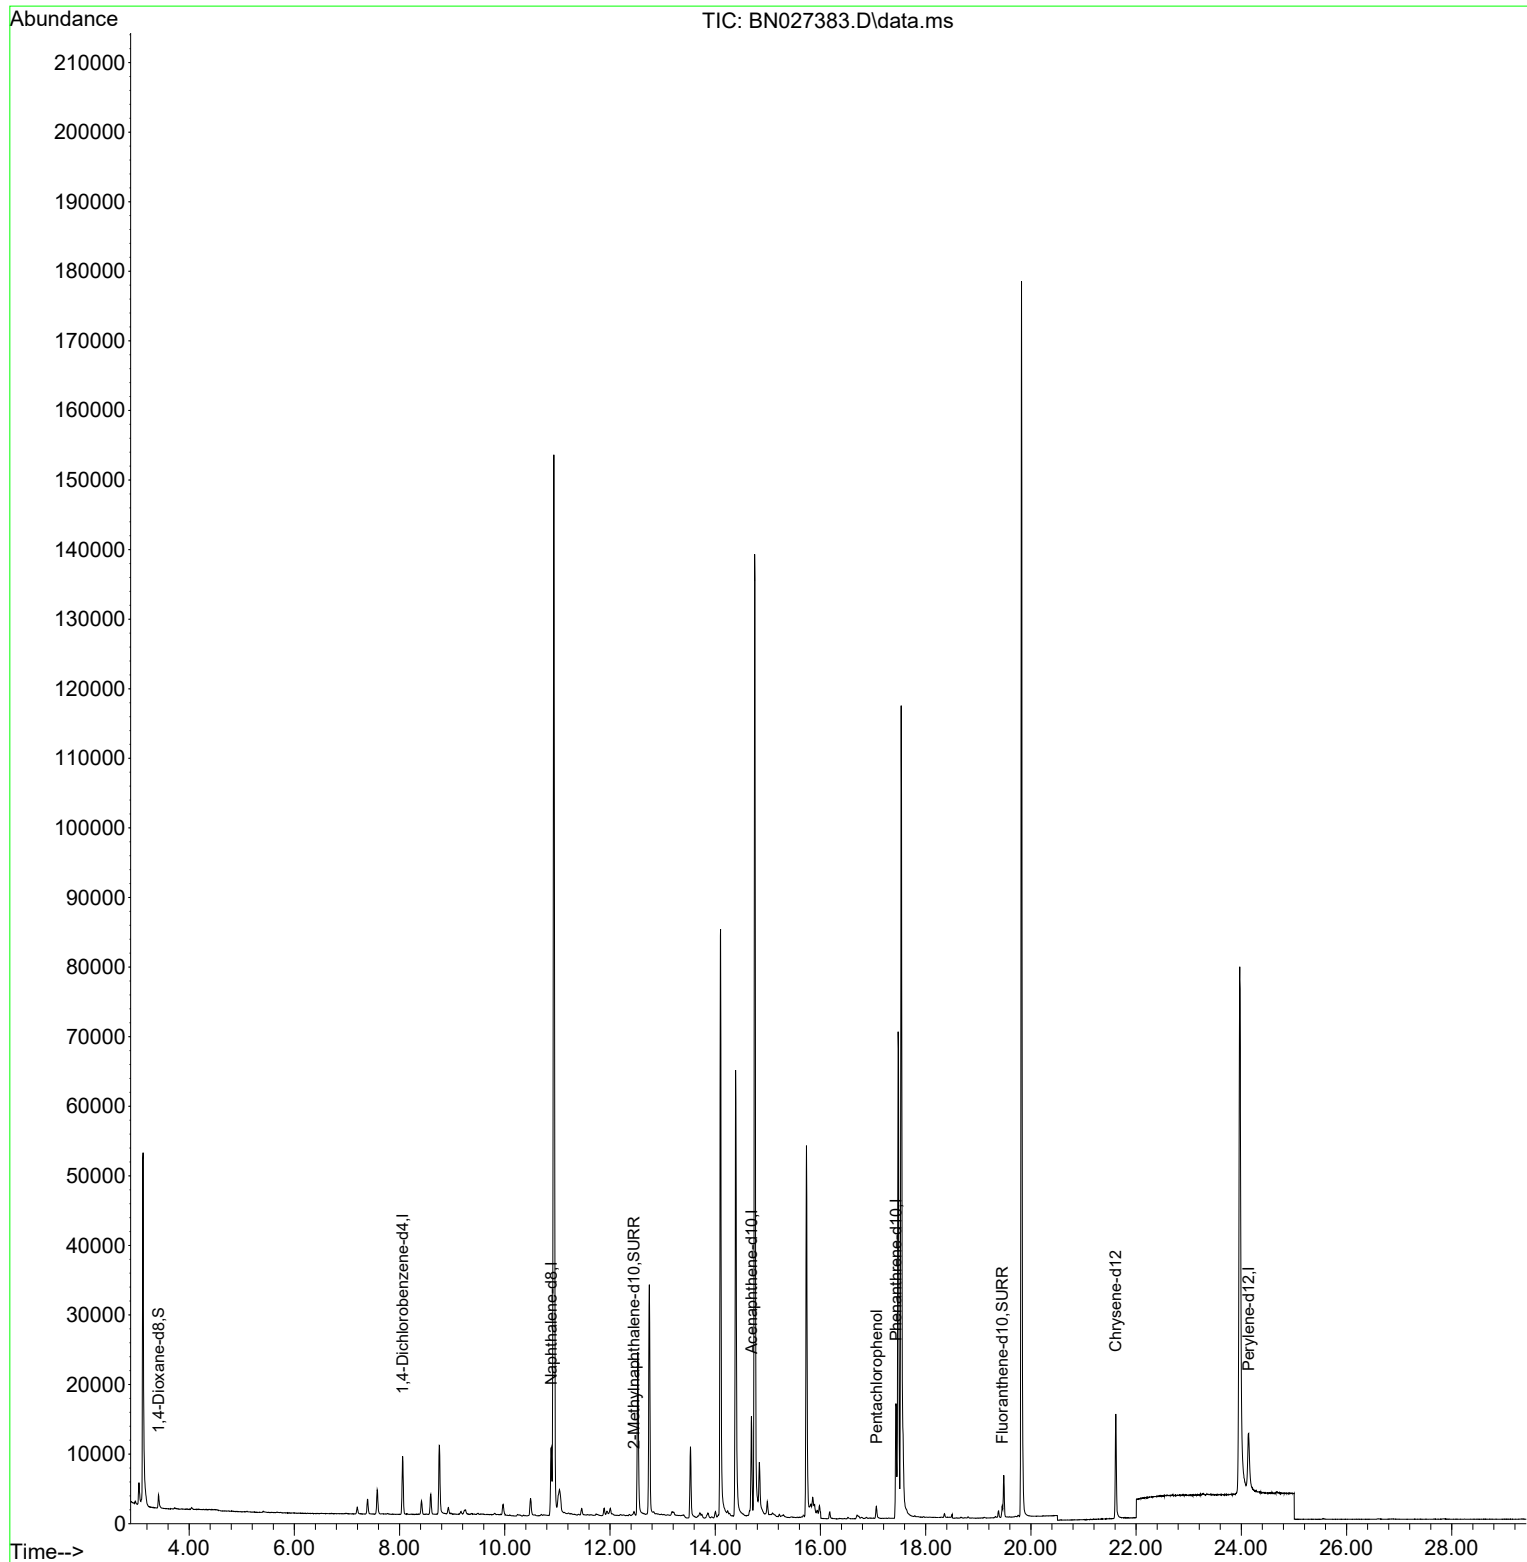

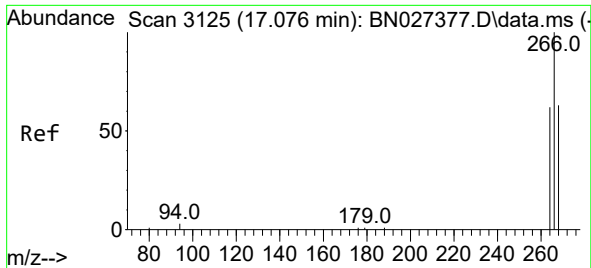

#14
 Pentachlorophenol
 Concen: 0.324 ng/ul
 RT: 17.063 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN027383.D
 Acq: 05 Sep 2023 19:54

Instrument :
 BNA_N
 ClientSampleId :
 DCHJ9DL

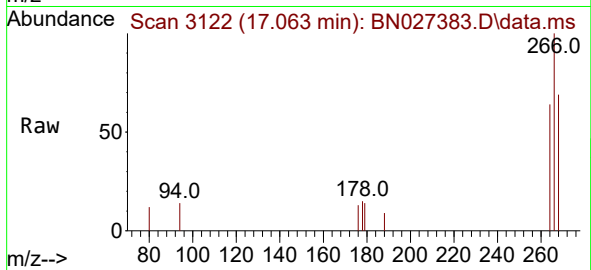

Tgt Ion:266 Resp: 1248
 Ion Ratio Lower Upper
 266 100
 264 63.1 50.4 75.6
 268 63.9 51.9 77.9

