

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
 Data File : BN027397.D
 Acq On : 06 Sep 2023 05:59
 Operator : MA/JU
 Sample : 04148-07RE
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJX0RE

Quant Time: Sep 06 06:29:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4347	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	15105	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.684	164	9549	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	21709	0.400	ng/ul #	0.00
17) Chrysene-d12	21.609	240	20043	0.400	ng/ul #	0.00
23) Perylene-d12	24.126	264	23865	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.418	96	26400	4.566	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	8613	0.376	ng/ul	0.00
18) Fluoranthene-d10	19.450	212	26007	0.379	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.456	88	1831	0.313	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027397.D
Acq On : 06 Sep 2023 05:59
Operator : MA/JU
Sample : 04148-07RE
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJX0RE

Quant Time: Sep 06 06:29:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

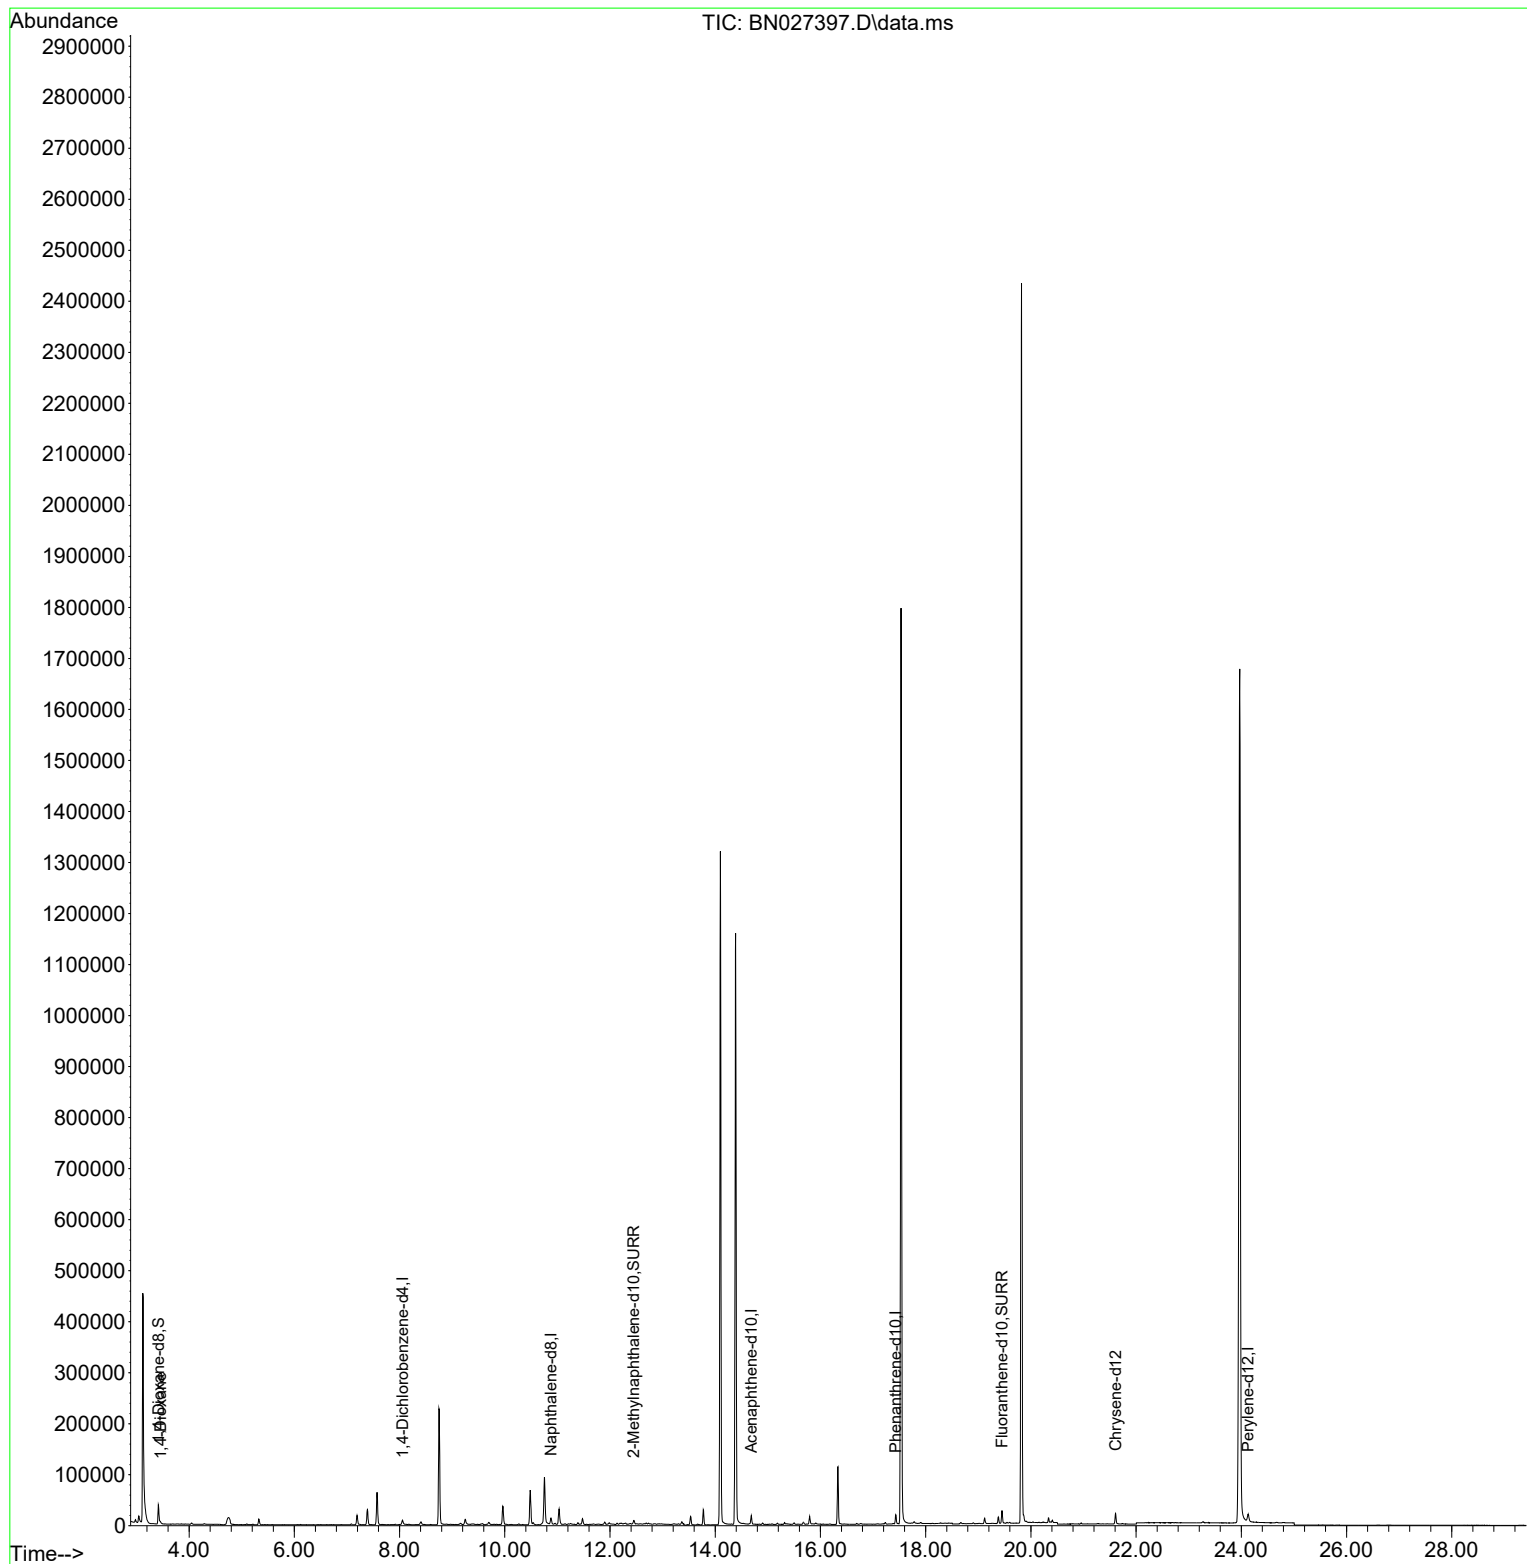

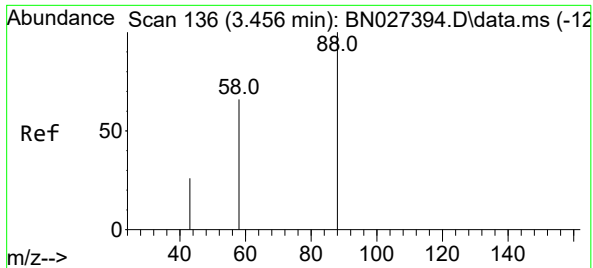

#2
 1,4-Dioxane
 Concen: 0.313 ng/ul
 RT: 3.456 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BN027397.D
 Acq: 06 Sep 2023 05:59

Instrument :
 BNA_N
 ClientSampleId :
 BBJX0RE

Tgt Ion:	88	Resp:	1831
Ion	Ratio	Lower	Upper
88	100		
43	36.7	26.8	40.2
58	33.8	39.9	59.9

