


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090523\
Data File : BN027367.D
Acq On : 05 Sep 2023 09:56
Operator : MA/JU
Sample : DFTPP369
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP369

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 02 06:16:48 2023

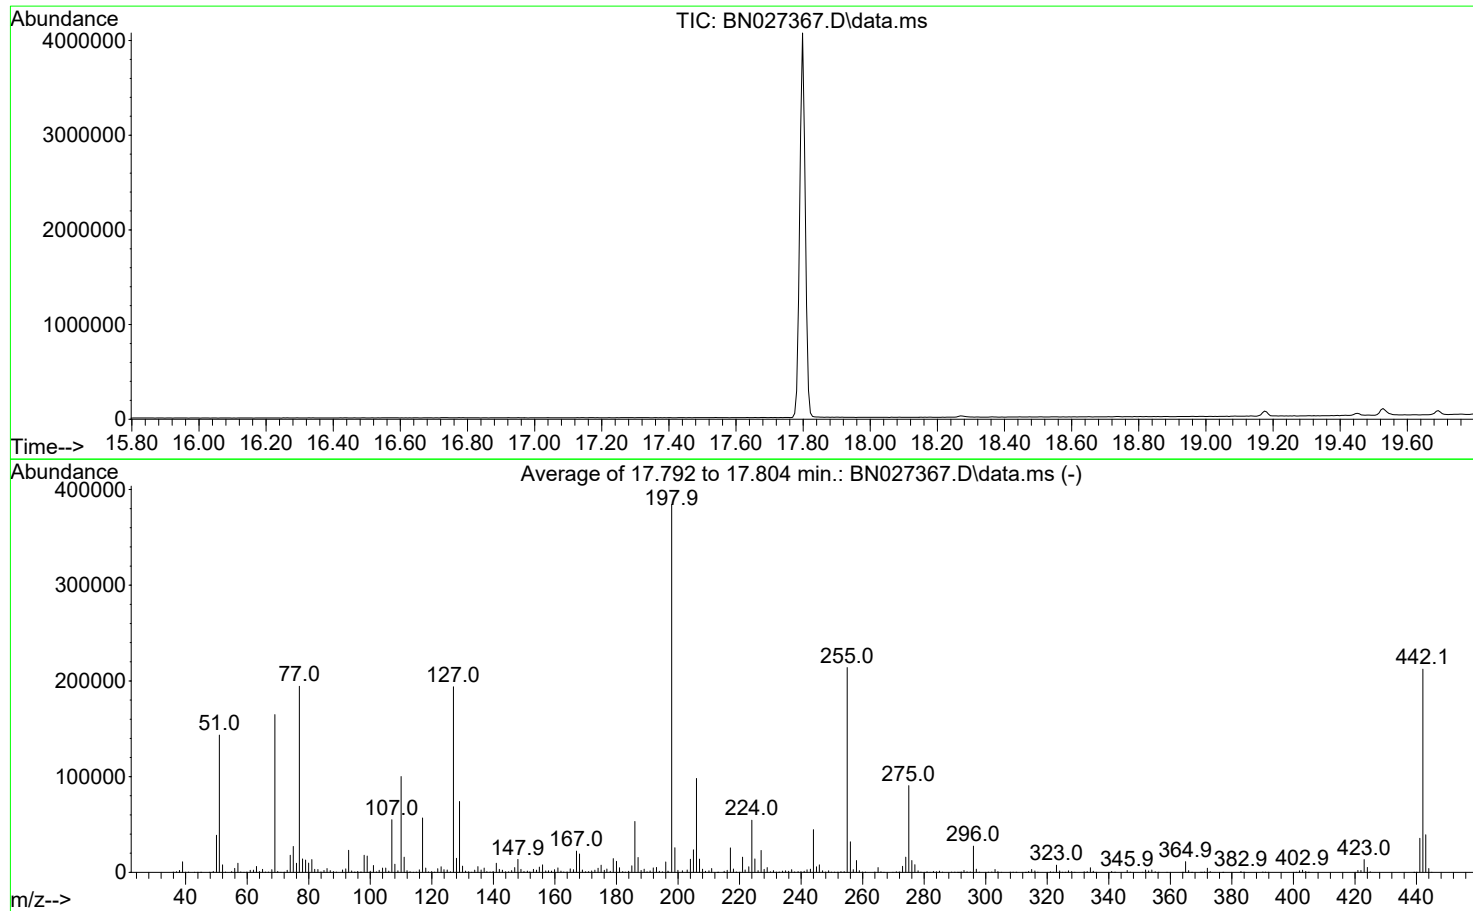

AutoFind: Scans 2534, 2535, 2536; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	143445	PASS
68	69	0.00	2	1.7	2798	PASS
69	198	0.00	100	42.9	164800	PASS
70	69	0.00	2	0.6	990	PASS
127	198	10	80	50.5	194005	PASS
197	198	0.00	2	0.3	1271	PASS
198	198	100	100	100.0	384320	PASS
199	198	5	9	6.7	25744	PASS
275	198	10	60	23.6	90544	PASS
365	198	1	100	2.9	11266	PASS
441	198	0.01	100	9.3	35563	PASS
442	198	50	100	55.3	212373	PASS
443	442	15	24	18.5	39291	PASS

m/z	Abundance
39.00	301.0
39.90	1691.0
41.00	187.0
41.90	167.0
43.00	168.0
44.00	3616.0
44.90	153.0
46.80	170.0
49.00	526.0
50.90	246.0
59.00	169.0
73.10	649.0
74.90	229.0
76.90	515.0
78.00	326.0
84.00	422.0
85.90	316.0
91.10	175.0
96.00	396.0
102.90	188.0
118.90	187.0
132.90	475.0
146.90	296.0
148.00	163.0
176.90	229.0
190.90	479.0
193.00	360.0
207.00	3480.0
208.00	875.0
208.90	613.0
280.90	428.0
281.90	251.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

m/z	Abundance
36.00	262.0
37.00	749.0
38.00	2500.0
39.00	11908.0
40.00	1886.0
40.90	585.0
42.00	256.0
43.00	356.0
44.00	3800.0
44.90	605.0
46.90	266.0
47.80	153.0
49.00	1640.0
50.00	40208.0
51.00	149504.0
52.00	8109.0
53.00	421.0
55.00	973.0
56.00	4410.0
57.00	10228.0
57.90	556.0
59.00	317.0
59.90	262.0
61.00	2170.0
62.00	2284.0
63.00	6682.0
64.00	833.0
65.00	3613.0
66.00	310.0
66.90	348.0
68.00	3039.0
69.00	170048.0
70.00	1037.0
73.00	2767.0
74.00	18696.0
75.00	27976.0
76.00	9759.0
77.00	197632.0
78.00	15485.0
79.00	13149.0
80.00	10663.0
81.00	14044.0
82.00	3024.0
83.00	3206.0
83.90	932.0
84.90	1965.0
86.00	4310.0
87.00	1860.0
88.00	1009.0
89.00	270.0
91.00	2854.0
92.00	3983.0
92.90	23120.0
93.90	1488.0
94.90	372.0
96.00	1374.0
96.80	421.0
97.10	387.0
98.00	18200.0
99.00	18464.0
100.00	1304.0
101.00	7370.0
102.10	481.0
102.90	2443.0
104.00	4570.0
105.00	4424.0
106.00	1248.0
107.00	54544.0
108.00	8524.0
109.00	1672.0
110.00	97944.0
111.00	16299.0
111.90	1906.0
113.00	643.0
114.90	350.0
115.90	2899.0
117.00	55304.0
118.00	4691.0
119.00	731.0
120.00	752.0
121.00	295.0
121.90	3476.0
123.00	5572.0
124.00	2905.0
125.00	2257.0
126.00	681.0
127.00	189888.0
128.00	14390.0
129.00	72552.0
130.00	6300.0
130.90	1339.0
132.00	736.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

132.90	507.0
134.00	2421.0
135.00	5777.0
136.00	2467.0
137.00	4674.0
137.90	910.0
138.90	472.0
139.90	980.0
140.90	8641.0
141.90	3386.0
143.00	2342.0
144.00	652.0
145.00	560.0
145.90	1814.0
147.00	5284.0
147.90	12800.0
148.90	3315.0
149.90	846.0
151.00	1235.0
151.70	658.0
153.00	3013.0
154.00	2419.0
155.00	5227.0
156.00	6882.0
157.00	1446.0
157.90	1464.0
158.90	1162.0
159.90	2643.0
161.00	4267.0
161.90	1405.0
162.90	432.0
163.90	507.0
165.00	3130.0
166.00	2727.0
167.00	20512.0
168.00	20576.0
168.90	2361.0
169.90	701.0
170.90	794.0
171.90	1391.0
173.00	2258.0
174.00	3972.0
175.00	6858.0
176.10	2084.0
177.00	3539.0
178.00	1167.0
179.00	13458.0
180.00	10685.0
181.00	4755.0
182.00	709.0
182.80	350.0
184.00	1009.0
185.00	6207.0
186.00	47104.0
187.00	14122.0
188.00	2011.0
189.00	3034.0
189.90	783.0
191.00	2092.0
191.90	4356.0
193.00	5408.0
194.00	990.0
194.90	626.0
196.00	9084.0
196.70	1667.0
197.90	337280.0
199.00	23320.0
200.00	2115.0
201.50	1389.0
203.00	2019.0
204.00	11585.0
205.00	20904.0
206.00	86128.0
207.00	16027.0
208.00	4041.0
209.00	1913.0
210.10	1499.0
210.90	3791.0
212.80	275.0
215.00	1132.0
216.00	2095.0
217.00	23616.0
218.00	3341.0
218.90	358.0
219.10	355.0
221.00	12987.0
221.80	3494.0
223.00	5192.0
224.00	48184.0
225.00	12505.0
226.00	1768.0
227.00	20448.0
228.00	3185.0
229.00	4346.0
230.00	489.0
231.00	1674.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

232.00	305.0
232.80	321.0
234.00	1312.0
234.90	1405.0
235.90	1093.0
236.90	2945.0
237.90	509.0
239.00	824.0
239.90	835.0
241.00	1157.0
242.00	2427.0
243.00	2616.0
244.00	37104.0
245.00	4851.0
246.00	7034.0
246.90	1573.0
247.90	293.0
248.90	1312.0
249.80	268.0
250.90	360.0
252.00	410.0
252.90	755.0
254.00	1172.0
255.00	172992.0
256.00	28472.0
257.00	2896.0
258.00	10431.0
259.00	1602.0
259.90	208.0
261.00	340.0
264.00	203.0
265.00	3929.0
266.00	659.0
266.90	240.0
269.90	193.0
270.90	650.0
271.80	407.0
272.10	400.0
272.90	4796.0
274.00	13490.0
275.00	78280.0
276.00	9737.0
277.00	6977.0
278.00	1538.0
279.00	325.0
281.00	939.0
281.90	429.0
283.00	852.0
284.00	452.0
285.00	1124.0
286.10	185.0
288.90	247.0
289.90	166.0
290.90	234.0
291.80	197.0
292.10	197.0
292.90	1632.0
293.90	567.0
294.90	407.0
296.00	22528.0
296.90	2920.0
298.00	253.0
300.90	226.0
301.90	341.0
303.00	2459.0
303.90	488.0
308.00	245.0
308.90	313.0
309.90	249.0
313.90	870.0
315.00	2524.0
316.00	990.0
317.00	244.0
321.00	397.0
322.00	352.0
323.00	5338.0
324.10	1209.0
326.90	1352.0
327.90	667.0
332.00	510.0
333.00	589.0
334.00	3935.0
334.90	933.0
335.90	180.0
341.00	729.0
342.00	280.0
345.90	1498.0
347.00	272.0
351.00	158.0
351.90	1786.0
353.00	1206.0
354.00	1757.0
355.00	477.0
356.00	151.0
358.90	196.0
364.90	7285.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

366.00	1284.0
369.90	221.0
371.00	434.0
372.00	3355.0
372.90	651.0
383.00	768.0
383.90	319.0
390.00	497.0
390.90	233.0
401.10	161.0
401.90	987.0
402.90	1831.0
404.00	886.0
404.80	276.0
421.00	1198.0
422.00	1233.0
423.00	8758.0
424.00	4143.0
424.90	485.0
441.00	23192.0
442.00	133120.0
443.00	25368.0
444.00	2834.0
445.00	179.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

m/z	Abundance
35.90	278.0
37.00	977.0
38.00	2212.0
39.00	13646.0
40.00	2058.0
41.00	718.0
41.90	162.0
42.90	308.0
44.00	3873.0
44.90	534.0
47.00	172.0
49.00	1775.0
50.00	46280.0
51.00	171648.0
52.00	9511.0
53.00	373.0
54.90	980.0
55.90	5090.0
57.00	11272.0
57.90	572.0
59.00	289.0
59.90	270.0
61.00	2517.0
62.00	3110.0
63.00	7458.0
64.00	1027.0
65.00	3399.0
66.00	291.0
66.90	305.0
68.00	3310.0
69.00	197824.0
70.00	1128.0
70.90	154.0
71.90	201.0
73.00	3173.0
74.00	21952.0
75.00	32840.0
76.00	11360.0
77.00	234816.0
78.00	16760.0
79.00	15041.0
80.00	11149.0
81.00	15646.0
82.00	3808.0
83.00	3904.0
84.00	952.0
85.00	2359.0
86.00	5332.0
87.00	2310.0
88.00	938.0
89.00	496.0
91.00	3330.0
92.00	4401.0
93.00	28504.0
94.00	1709.0
94.90	442.0
96.00	1497.0
97.00	509.0
98.00	21192.0
99.00	20104.0
100.00	1353.0
101.00	8403.0
102.00	575.0
102.90	2627.0
104.00	5701.0
105.00	5810.0
106.00	1732.0
107.00	67992.0
108.00	10345.0
109.00	2024.0
110.00	120880.0
111.00	19152.0
112.00	2277.0
112.90	879.0
114.10	199.0
114.90	418.0
116.00	3264.0
117.00	68488.0
118.00	5583.0
118.90	656.0
119.90	949.0
121.00	340.0
121.90	4855.0
123.00	7099.0
123.90	3336.0
125.00	3070.0
126.10	833.0
127.00	236736.0
128.00	17848.0
129.00	88336.0
130.00	7997.0
131.00	1399.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

131.90	948.0
132.90	854.0
133.90	2714.0
135.00	7156.0
136.00	3086.0
137.00	5226.0
137.90	1054.0
139.00	455.0
139.90	1269.0
141.00	11852.0
142.00	3809.0
142.90	2705.0
143.90	680.0
144.90	870.0
146.00	2172.0
147.00	6318.0
148.00	16632.0
149.00	4080.0
150.00	1206.0
151.00	1439.0
151.90	1036.0
153.00	4151.0
154.00	3001.0
155.00	6622.0
156.00	9718.0
157.00	1914.0
157.90	2374.0
158.90	1755.0
159.90	3567.0
160.90	5707.0
162.00	1540.0
162.90	513.0
164.00	495.0
165.00	4554.0
166.00	3597.0
167.00	26840.0
168.00	22280.0
169.00	2972.0
169.90	795.0
171.00	1085.0
172.00	2047.0
173.00	2949.0
174.00	5154.0
175.00	8913.0
176.00	2476.0
177.00	4768.0
177.90	1378.0
179.00	17800.0
180.00	14437.0
181.00	5673.0
182.00	901.0
182.90	565.0
184.00	1460.0
185.00	8537.0
186.00	63944.0
187.00	18456.0
188.00	2506.0
189.00	3960.0
190.00	751.0
191.00	2474.0
192.00	6038.0
193.00	6844.0
194.00	1403.0
195.00	879.0
196.00	14170.0
196.80	2145.0
198.00	474368.0
199.00	31000.0
200.00	2495.0
201.40	2139.0
203.00	3456.0
204.00	17336.0
205.00	29288.0
206.00	120760.0
207.00	20184.0
208.00	4846.0
208.90	2282.0
210.10	2169.0
210.90	4955.0
213.00	321.0
215.00	1260.0
216.00	2685.0
217.00	31088.0
218.00	4445.0
219.00	384.0
221.00	20176.0
221.80	4321.0
223.00	7464.0
224.00	66624.0
225.00	16928.0
226.00	2163.0
227.00	27648.0
228.00	3801.0
229.00	6093.0
229.90	868.0
231.00	2181.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

231.90	345.0
233.00	473.0
234.00	1498.0
235.00	2284.0
236.00	1367.0
237.00	3114.0
238.00	633.0
239.00	961.0
239.90	837.0
241.00	1381.0
241.90	3160.0
243.00	4302.0
244.00	55880.0
245.00	7273.0
246.00	9705.0
247.00	2066.0
247.90	523.0
249.00	2006.0
249.90	367.0
251.00	535.0
251.90	404.0
253.00	1054.0
254.00	1517.0
255.00	264256.0
256.00	38904.0
257.00	3360.0
258.00	15047.0
258.90	2379.0
260.00	526.0
261.00	352.0
263.90	322.0
265.00	6195.0
265.90	899.0
267.00	267.0
269.90	187.0
271.00	769.0
272.00	661.0
273.00	8191.0
274.00	18336.0
275.00	103040.0
276.00	15095.0
277.00	9610.0
278.00	1727.0
278.90	443.0
281.00	1206.0
281.90	456.0
283.00	1040.0
284.00	809.0
285.00	1624.0
285.90	344.0
288.90	318.0
290.00	435.0
291.10	241.0
292.00	516.0
293.00	2635.0
293.90	828.0
295.00	692.0
296.00	33000.0
297.00	4287.0
297.90	453.0
300.90	468.0
302.00	710.0
303.00	4112.0
303.90	1027.0
305.10	210.0
307.90	419.0
308.90	247.0
310.10	478.0
312.90	218.0
314.00	1393.0
314.90	3335.0
315.90	1795.0
316.90	364.0
321.00	817.0
322.00	353.0
323.00	9559.0
324.00	1781.0
324.90	316.0
325.90	184.0
326.90	1894.0
328.00	1101.0
329.00	193.0
332.00	722.0
333.00	883.0
334.00	5834.0
334.90	1505.0
335.90	256.0
340.90	1293.0
342.00	390.0
345.90	2371.0
347.00	427.0
352.00	3075.0
353.00	1899.0
354.00	3022.0
355.00	720.0
363.90	166.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

364.90	14752.0
365.90	2115.0
369.90	308.0
371.10	698.0
372.00	5206.0
373.00	1024.0
377.00	157.0
382.90	1320.0
384.00	471.0
390.10	530.0
391.00	408.0
391.90	331.0
400.90	267.0
401.90	1976.0
403.00	2347.0
404.00	1133.0
405.10	358.0
421.00	2614.0
421.90	2858.0
423.00	16624.0
424.00	6208.0
425.00	1073.0
439.10	197.0
441.10	49952.0
442.10	261504.0
443.00	51960.0
444.00	4997.0
444.90	351.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

m/z	Abundance
36.00	246.0
37.00	534.0
38.00	1293.0
39.00	8542.0
39.90	1600.0
41.00	369.0
43.00	213.0
44.00	3491.0
45.10	399.0
47.90	170.0
48.90	1358.0
50.00	29624.0
51.00	109920.0
52.00	6152.0
53.00	352.0
55.00	738.0
56.00	3133.0
57.00	7117.0
57.90	330.0
58.90	253.0
59.90	243.0
61.00	1879.0
62.00	1657.0
63.00	4564.0
64.00	787.0
65.00	2544.0
66.00	216.0
66.90	284.0
68.00	2044.0
69.00	126528.0
69.90	805.0
71.00	195.0
73.00	2337.0
74.00	13246.0
75.00	21016.0
76.00	7330.0
77.00	152384.0
78.00	11083.0
78.90	10560.0
79.90	7532.0
81.00	10454.0
81.90	2752.0
83.00	2189.0
83.90	863.0
84.90	1721.0
86.00	3120.0
87.00	1560.0
87.90	647.0
88.90	289.0
91.00	2129.0
92.00	2871.0
92.90	17864.0
94.00	1213.0
95.10	411.0
95.90	1225.0
96.90	356.0
98.00	14241.0
99.00	12664.0
100.00	964.0
101.00	5823.0
101.90	239.0
102.90	2032.0
104.00	3488.0
105.00	3209.0
106.00	1225.0
107.00	42592.0
108.00	6501.0
108.90	1146.0
110.00	81376.0
111.00	12169.0
112.00	1422.0
113.00	564.0
113.90	162.0
115.00	339.0
116.00	2111.0
117.00	46880.0
118.00	3532.0
118.90	709.0
120.00	696.0
120.90	310.0
121.90	3240.0
123.00	4938.0
124.00	2332.0
125.00	1994.0
126.00	640.0
127.00	155392.0
128.00	11826.0
129.00	61176.0
130.00	5172.0
131.00	1183.0
131.90	549.0
133.00	790.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

134.00	1984.0
135.00	5233.0
136.00	1858.0
137.00	3828.0
137.90	659.0
138.90	453.0
140.00	638.0
141.00	8398.0
142.00	2559.0
143.00	1870.0
144.00	529.0
145.00	532.0
145.90	1598.0
147.00	4561.0
148.00	11514.0
148.90	2377.0
150.00	824.0
151.10	1157.0
151.70	524.0
153.00	2599.0
153.90	1739.0
154.90	4490.0
156.00	6910.0
157.00	1315.0
157.90	1399.0
158.90	1292.0
159.90	2537.0
160.90	3864.0
161.90	1180.0
162.90	425.0
163.90	444.0
165.00	3203.0
166.00	2429.0
167.00	19448.0
168.00	15091.0
169.00	2031.0
170.00	518.0
171.00	708.0
171.90	1250.0
173.00	1731.0
174.00	3825.0
175.00	6987.0
176.00	1842.0
176.90	2911.0
178.00	1027.0
178.90	12000.0
180.00	9366.0
181.00	4062.0
182.10	752.0
182.80	309.0
183.90	951.0
185.00	5811.0
186.00	48312.0
187.00	14165.0
188.00	1719.0
189.00	3208.0
189.90	620.0
190.90	1656.0
192.00	3799.0
193.00	4621.0
193.90	1012.0
195.00	459.0
196.00	9288.0
197.00	1198.0
197.90	341312.0
199.00	22912.0
199.90	1871.0
201.40	1342.0
203.00	1989.0
204.00	12206.0
205.00	20736.0
206.00	87440.0
207.00	16005.0
208.00	3701.0
209.00	1433.0
210.00	1534.0
211.00	3376.0
213.10	280.0
215.00	1000.0
216.00	2030.0
217.00	22248.0
218.00	2932.0
219.00	323.0
220.10	561.0
221.00	14574.0
223.00	5153.0
224.00	48728.0
225.00	12516.0
226.00	1579.0
227.00	20832.0
228.00	2776.0
229.00	4851.0
230.10	683.0
231.00	1477.0
232.00	452.0
233.00	425.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

233.90	1290.0
235.00	1167.0
236.00	1131.0
237.00	2450.0
237.90	422.0
239.00	728.0
240.00	816.0
241.00	1005.0
242.00	2518.0
243.00	3017.0
244.00	40768.0
245.00	5231.0
245.90	7050.0
247.00	1620.0
248.00	375.0
249.00	1675.0
249.90	316.0
251.00	363.0
251.90	262.0
252.90	871.0
255.00	204672.0
256.00	28608.0
256.90	2497.0
258.00	11536.0
259.00	1675.0
260.00	410.0
260.90	244.0
264.10	354.0
265.00	4993.0
265.90	734.0
267.00	252.0
269.80	203.0
271.00	573.0
272.10	657.0
273.00	5951.0
274.00	15900.0
275.00	90312.0
276.00	12081.0
277.00	7636.0
278.00	1545.0
278.90	337.0
281.00	1112.0
281.90	378.0
283.00	1091.0
284.00	608.0
285.00	1178.0
286.00	288.0
289.00	313.0
290.00	179.0
290.90	169.0
292.00	407.0
293.00	1800.0
294.00	541.0
295.00	562.0
296.00	26536.0
297.00	2934.0
297.90	267.0
300.80	282.0
302.10	554.0
303.00	2441.0
304.00	815.0
305.00	169.0
307.90	354.0
308.90	220.0
309.90	314.0
314.00	1045.0
314.90	2982.0
316.00	1865.0
316.90	329.0
321.00	882.0
321.80	299.0
323.00	7547.0
324.00	1661.0
325.00	174.0
325.90	276.0
326.90	1837.0
327.90	669.0
328.90	159.0
332.00	786.0
333.00	866.0
334.00	5022.0
335.00	1346.0
340.90	1101.0
342.00	298.0
346.00	1998.0
346.90	579.0
351.00	206.0
352.00	2505.0
352.90	1437.0
354.00	2738.0
355.10	817.0
358.90	215.0
365.00	11762.0
365.90	1966.0
366.90	216.0
370.10	188.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369

371.00	635.0
372.00	4634.0
373.00	1089.0
382.90	1123.0
384.00	349.0
390.00	651.0
390.90	452.0
392.00	370.0
400.90	227.0
402.00	1979.0
403.00	2773.0
404.00	1058.0
405.00	321.0
420.90	2026.0
422.00	2014.0
423.00	14725.0
424.00	5301.0
425.00	711.0
439.90	281.0
441.10	33544.0
442.00	242496.0
443.00	40544.0
444.00	4251.0
445.00	205.0

Instrument :
BNA_N
ClientSampleId :
DFTPP369