


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN090619\
 Data File : BN007544.D
 Acq On : 06 Sep 2019 16:24
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 29 12:18:45 2019

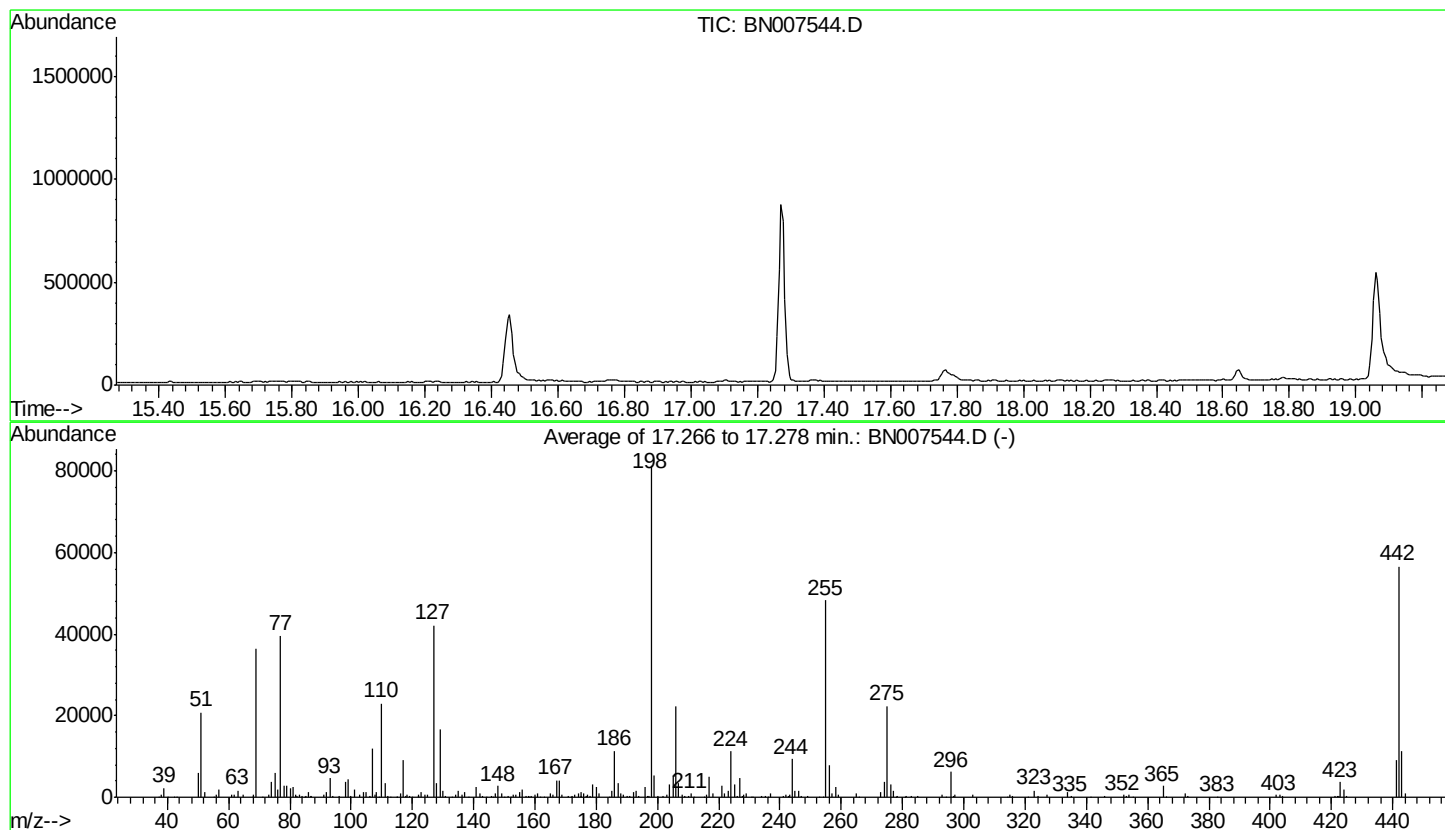

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	20730	PASS
68	69	0.00	2	1.4	521	PASS
69	198	0.00	100	45.0	36557	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	42208	PASS
197	198	0.00	2	0.4	327	PASS
198	198	100	100	100.0	81322	PASS
199	198	5	9	6.5	5309	PASS
275	198	10	60	27.4	22293	PASS
365	198	1	100	3.3	2684	PASS
441	198	0.01	100	11.1	9000	PASS
442	198	50	100	69.6	56592	PASS
443	442	15	24	20.2	11449	PASS