

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027414.D
 Acq On : 06 Sep 2023 19:31
 Operator : MA/JU
 Sample : 04148-04RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH958

Quant Time: Sep 06 23:25:26 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	6215	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	21383	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.684	164	12910	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	29066	0.400	ng/ul	0.00
17) Chrysene-d12	21.606	240	23835	0.400	ng/ul	0.00
23) Perylene-d12	24.120	264	24957	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	31625	3.825	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	10543	0.325	ng/ul	0.00
18) Fluoranthene-d10	19.450	212	31432	0.385	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	51350	6.138	ng/ul#	83
20) Pyrene	19.817	202	5570	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.956	252	10820	0.118	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027414.D
Acq On : 06 Sep 2023 19:31
Operator : MA/JU
Sample : 04148-04RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH958

Quant Time: Sep 06 23:25:26 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




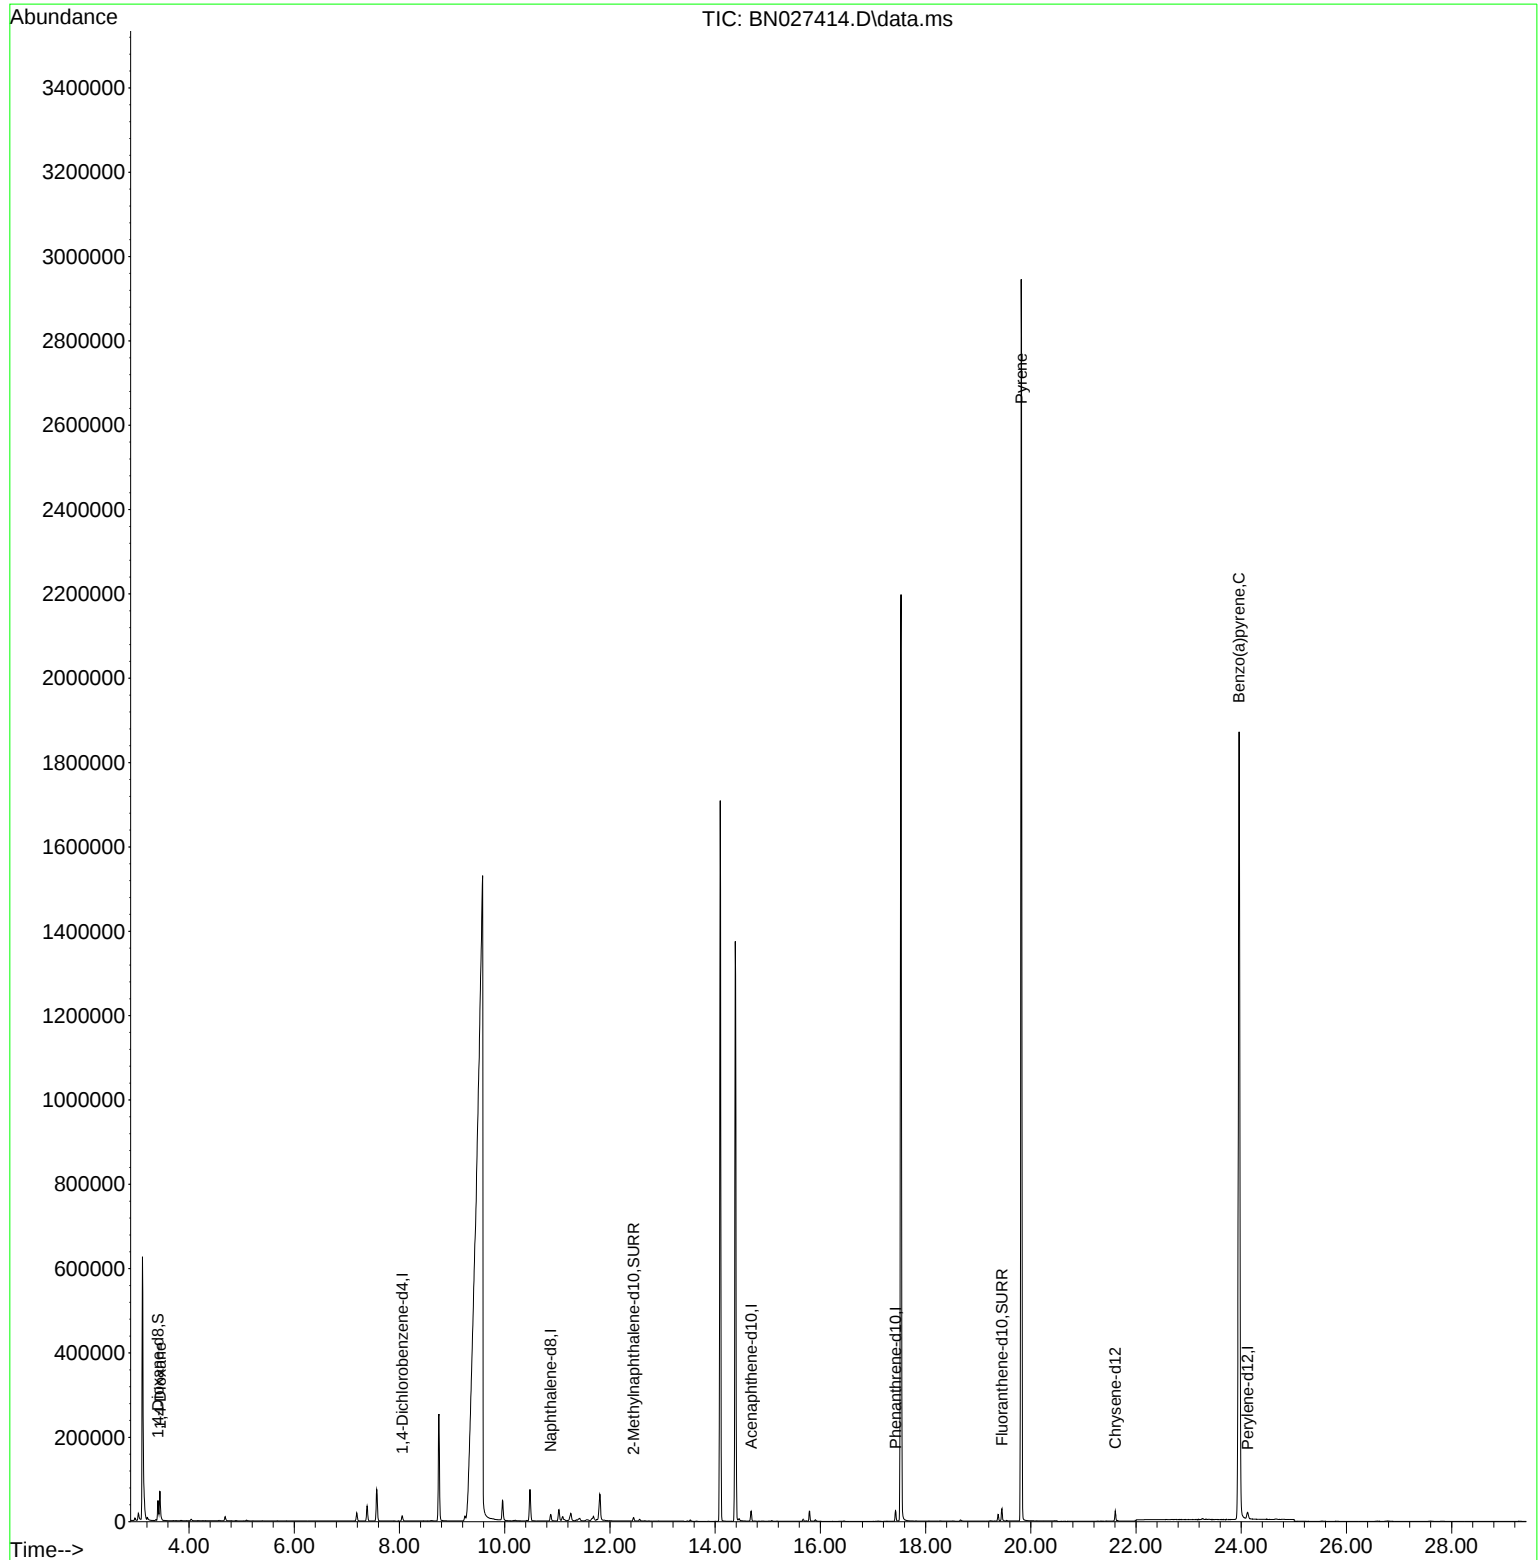


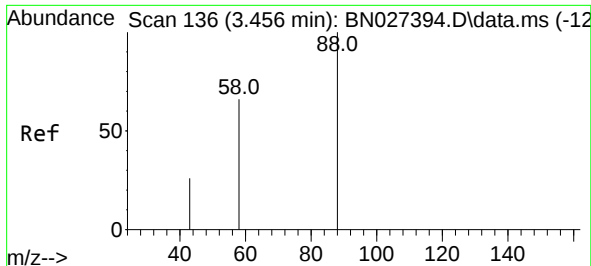

#2
1,4-Dioxane
Concen: 6.138 ng/ul
RT: 3.448 min Scan# 136
Delta R.T. -0.009 min
Lab File: BN027414.D
Acq: 06 Sep 2023 19:31




Instrument :
BNA_N
ClientSampleId :
BH958


Tgt Ion: 88 Resp: 51350
Ion Ratio Lower Upper
88 100
43 27.0 26.8 40.2
58 64.7 39.9 59.9#

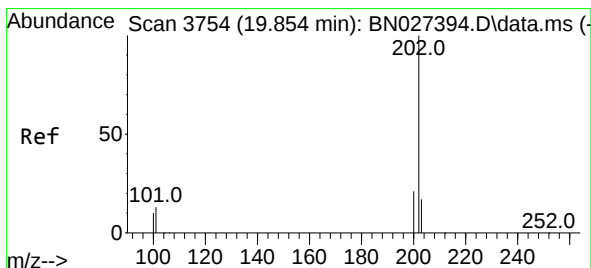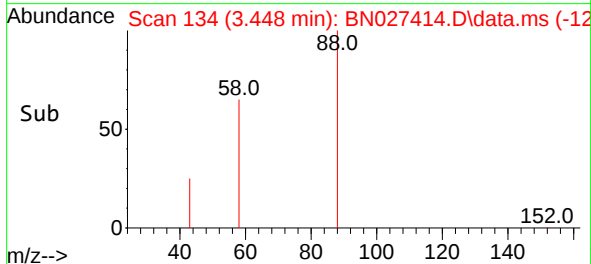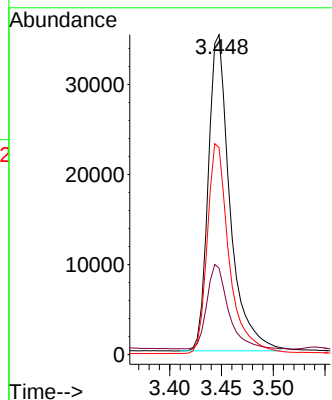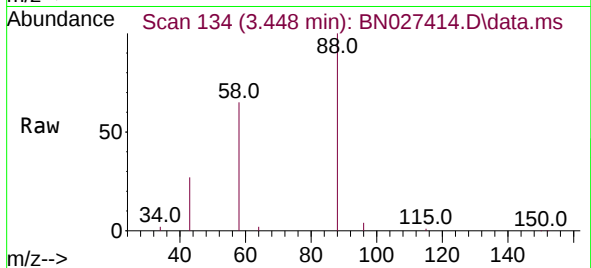

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.817 min Scan# 3746
Delta R.T. -0.032 min
Lab File: BN027414.D
Acq: 06 Sep 2023 19:31


Tgt Ion: 202 Resp: 5570
Ion Ratio Lower Upper
202 100
101 161.6 11.4 17.2#
100 1224.7 9.4 14.2#

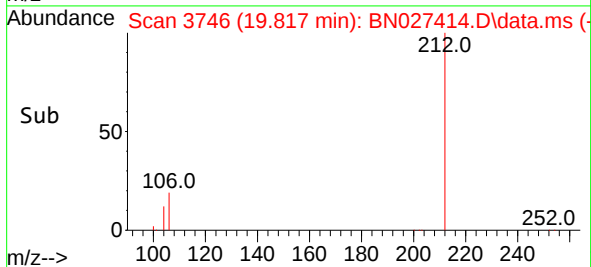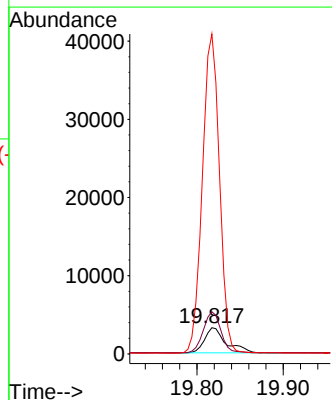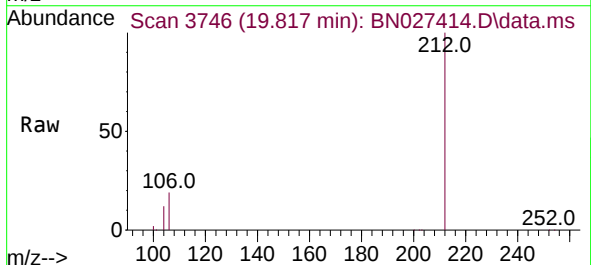

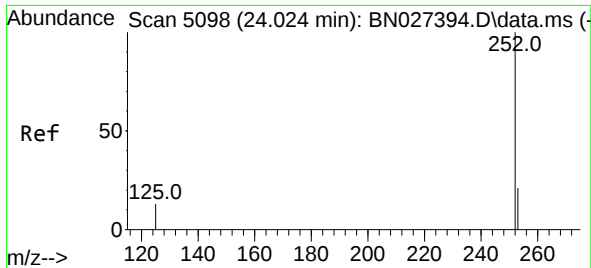

#26
 Benzo(a)pyrene
 Concen: 0.118 ng/ul
 RT: 23.956 min Scan# 50
 Delta R.T. -0.061 min
 Lab File: BN027414.D
 Acq: 06 Sep 2023 19:31

Instrument :
 BNA_N
 ClientSampleId :
 BH958

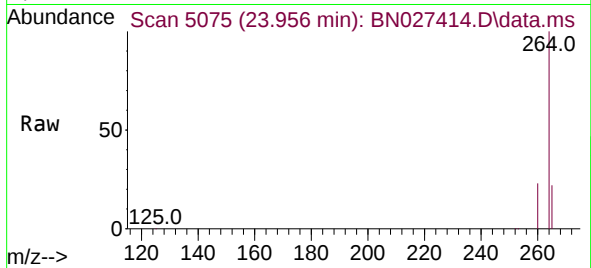

Tgt Ion:252 Resp: 10820
 Ion Ratio Lower Upper
 252 100
 253 39.9 22.4 33.6#
 125 36.8 17.4 26.2#

