

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027417.D
 Acq On : 06 Sep 2023 22:02
 Operator : MA/JU
 Sample : 04148-05RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBKF1

Quant Time: Sep 06 23:26:02 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	6106	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	22082	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	13819	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	30713	0.400	ng/ul	0.00
17) Chrysene-d12	21.603	240	25795	0.400	ng/ul	0.00
23) Perylene-d12	24.117	264	27178	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	38921	4.792	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	11833	0.353	ng/ul	-0.01
18) Fluoranthene-d10	19.446	212	36726	0.416	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	1900	0.231	ng/ul#	82
20) Pyrene	19.817	202	6103	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.957	252	12757	0.127	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027417.D
Acq On : 06 Sep 2023 22:02
Operator : MA/JU
Sample : 04148-05RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBKF1

Quant Time: Sep 06 23:26:02 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




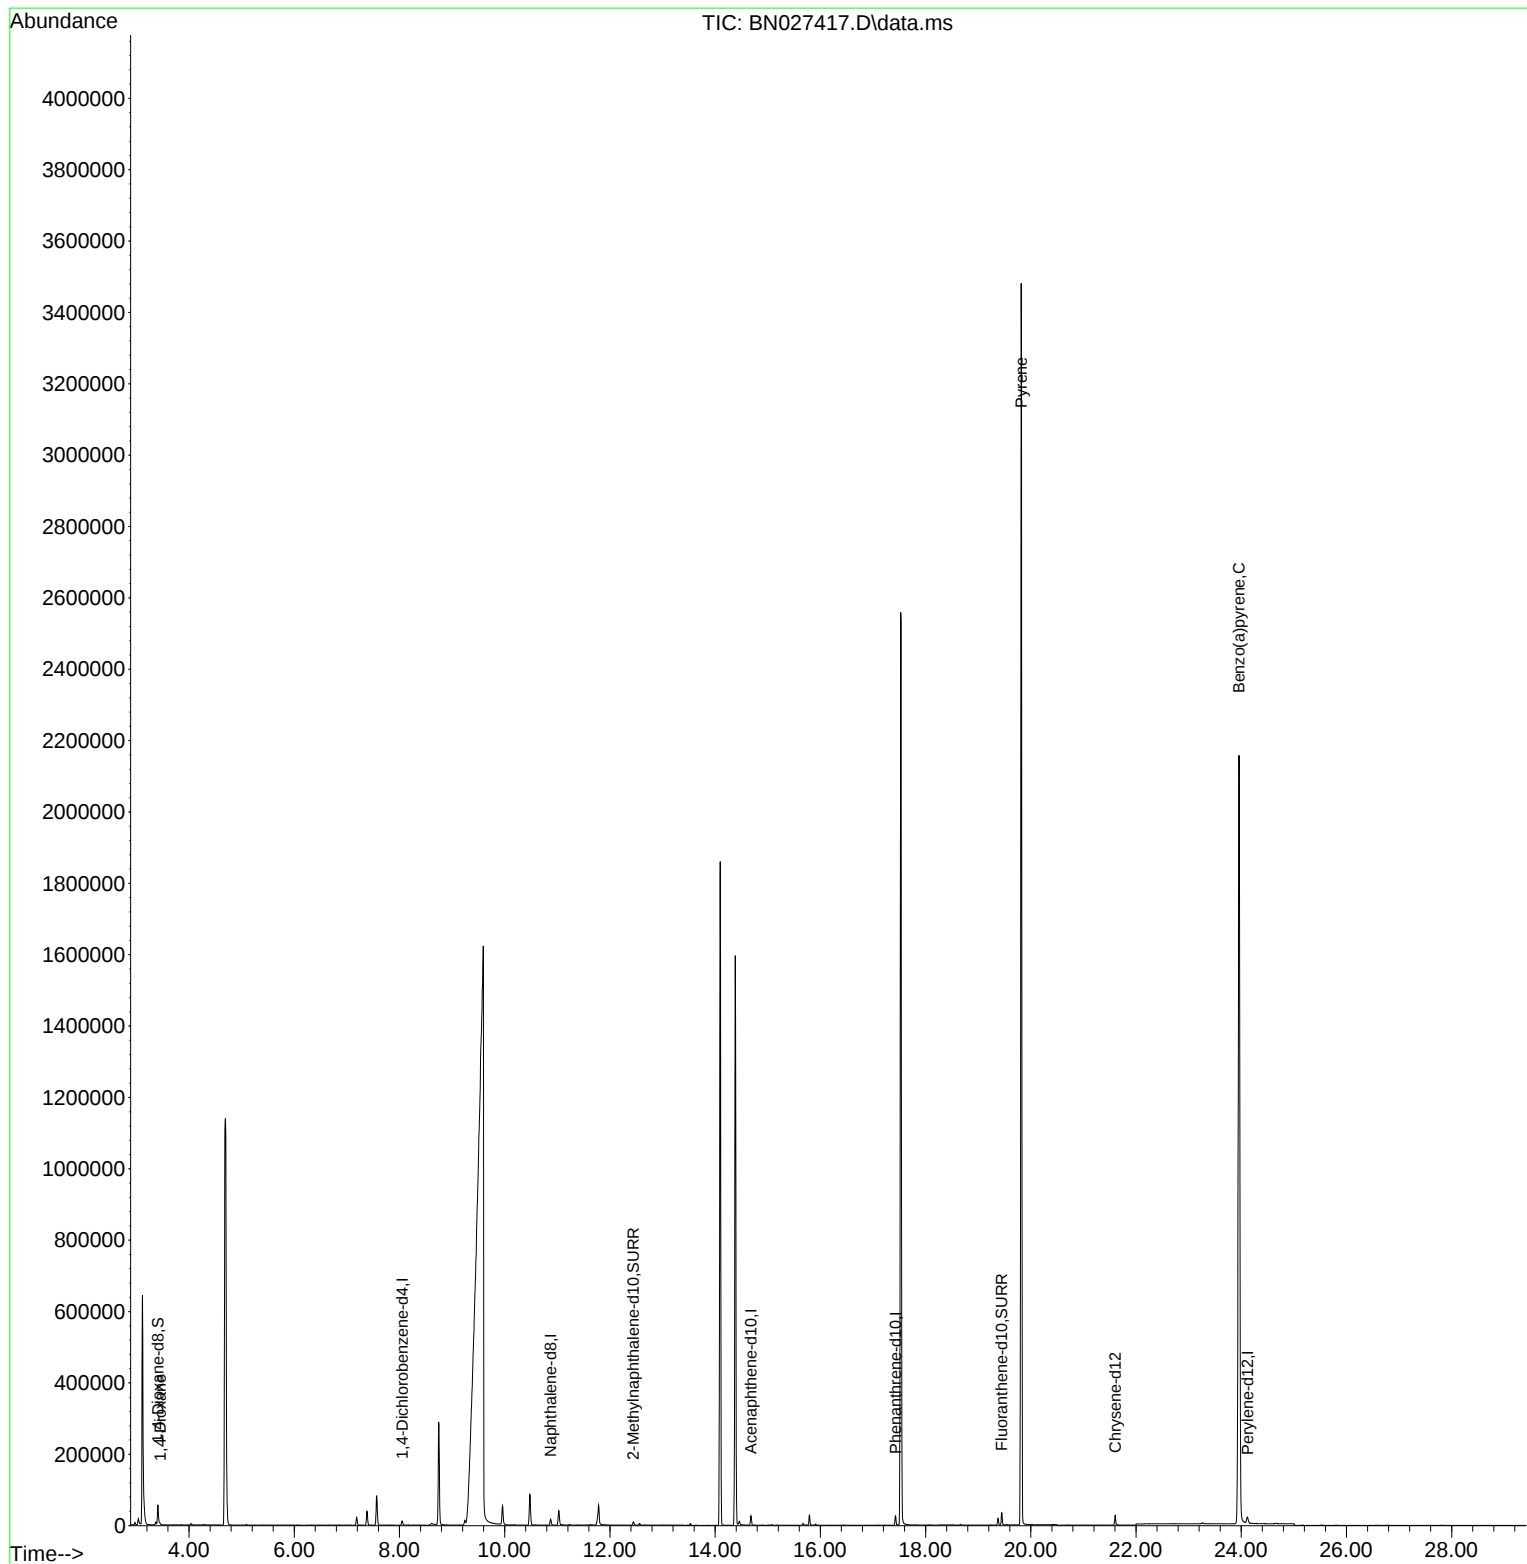


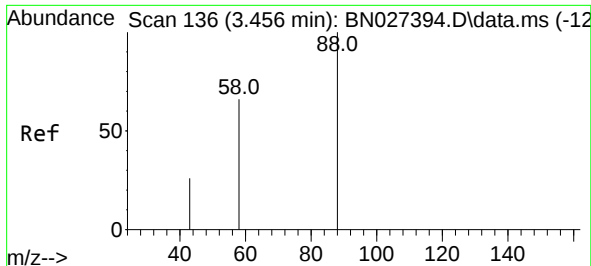

#2
1,4-Dioxane
Concen: 0.231 ng/ul
RT: 3.448 min Scan# 136
Delta R.T. -0.008 min
Lab File: BN027417.D
Acq: 06 Sep 2023 22:02




Instrument :
BNA_N
ClientSampleId :
BBKF1


Tgt Ion: 88 Resp: 1900
Ion Ratio Lower Upper
88 100
43 53.5 26.8 40.2#
58 54.3 39.9 59.9

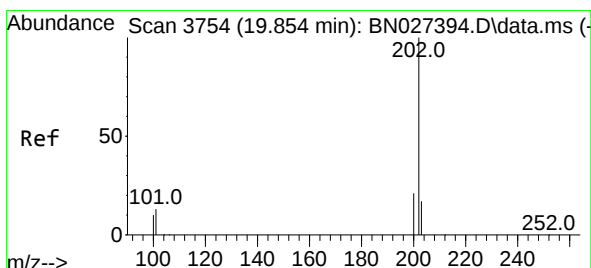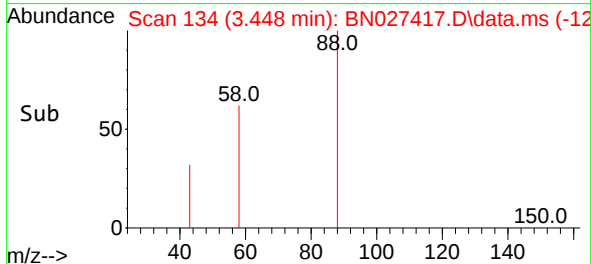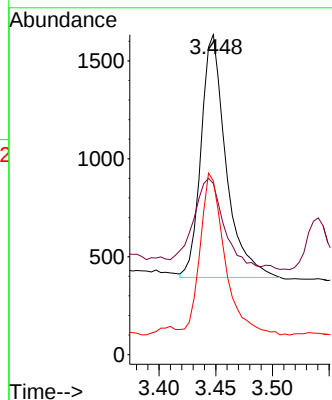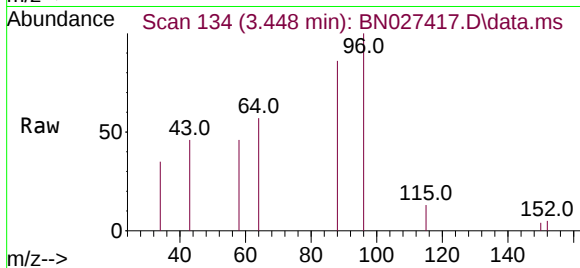

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.817 min Scan# 3746
Delta R.T. -0.032 min
Lab File: BN027417.D
Acq: 06 Sep 2023 22:02


Tgt Ion: 202 Resp: 6103
Ion Ratio Lower Upper
202 100
101 156.2 11.4 17.2#
100 1162.4 9.4 14.2#

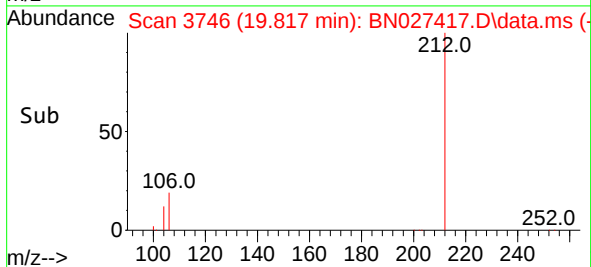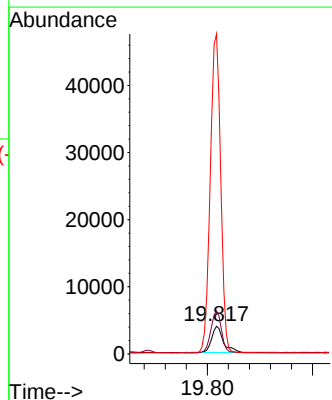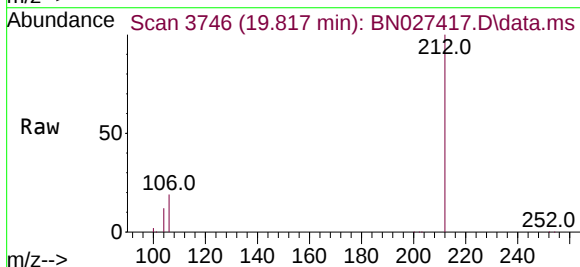

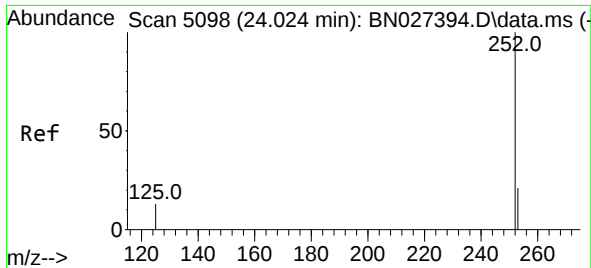

#26
Benzo(a)pyrene
Concen: 0.127 ng/ul
RT: 23.957 min Scan# 50
Delta R.T. -0.061 min
Lab File: BN027417.D
Acq: 06 Sep 2023 22:02

Instrument :
BNA_N
ClientSampleId :
BBKF1

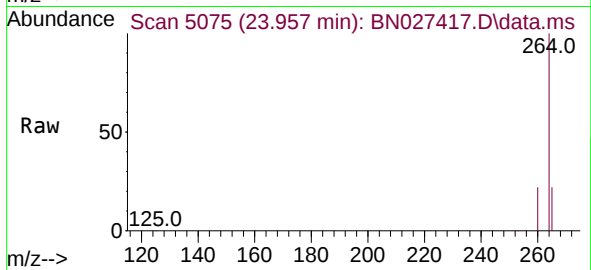

Tgt Ion:252 Resp: 12757
Ion Ratio Lower Upper
252 100
253 39.3 22.4 33.6#
125 35.8 17.4 26.2#

