

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027440.D
 Acq On : 07 Sep 2023 13:31
 Operator : MA/JU
 Sample : 04123-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH920

Quant Time: Sep 08 01:56:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	9157	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	30919	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	17792	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	37092	0.400	ng/ul	0.00
17) Chrysene-d12	21.618	240	24626	0.400	ng/ul	# 0.00
23) Perylene-d12	24.138	264	24027	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	48877	4.013	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	14137	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	33579	0.398	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	1327	0.108	ng/ul#	56
20) Pyrene	19.827	202	5497	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.974	252	7482	0.084	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027440.D
Acq On : 07 Sep 2023 13:31
Operator : MA/JU
Sample : 04123-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH920

Quant Time: Sep 08 01:56:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




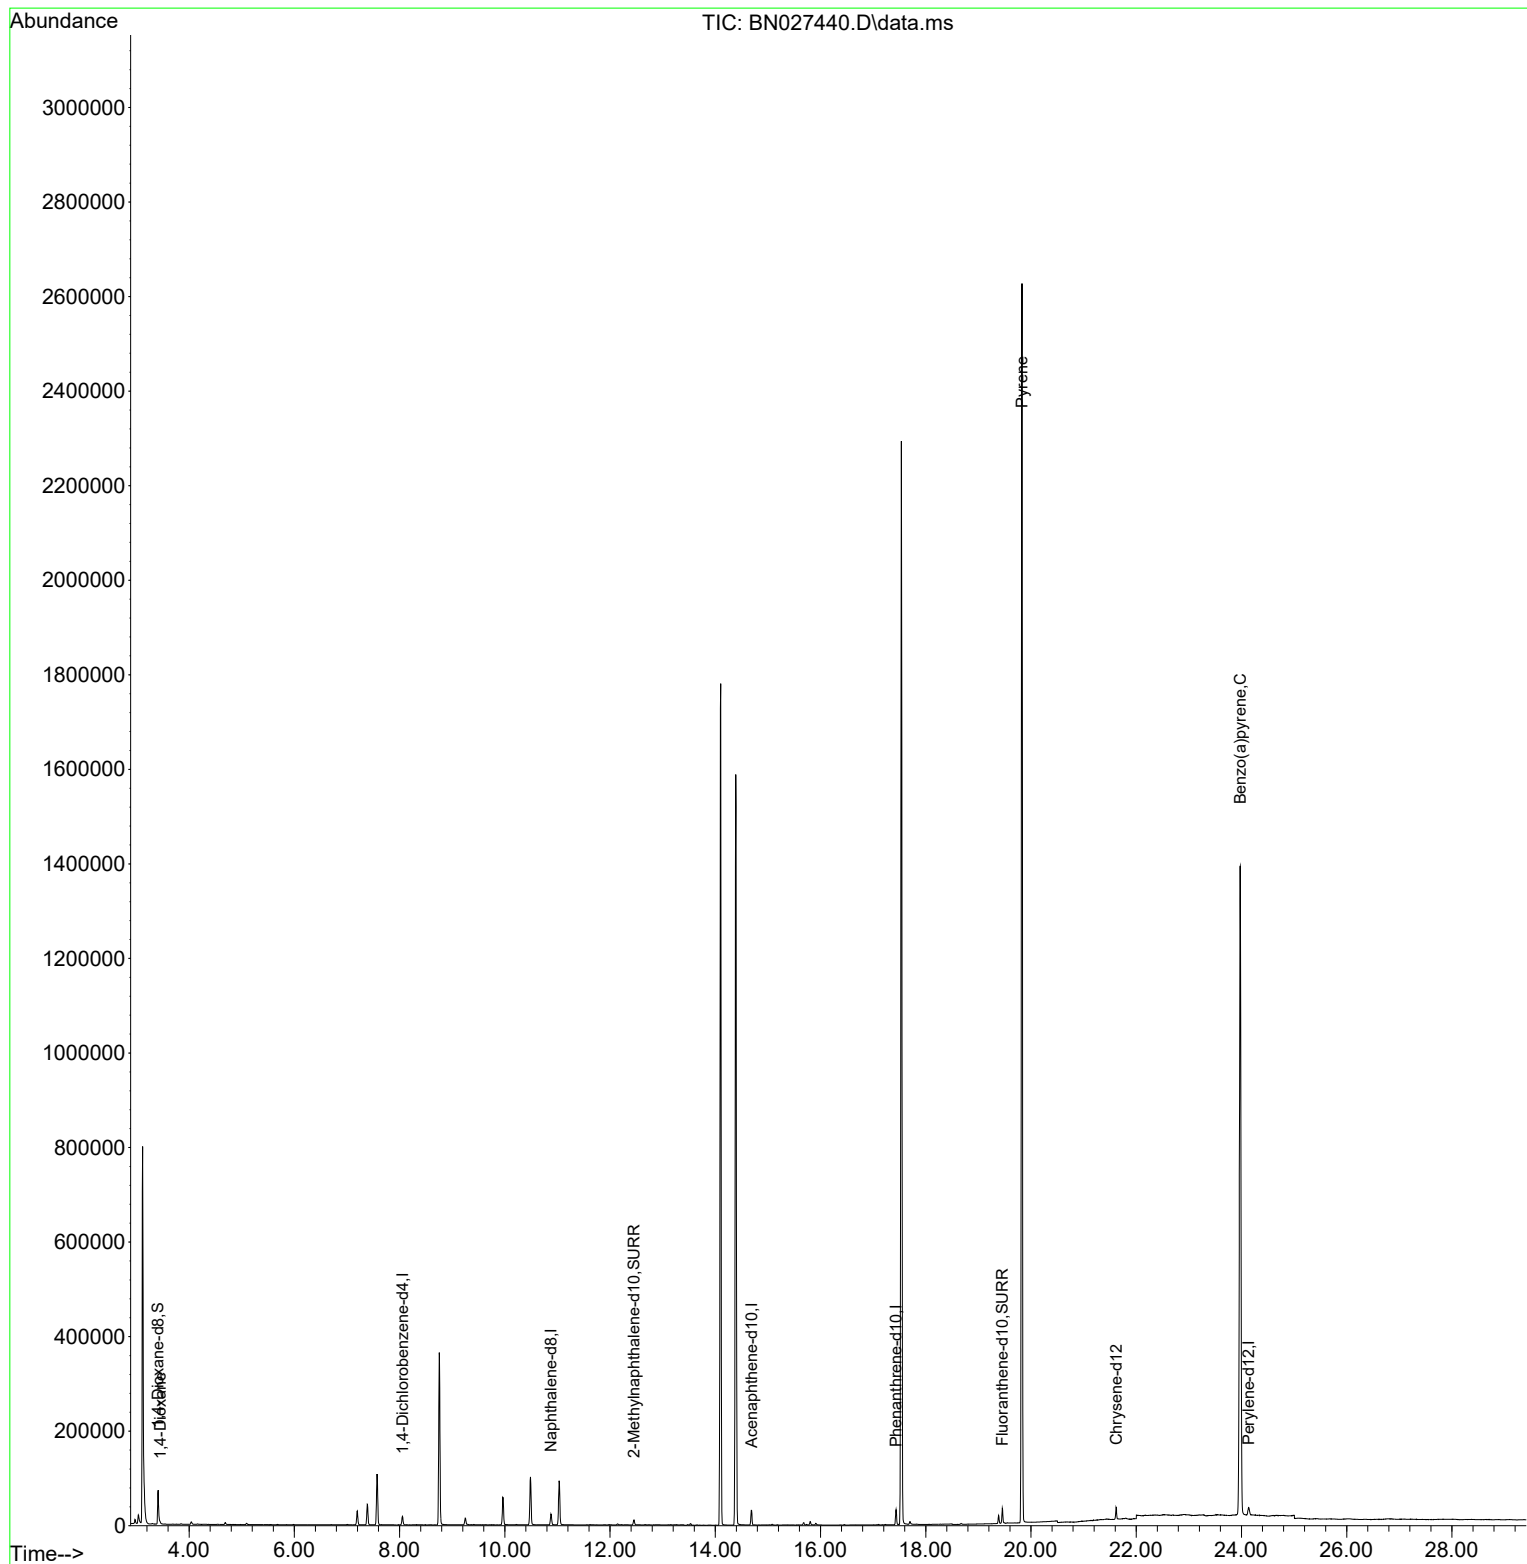


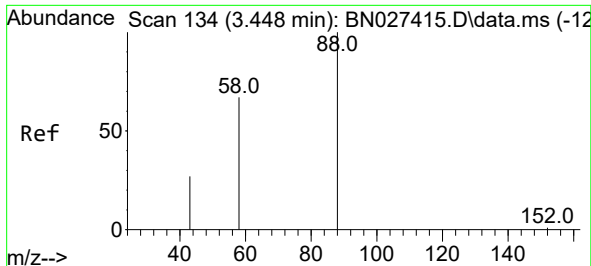

#2
1,4-Dioxane
Concen: 0.108 ng/ul
RT: 3.448 min Scan# 11
Delta R.T. -0.009 min
Lab File: BN027440.D
Acq: 07 Sep 2023 13:31




Instrument :
BNA_N
ClientSampleId :
BH920


Tgt Ion: 88 Resp: 1327
Ion Ratio Lower Upper
88 100
43 90.0 26.8 40.2#
58 54.4 39.9 59.9

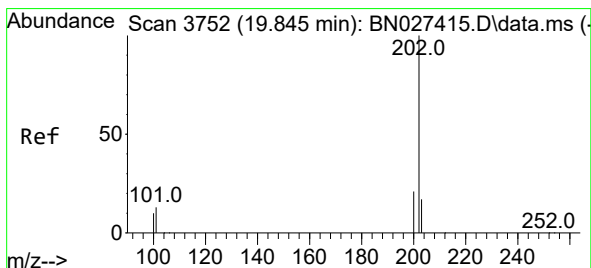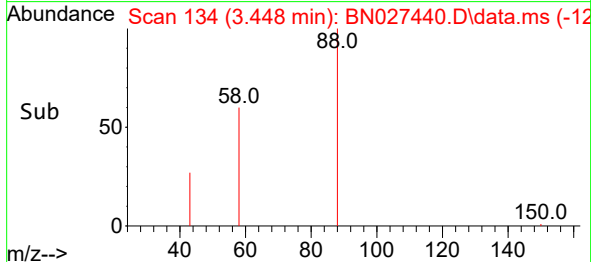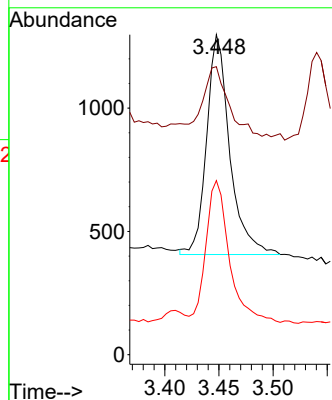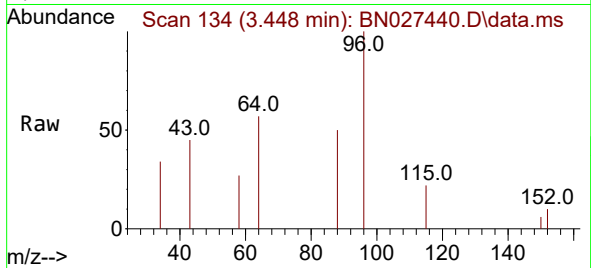

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.827 min Scan# 3748
Delta R.T. -0.023 min
Lab File: BN027440.D
Acq: 07 Sep 2023 13:31


Tgt Ion: 202 Resp: 5497
Ion Ratio Lower Upper
202 100
101 127.1 11.4 17.2#
100 892.7 9.4 14.2#

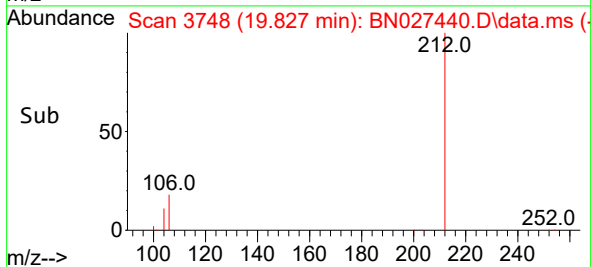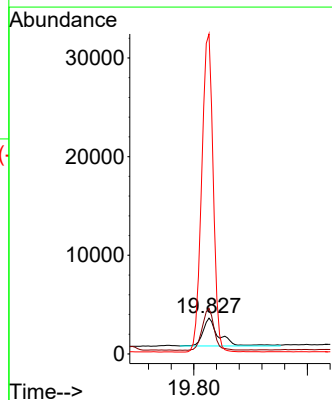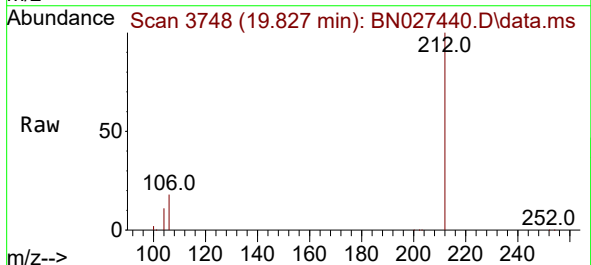

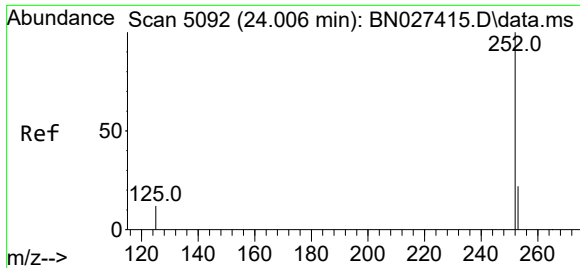

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.974 min Scan# 50
Delta R.T. -0.044 min
Lab File: BN027440.D
Acq: 07 Sep 2023 13:31

Instrument :
BNA_N
ClientSampleId :
BH920

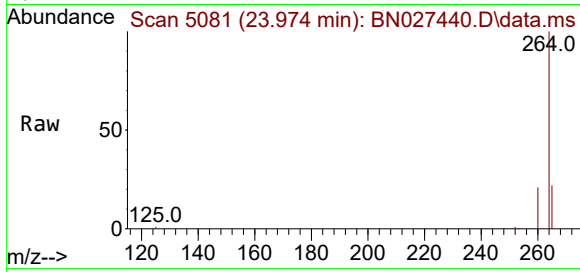

Tgt Ion:252 Resp: 7482
Ion Ratio Lower Upper
252 100
253 76.1 22.4 33.6#
125 126.6 17.4 26.2#

