

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027443.D
 Acq On : 07 Sep 2023 15:25
 Operator : MA/JU
 Sample : 04123-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9G2

Quant Time: Sep 08 01:56:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	8773	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	30217	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	17619	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	36290	0.400	ng/ul	0.00
17) Chrysene-d12	21.615	240	22706	0.400	ng/ul	0.00
23) Perylene-d12	24.129	264	22986	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	46504	3.985	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.450	152	13143	0.287	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	29871	0.384	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	1049	0.089	ng/ul#	51
20) Pyrene	19.822	202	4189	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.968	252	6141	0.072	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027443.D
Acq On : 07 Sep 2023 15:25
Operator : MA/JU
Sample : 04123-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9G2

Quant Time: Sep 08 01:56:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




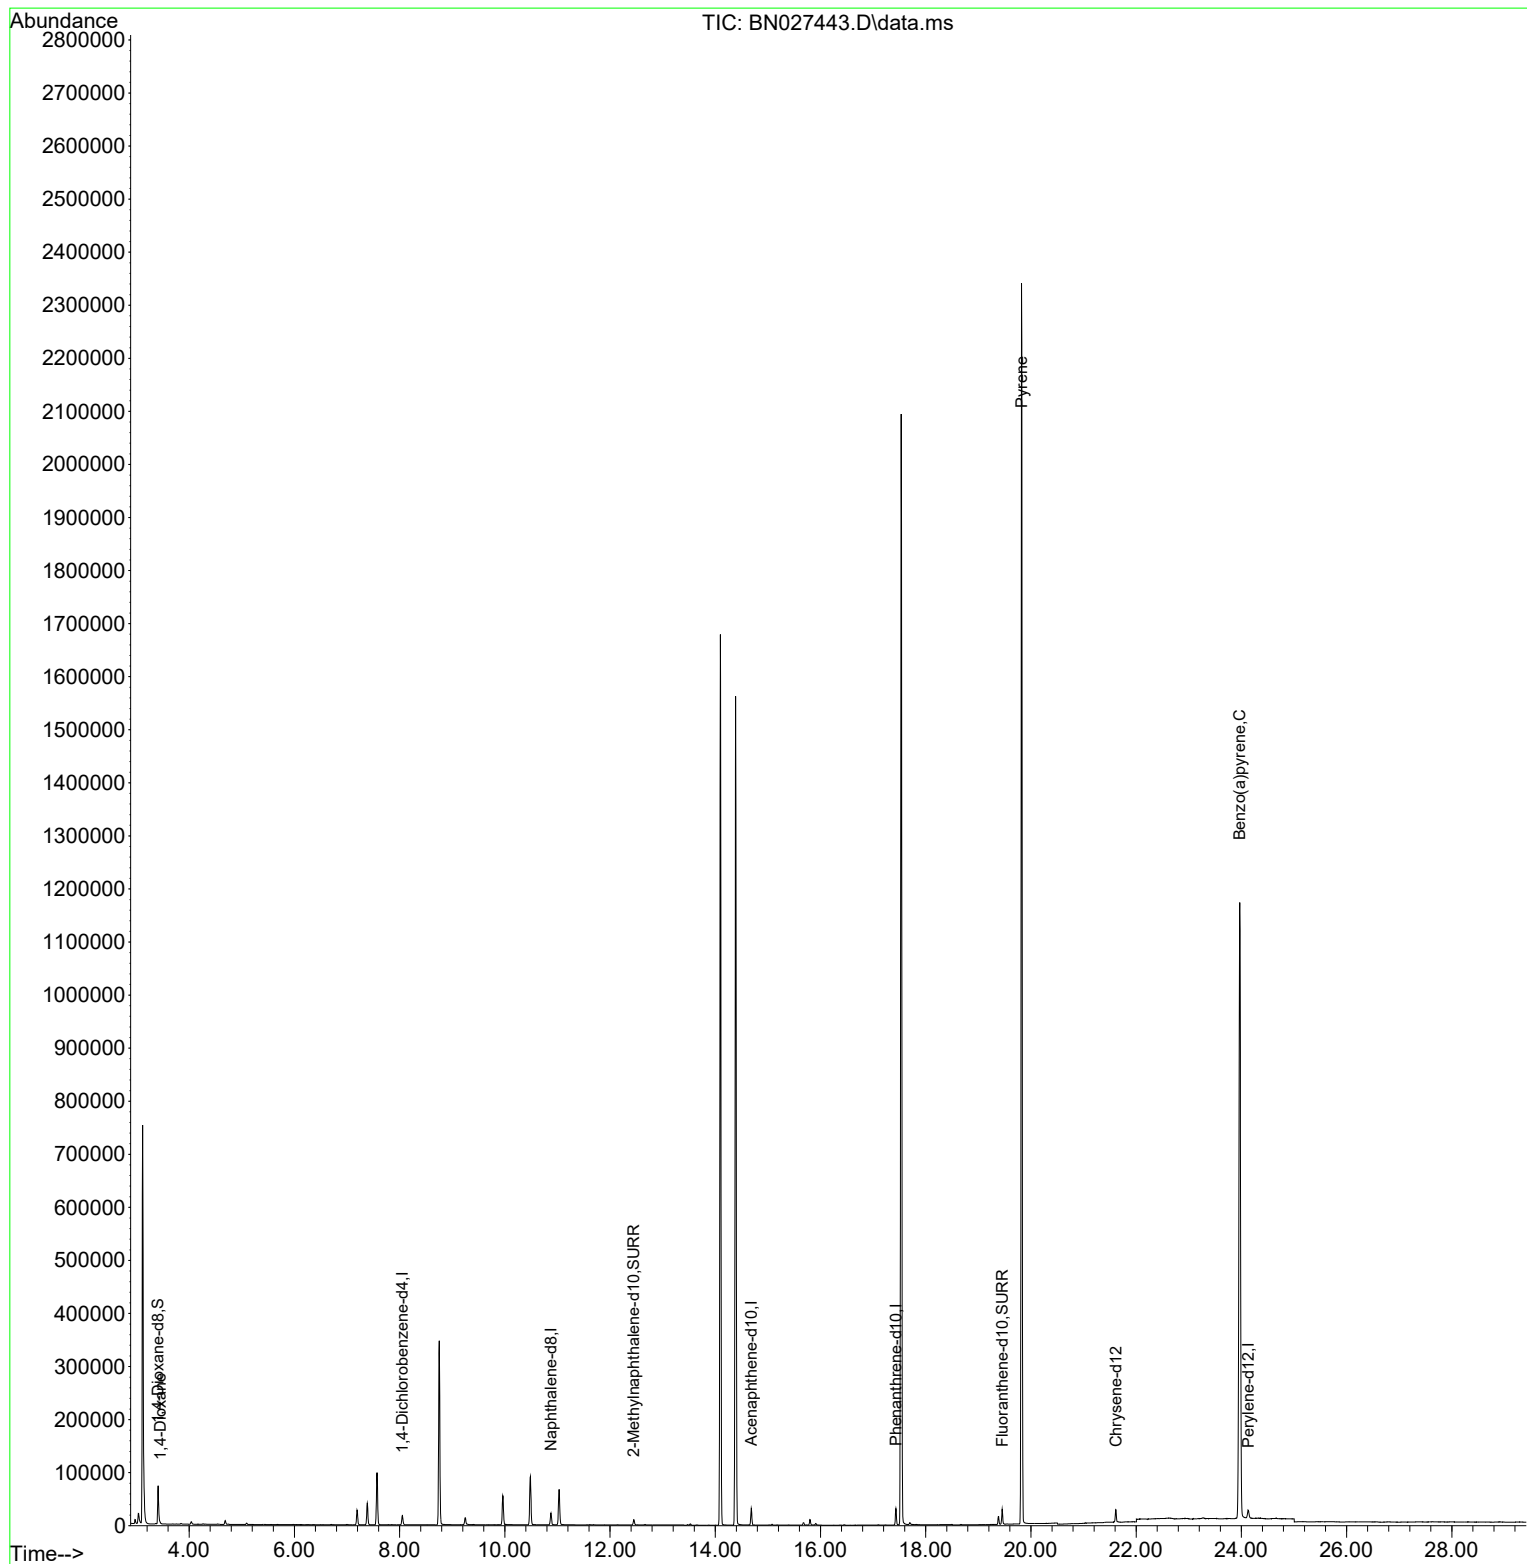


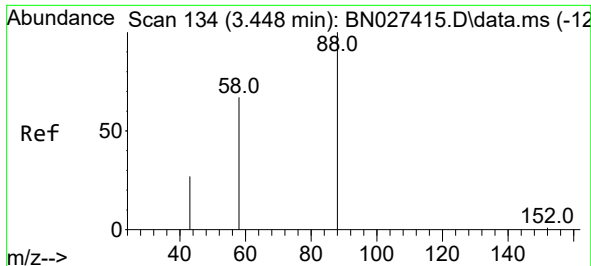

#2
1,4-Dioxane
Concen: 0.089 ng/ul
RT: 3.448 min Scan# 11
Delta R.T. -0.009 min
Lab File: BN027443.D
Acq: 07 Sep 2023 15:25




Instrument :
BNA_N
ClientSampleId :
BH9G2


Tgt Ion: 88 Resp: 1049
Ion Ratio Lower Upper
88 100
43 98.7 26.8 40.2#
58 53.7 39.9 59.9

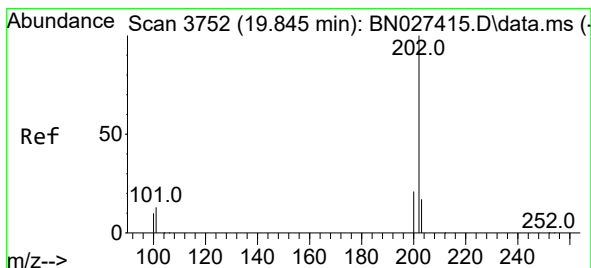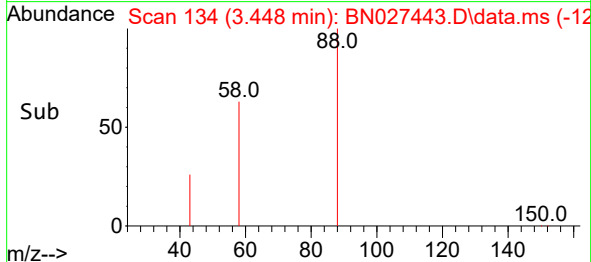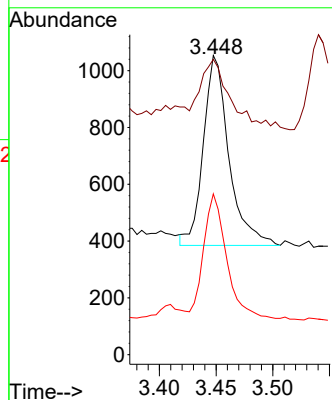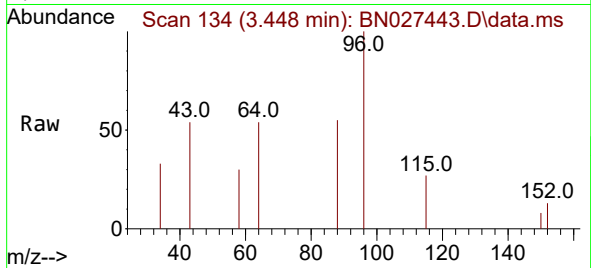

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.822 min Scan# 3747
Delta R.T. -0.028 min
Lab File: BN027443.D
Acq: 07 Sep 2023 15:25


Tgt Ion: 202 Resp: 4189
Ion Ratio Lower Upper
202 100
101 141.4 11.4 17.2#
100 1045.1 9.4 14.2#

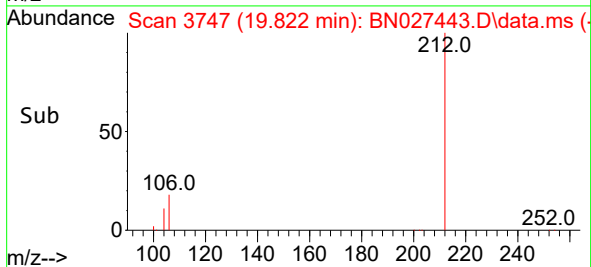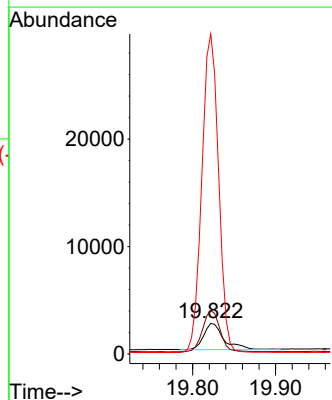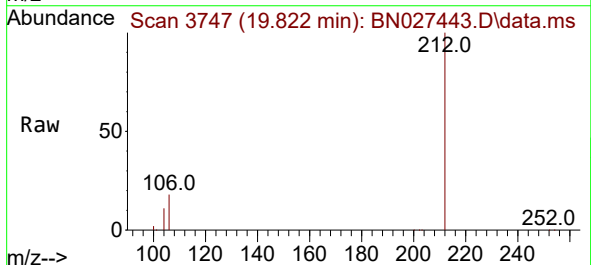

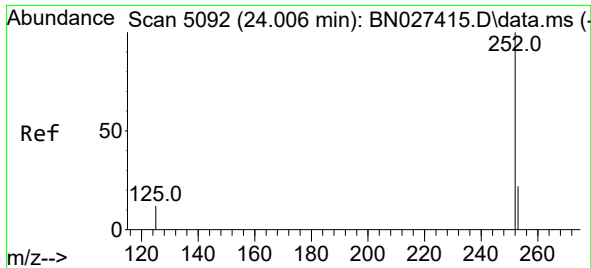

#26
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 23.968 min Scan# 5092
Delta R.T. -0.050 min
Lab File: BN027443.D
Acq: 07 Sep 2023 15:25

Instrument :
BNA_N
ClientSampleId :
BH9G2

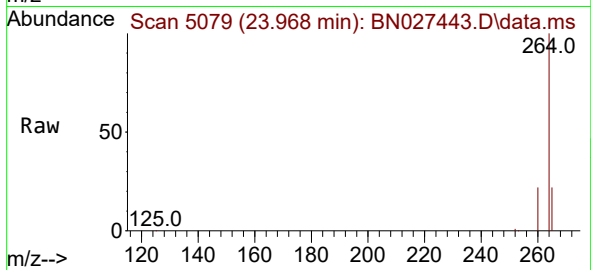

Tgt Ion:252 Resp: 6141
Ion Ratio Lower Upper
252 100
253 69.0 22.4 33.6#
125 93.8 17.4 26.2#

