

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027446.D
 Acq On : 07 Sep 2023 17:58
 Operator : MA/JU
 Sample : PB155235BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK235

Quant Time: Sep 08 01:57:17 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	7626	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	26043	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	15030	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	31161	0.400	ng/ul	0.00
17) Chrysene-d12	21.609	240	20128	0.400	ng/ul	0.00
23) Perylene-d12	24.123	264	20531	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	52571	5.182	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	14012	0.355	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	28438	0.412	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.822	202	3606	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.959	252	6036	0.080	ng/ul#	23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027446.D
Acq On : 07 Sep 2023 17:58
Operator : MA/JU
Sample : PB155235BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK235

Quant Time: Sep 08 01:57:17 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




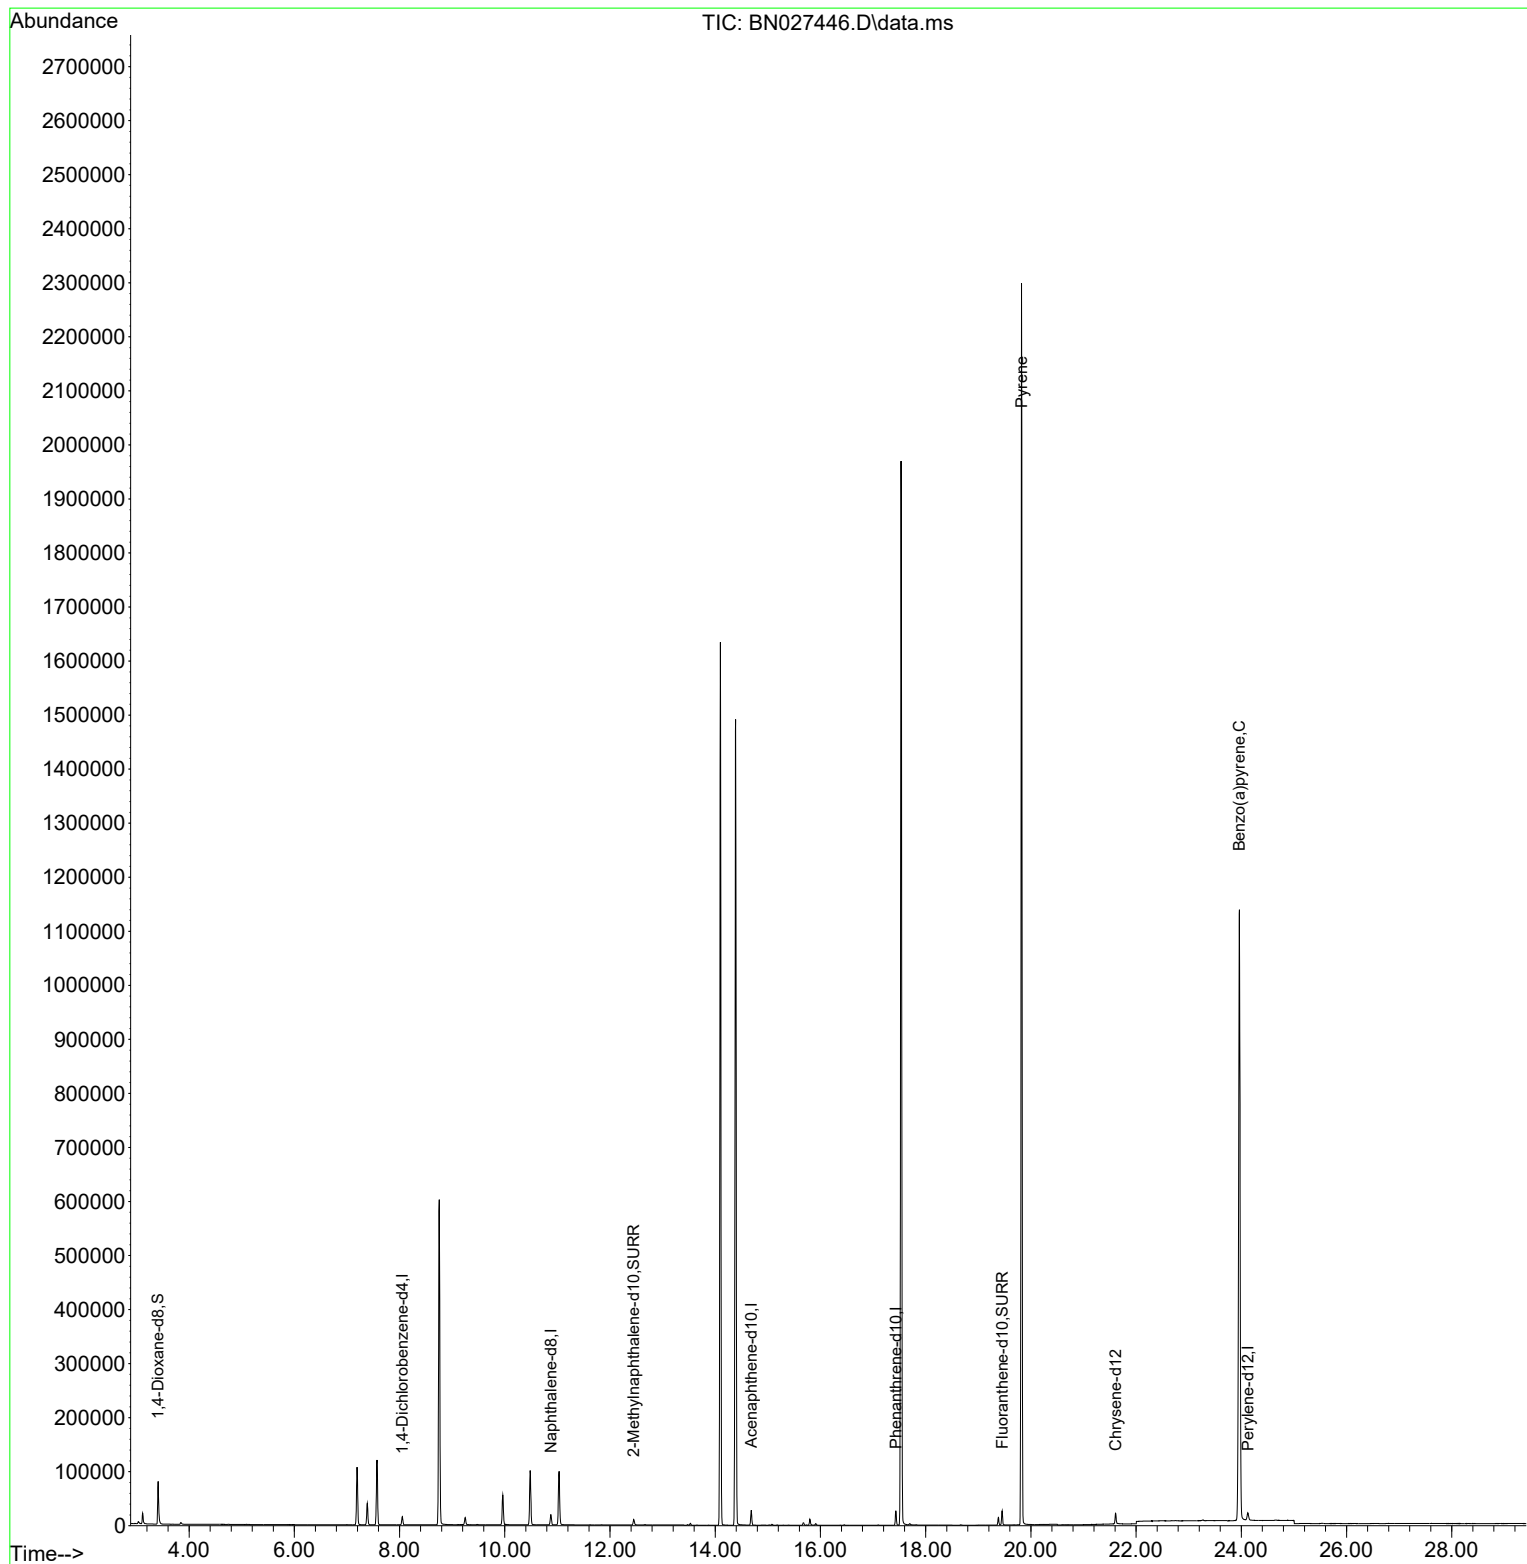


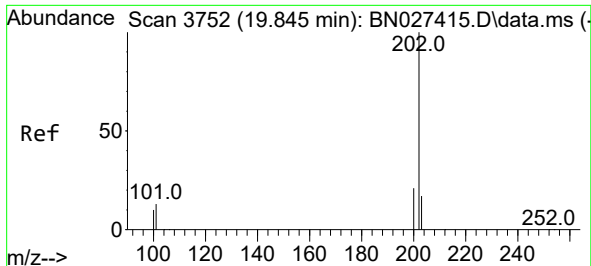

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.822 min Scan# 31
Delta R.T. -0.028 min
Lab File: BN027446.D
Acq: 07 Sep 2023 17:58

Instrument :
BNA_N
ClientSampleId :
SBLK235

Tgt Ion:202 Resp: 3606
Ion Ratio Lower Upper
202 100
101 150.0 11.4 17.2#
100 1103.3 9.4 14.2#

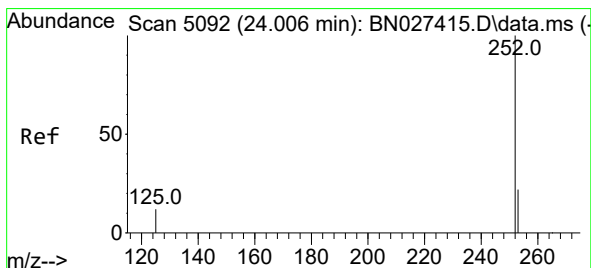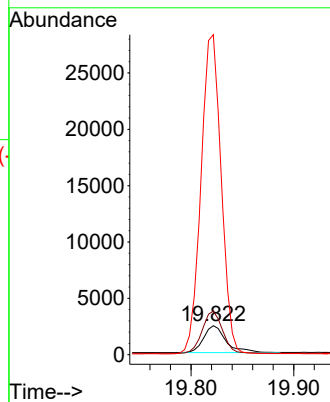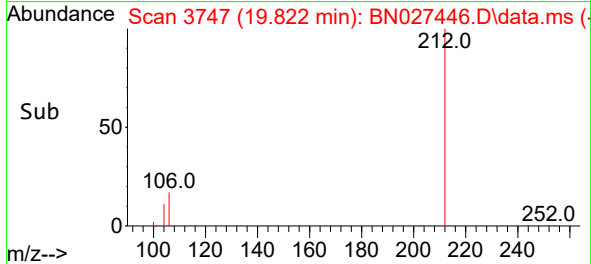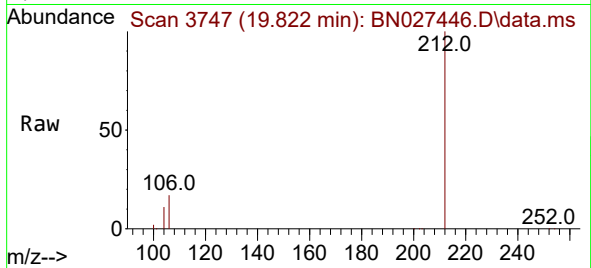

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.959 min Scan# 5076
Delta R.T. -0.058 min
Lab File: BN027446.D
Acq: 07 Sep 2023 17:58

Tgt Ion:252 Resp: 6036
Ion Ratio Lower Upper
252 100
253 60.7 22.4 33.6#
125 67.0 17.4 26.2#

