

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027447.D
 Acq On : 07 Sep 2023 18:37
 Operator : MA/JU
 Sample : PB155066BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK066

Quant Time: Sep 08 01:57:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	10153	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	34900	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.685	164	20311	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	42454	0.400	ng/ul	0.00
17) Chrysene-d12	21.609	240	28196	0.400	ng/ul	0.00
23) Perylene-d12	24.123	264	27731	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	75600	5.598	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	14799	0.279	ng/ul	0.00
18) Fluoranthene-d10	19.450	212	32708	0.339	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.822	202	4308	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.959	252	7411	0.072	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027447.D
Acq On : 07 Sep 2023 18:37
Operator : MA/JU
Sample : PB155066BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK066

Quant Time: Sep 08 01:57:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

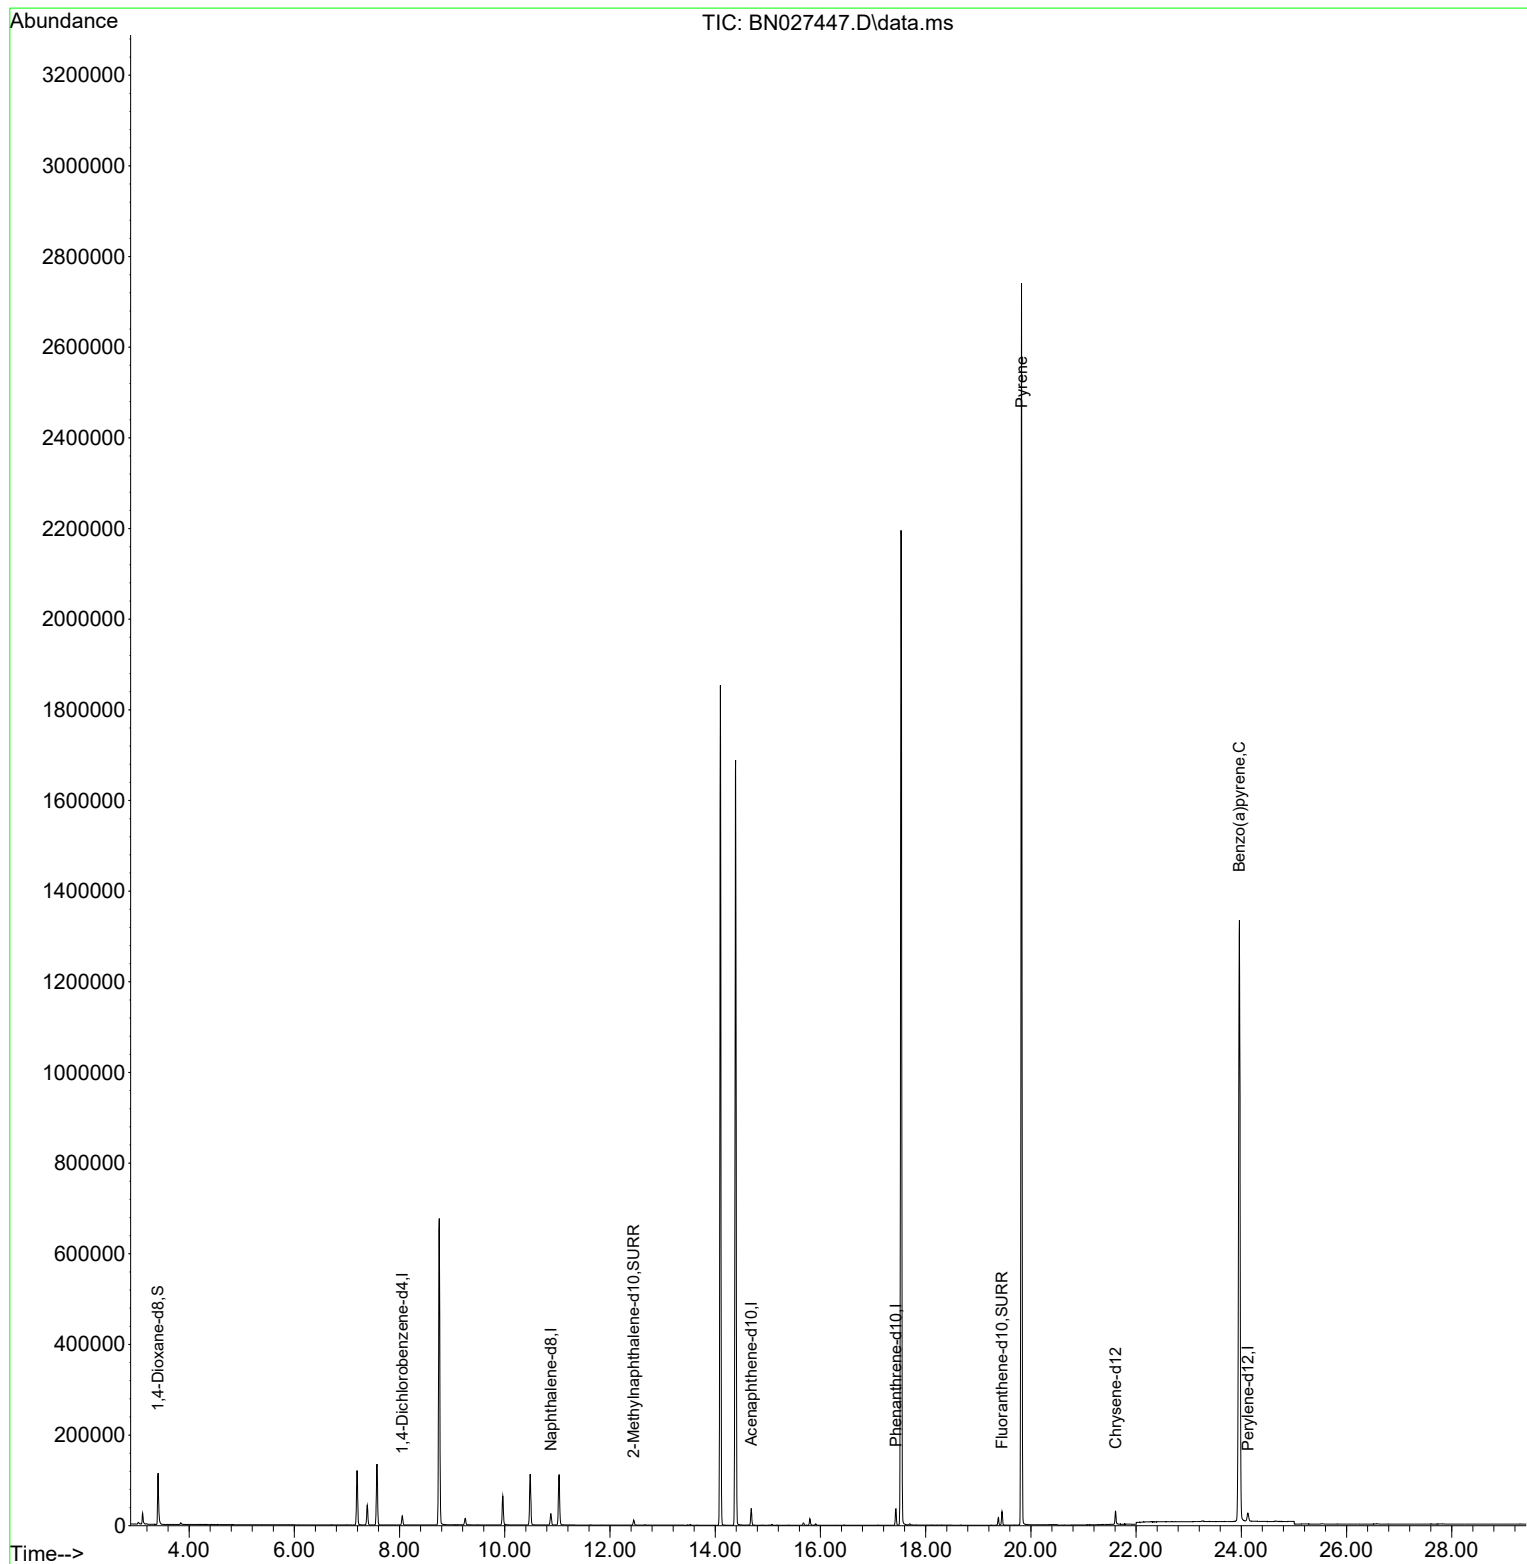

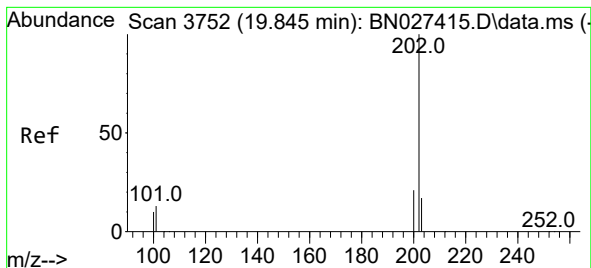

#20

Pyrene

Concen: 0.033 ng/ul

RT: 19.822 min Scan# 31

Delta R.T. -0.028 min

Lab File: BN027447.D

Acq: 07 Sep 2023 18:37

Instrument :

BNA_N

ClientSampleId :

SBLK066





Tgt Ion:202 Resp: 4308

Ion Ratio Lower Upper

202 100

101 146.2 11.4 17.2#

100 1042.1 9.4 14.2#

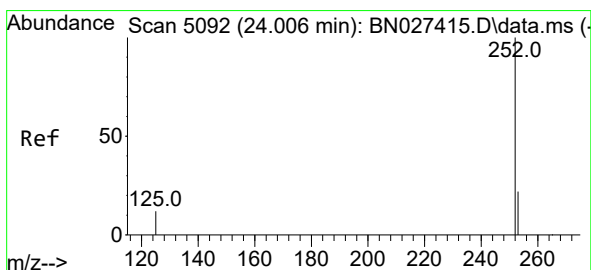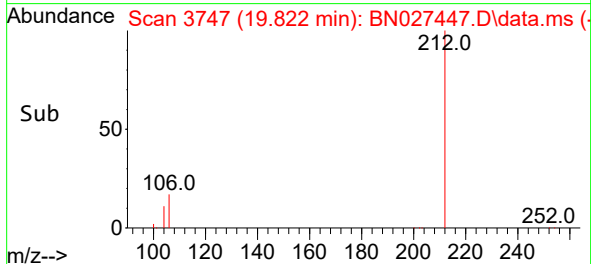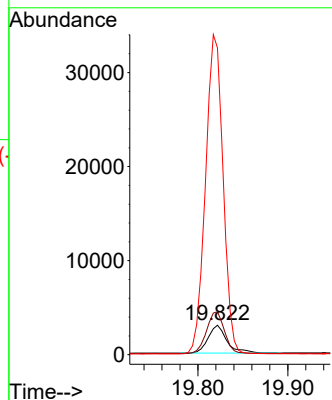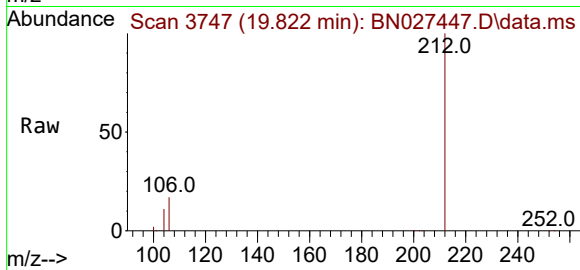

#26

Benzo(a)pyrene

Concen: 0.072 ng/ul

RT: 23.959 min Scan# 5076

Delta R.T. -0.058 min

Lab File: BN027447.D

Acq: 07 Sep 2023 18:37

Tgt Ion:252 Resp: 7411

Ion Ratio Lower Upper

252 100

253 57.0 22.4 33.6#

125 60.3 17.4 26.2#

