

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027448.D
 Acq On : 07 Sep 2023 19:15
 Operator : MA/JU
 Sample : PB155069BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK069

Quant Time: Sep 08 01:57:29 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	8056	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	27936	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	16185	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	33825	0.400	ng/ul	0.00
17) Chrysene-d12	21.606	240	22773	0.400	ng/ul	0.00
23) Perylene-d12	24.120	264	22477	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	57410	5.357	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	11299	0.266	ng/ul	0.00
18) Fluoranthene-d10	19.450	212	24603	0.315	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.822	202	3345	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.956	252	5086	0.061	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027448.D
Acq On : 07 Sep 2023 19:15
Operator : MA/JU
Sample : PB155069BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK069

Quant Time: Sep 08 01:57:29 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




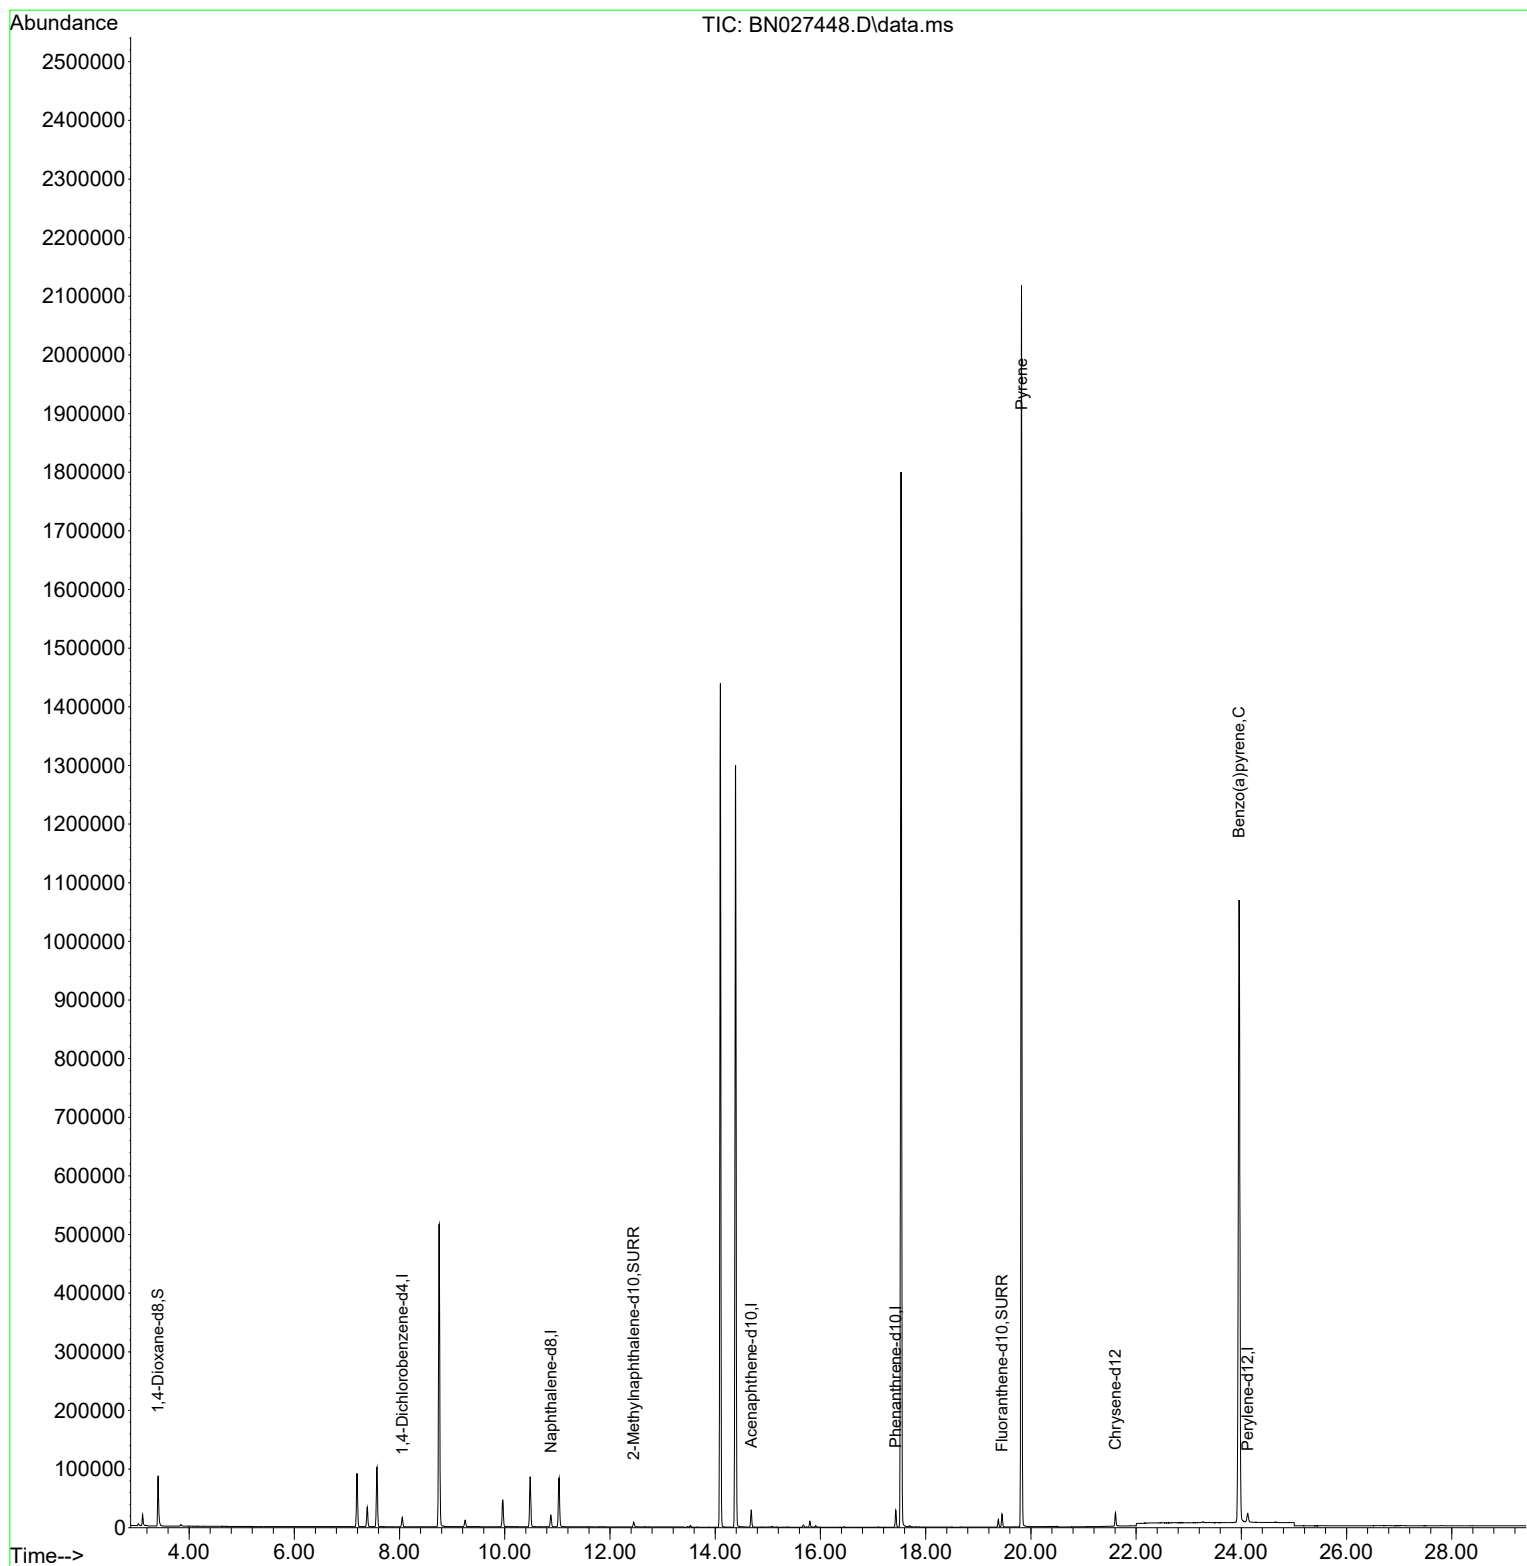


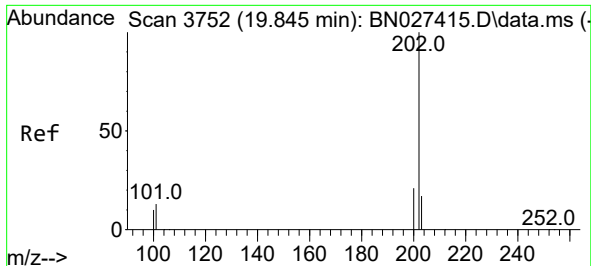

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.822 min Scan# 31
Delta R.T. -0.028 min
Lab File: BN027448.D
Acq: 07 Sep 2023 19:15

Instrument :
BNA_N
ClientSampleId :
SBLK069

Tgt Ion:202 Resp: 3345
Ion Ratio Lower Upper
202 100
101 147.5 11.4 17.2#
100 1054.4 9.4 14.2#

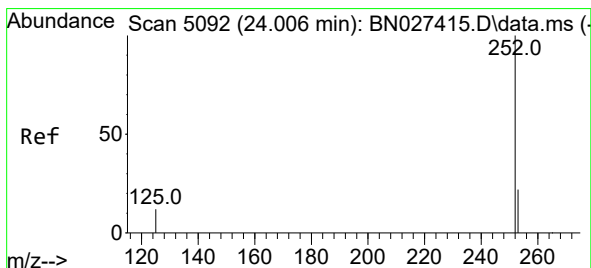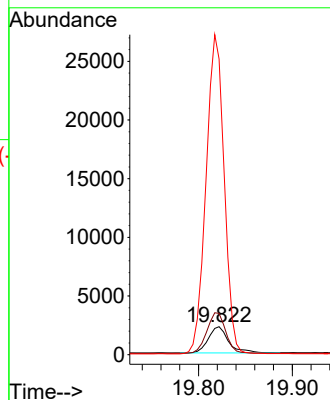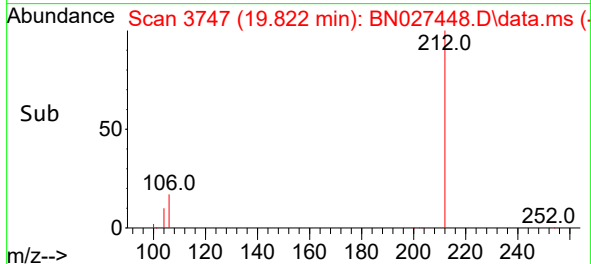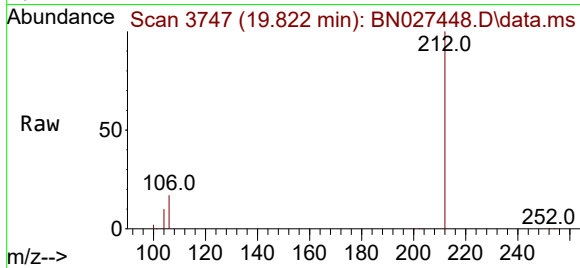

#26
Benzo(a)pyrene
Concen: 0.061 ng/ul
RT: 23.956 min Scan# 5075
Delta R.T. -0.061 min
Lab File: BN027448.D
Acq: 07 Sep 2023 19:15

Tgt Ion:252 Resp: 5086
Ion Ratio Lower Upper
252 100
253 61.1 22.4 33.6#
125 62.5 17.4 26.2#

